

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042815\
 Data File : BG016787.D
 Acq On : 29 Apr 2015 6:46
 Operator : TP/IZ
 Sample : G2004-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-25

Quant Time: Apr 29 07:53:21 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 23 19:19:11 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	85933	20.00	ng	-0.04
21) Naphthalene-d8	10.35	136	368291	20.00	ng	-0.04
38) Acenaphthene-d10	14.23	164	204309	20.00	ng	-0.02
63) Phenanthrene-d10	16.97	188	365138	20.00	ng	-0.02
75) Chrysene-d12	21.17	240	309102	20.00	ng	-0.02
86) Perylene-d12	23.36	264	296996	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	224425	42.38	ng	-0.03
7) Phenol-d6	6.77	99	189863	25.56	ng	-0.03
23) Nitrobenzene-d5	8.73	82	384798	66.02	ng	-0.04
41) 2,4,6-Tribromophenol	15.73	330	136274	89.91	ng	-0.02
44) 2-Fluorobiphenyl	12.84	172	910811	71.62	ng	-0.03
78) Terphenyl-d14	19.61	244	712965	53.13	ng	-0.02
Target Compounds						Qvalue
18) Hexachloroethane	8.67	117	6863	2.81	ng	# 1
32) Benzoic acid	9.71	122	1224	9.17	ng	# 1
53) 2,4-Dinitrophenol	14.39	184	234	7.71	ng	# 1
69) Pentachlorophenol	16.64	266	4942	3.24	ng	# 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042815\
Data File : BG016787.D
Acq On : 29 Apr 2015 6:46
Operator : TP/IZ
Sample : G2004-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-25

Quant Time: Apr 29 07:53:21 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

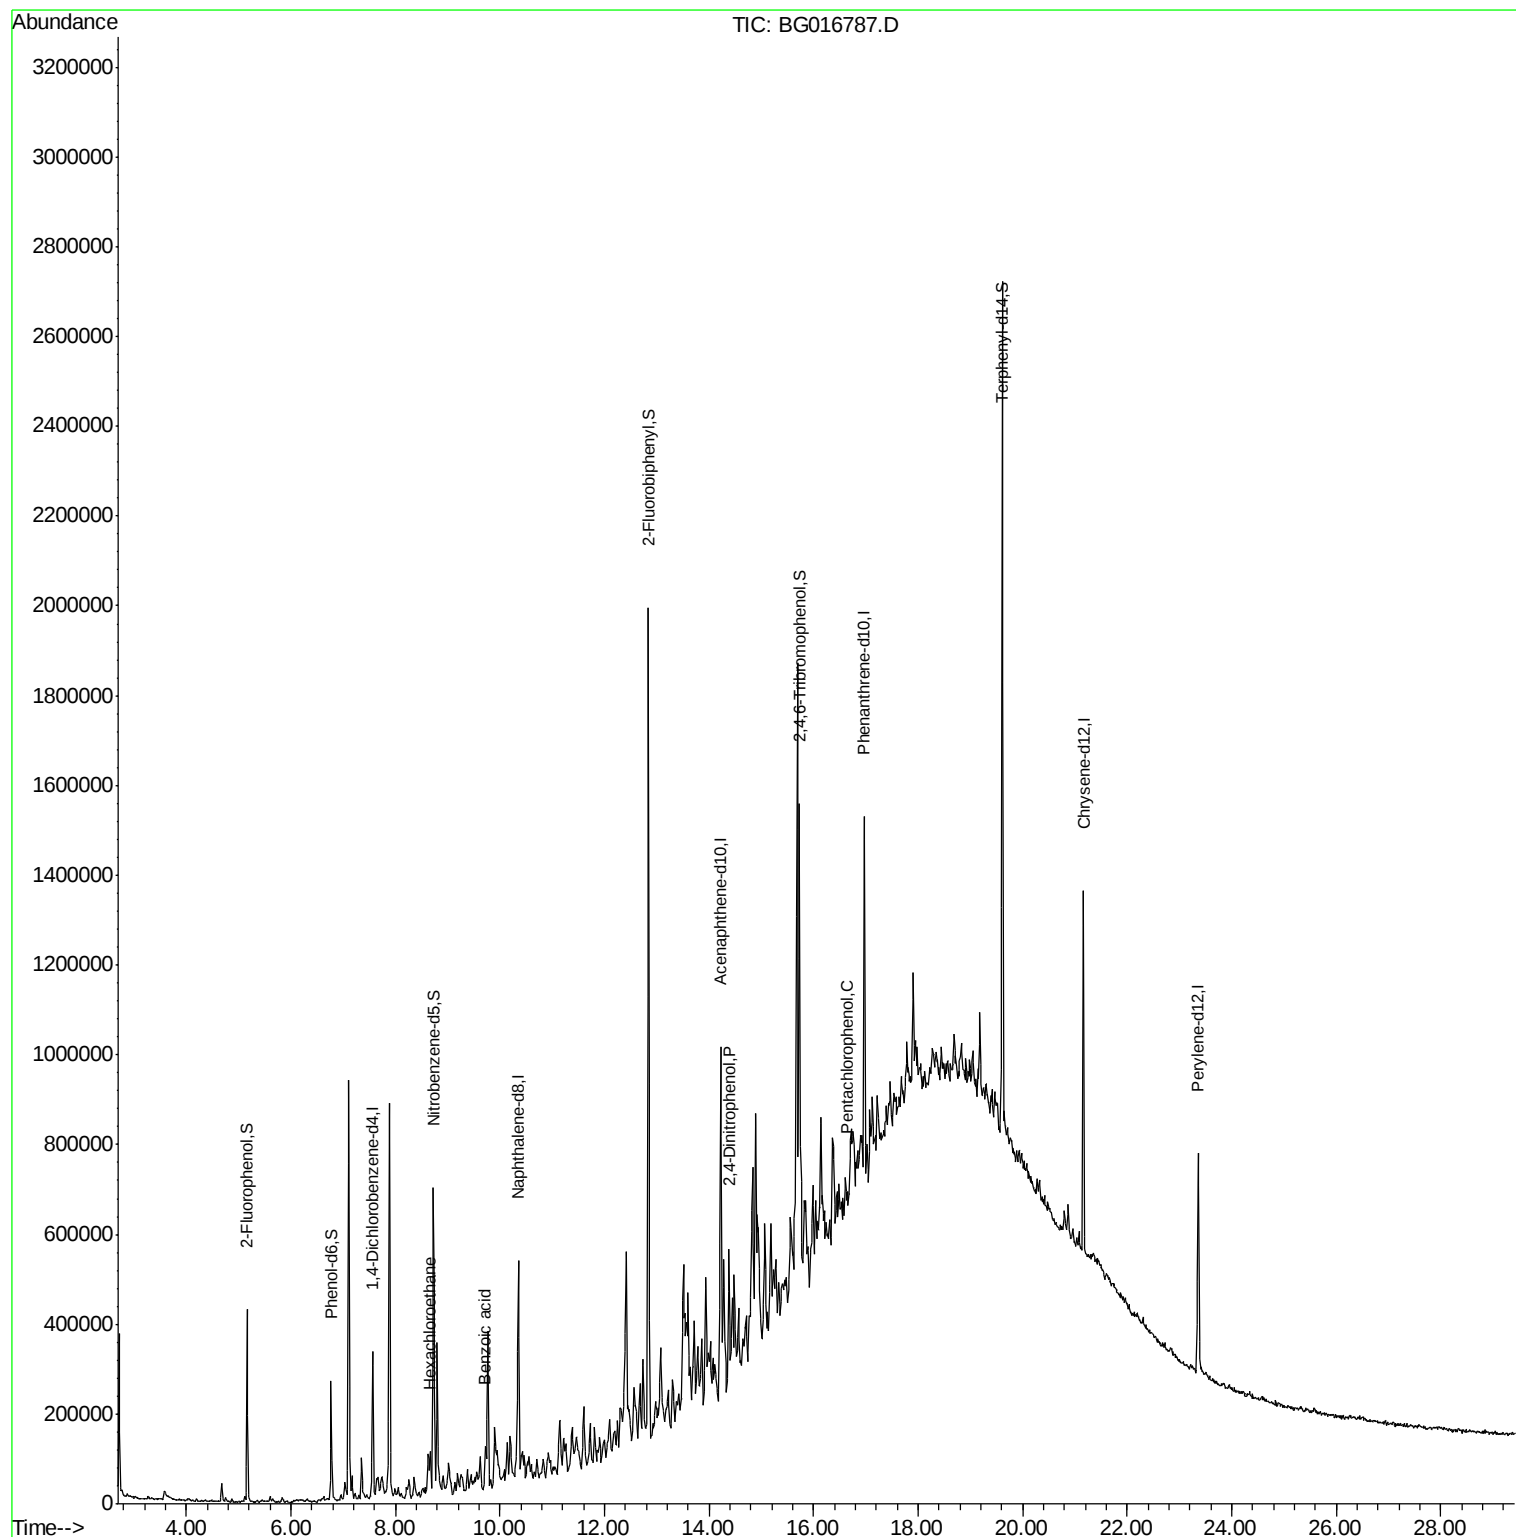

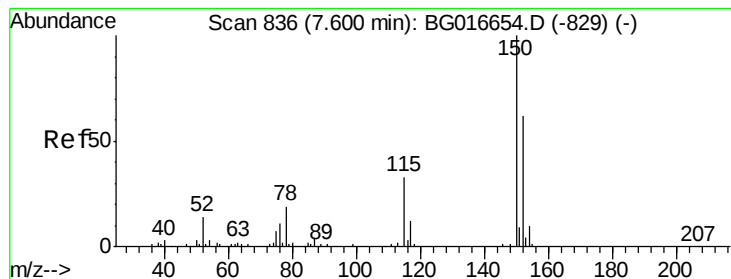

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.56 min Scan# 830

Delta R.T. -0.04 min

Lab File: BG016787.D

Acq: 29 Apr 2015 6:46

Instrument :

BNA_G

ClientSampleId :

MW-25


Tgt Ion:152 Resp: 85933

Ion Ratio Lower Upper

152 100

150 150.9 129.6 194.4




115 52.6 43.0 64.6

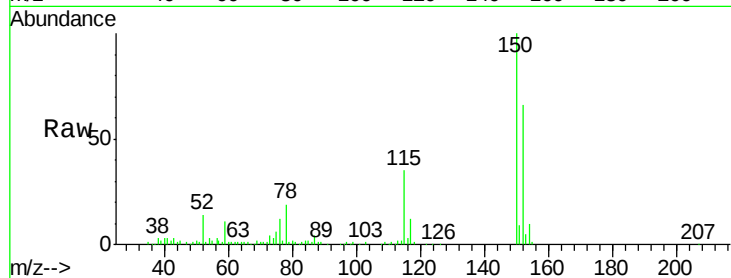

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

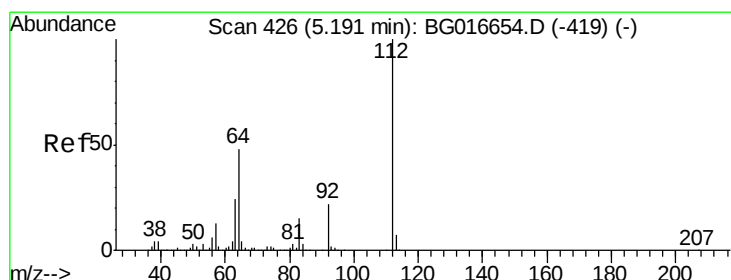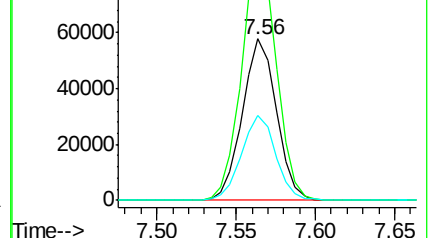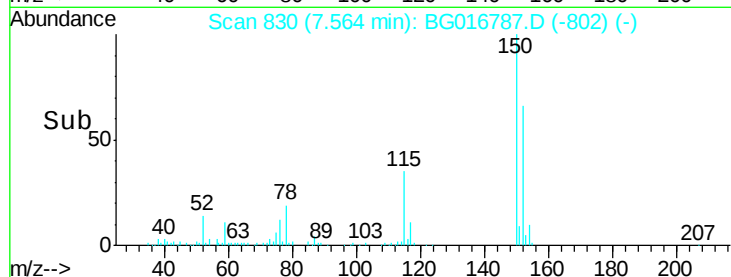

#5

2-Fluorophenol

Concen: 42.38 ng

RT: 5.16 min Scan# 421

Delta R.T. -0.03 min

Lab File: BG016787.D

Acq: 29 Apr 2015 6:46


Tgt Ion:112 Resp: 224425

Ion Ratio Lower Upper

112 100

64 44.7 38.3 57.5



63 22.0 18.9 28.3

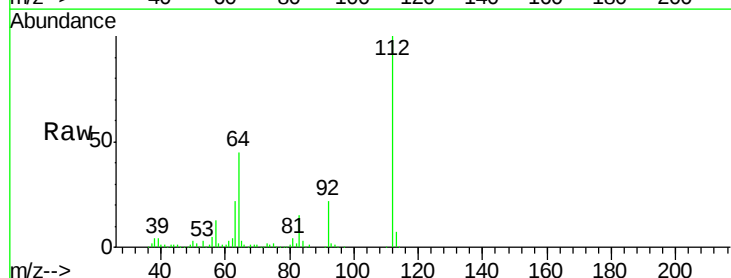


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

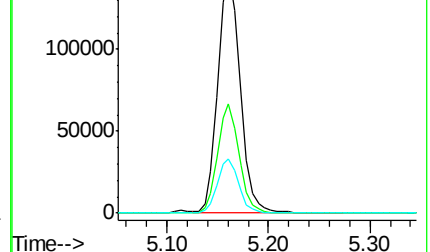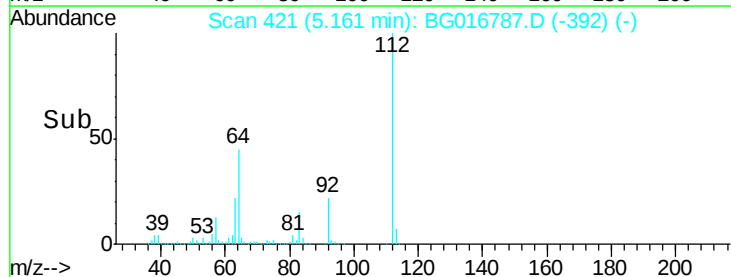

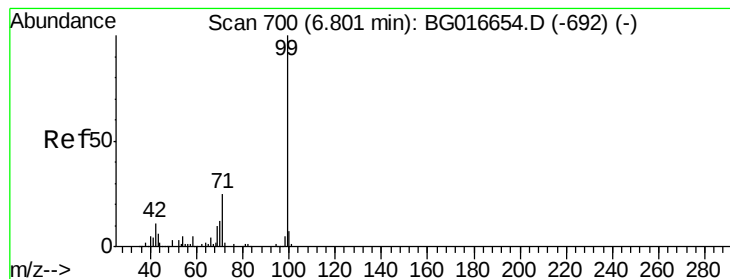

#7

Phenol-d6

Concen: 25.56 ng

RT: 6.77 min Scan# 695

Delta R.T. -0.03 min

Lab File: BG016787.D

Acq: 29 Apr 2015 6:46

Instrument :

BNA_G

ClientSampleId :

MW-25





Tgt Ion: 99 Resp: 189863

Ion Ratio Lower Upper

99 100

42 11.2 8.8 13.2

71 25.0 19.9 29.9

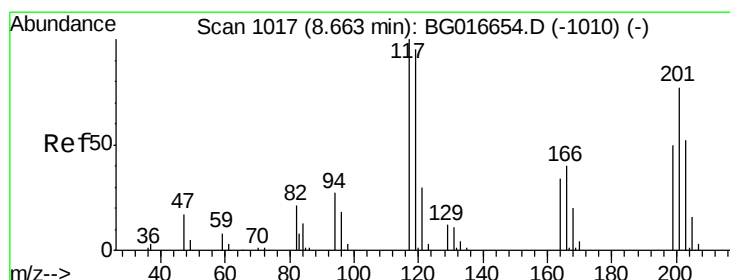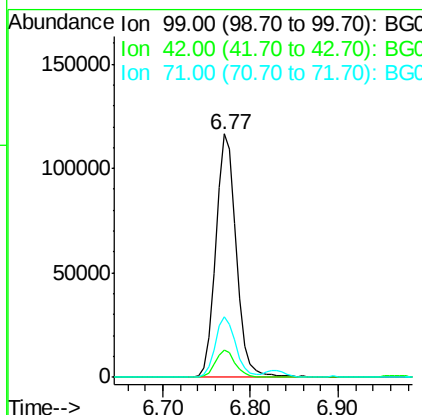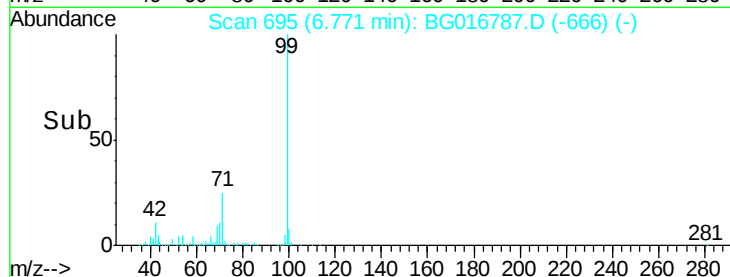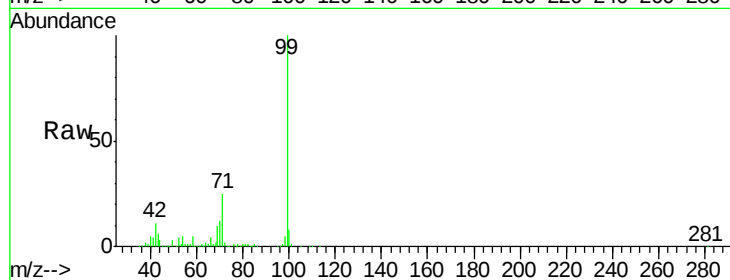

#18

Hexachloroethane

Concen: 2.81 ng

RT: 8.67 min Scan# 1018

Delta R.T. 0.01 min

Lab File: BG016787.D

Acq: 29 Apr 2015 6:46




Tgt Ion: 117 Resp: 6863


Ion Ratio Lower Upper

117 100

119 432.2 76.3 114.5#

201 0.0 61.5 92.3#

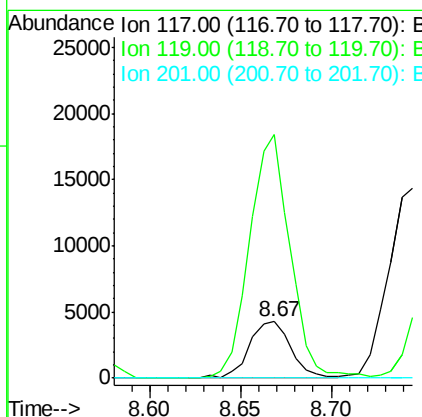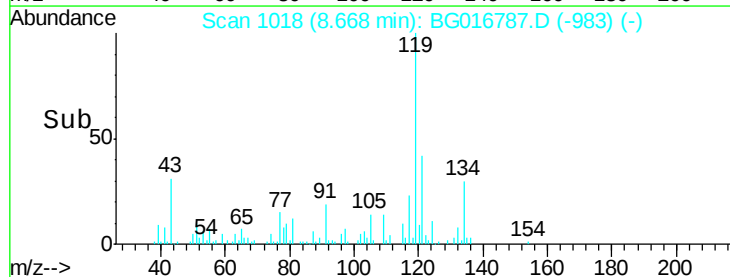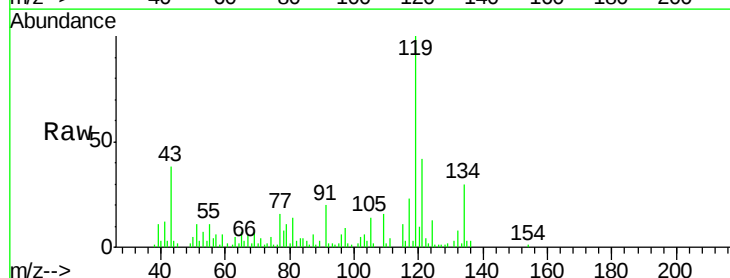


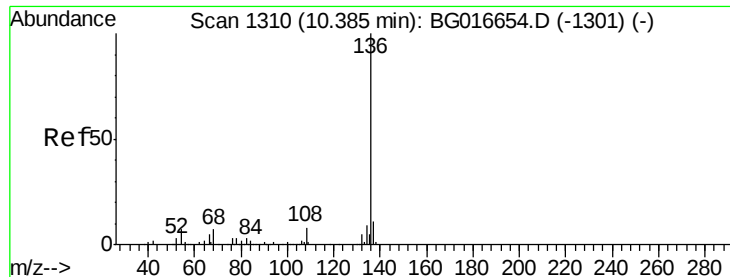




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.35 min Scan# 1304
Delta R.T. -0.04 min
Lab File: BG016787.D
Acq: 29 Apr 2015 6:46

Instrument :
BNA_G
ClientSampleId :
MW-25

Tgt Ion:	136	Resp:	368291
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.5	12.7
54	6.4	5.4	8.2
68	6.8	5.2	7.8

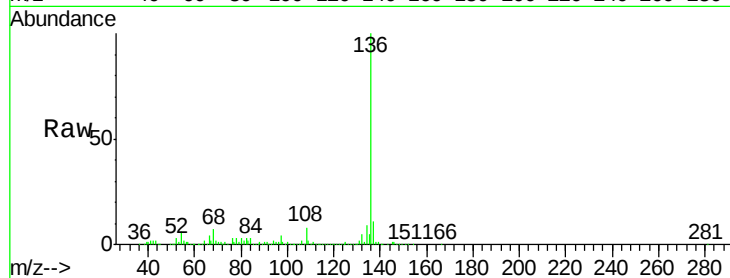


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

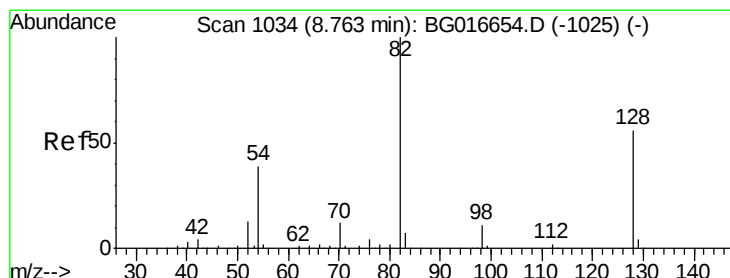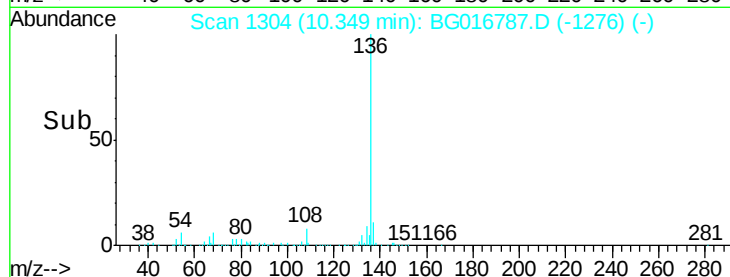
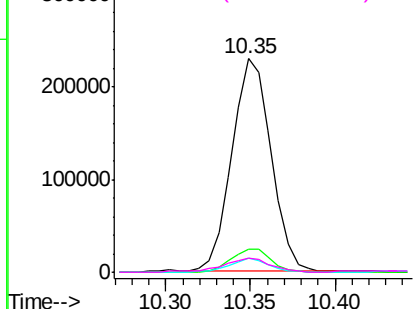



#23
Nitrobenzene-d5
Concen: 66.02 ng
RT: 8.73 min Scan# 1028
Delta R.T. -0.04 min
Lab File: BG016787.D
Acq: 29 Apr 2015 6:46

Tgt Ion:	82	Resp:	384798
Ion	Ratio	Lower	Upper
82	100		
128	57.6	44.7	67.1
54	37.6	30.9	46.3

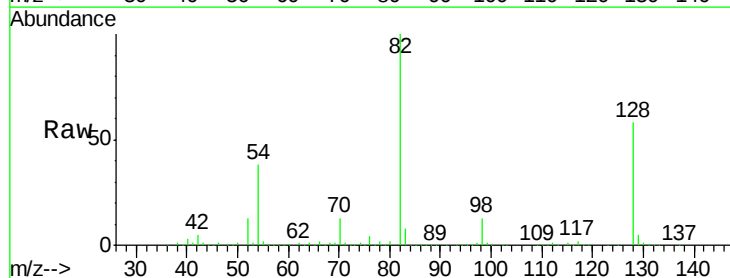

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

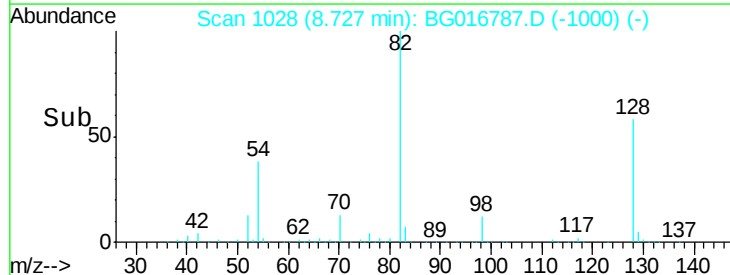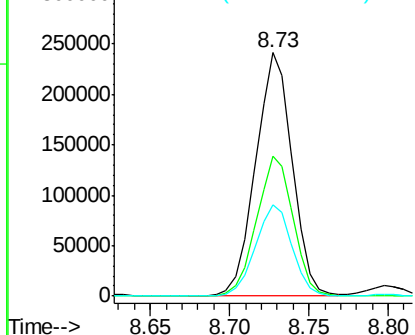

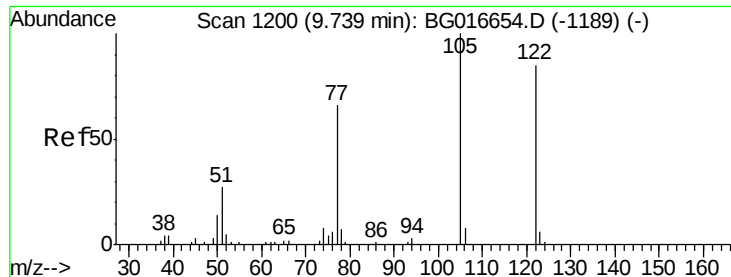

#32

Benzoic acid

Concen: 9.17 ng

RT: 9.71 min Scan# 1196

Delta R.T. -0.02 min

Lab File: BG016787.D

Acq: 29 Apr 2015 6:46

Instrument :

BNA_G

ClientSampleId :

MW-25


Tgt Ion:122 Resp: 1224

Ion Ratio Lower Upper

122 100

105 266.7 97.2 137.2#




77 326.7 58.4 98.4#

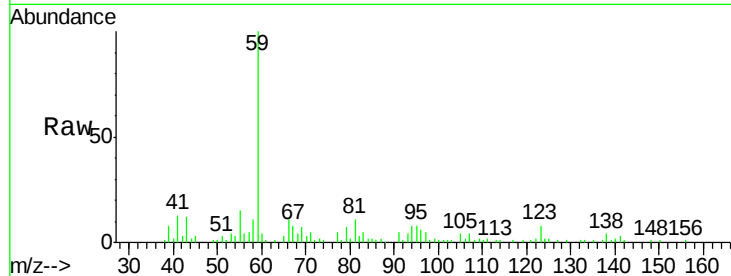

Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BGC

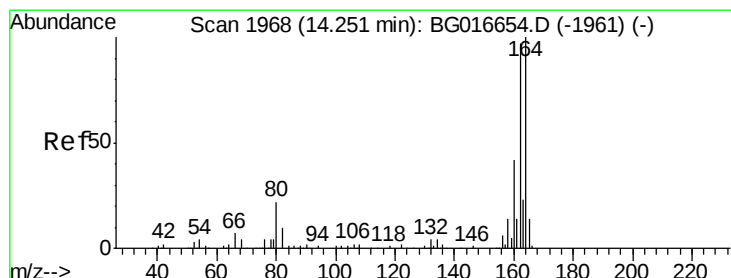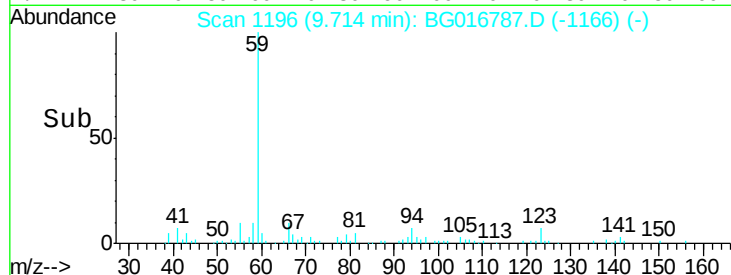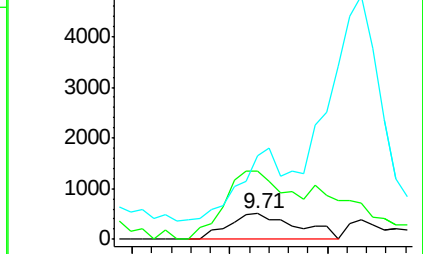

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.23 min Scan# 1964

Delta R.T. -0.02 min

Lab File: BG016787.D

Acq: 29 Apr 2015 6:46


Tgt Ion:164 Resp: 204309

Ion Ratio Lower Upper

164 100

162 96.9 77.3 115.9



160 53.0 33.7 50.5#

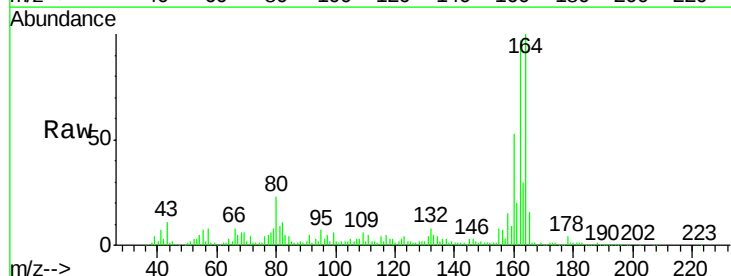


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

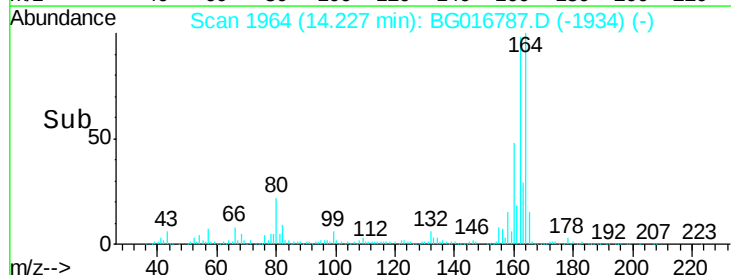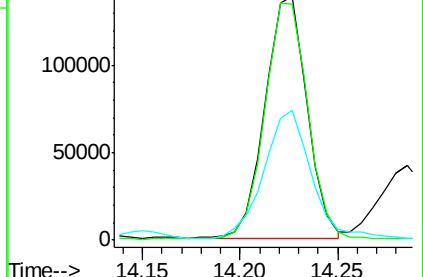


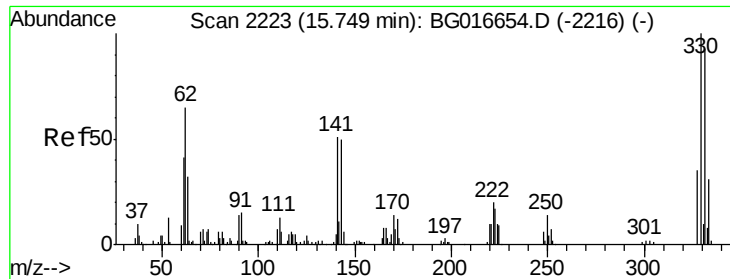




#41
 2,4,6-Tribromophenol
 Concen: 89.91 ng
 RT: 15.73 min Scan# 2220
 Delta R.T. -0.02 min
 Lab File: BG016787.D
 Acq: 29 Apr 2015 6:46

Instrument :
 BNA_G
 ClientSampleId :
 MW-25

Tgt Ion: 330 Resp: 136274
 Ion Ratio Lower Upper
 330 100
 332 96.7 76.2 114.4
 141 56.3 43.0 64.6

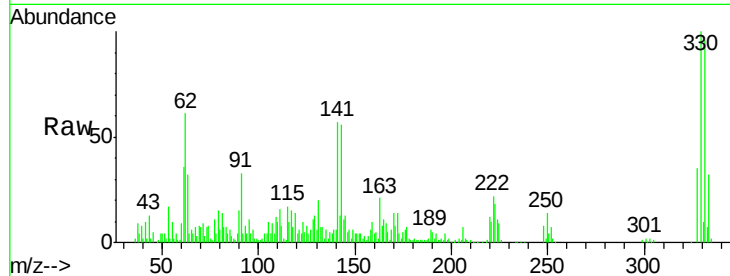


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

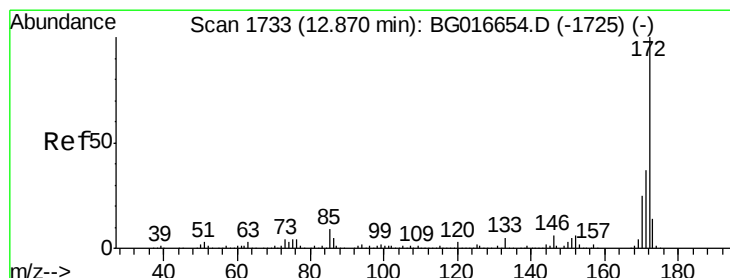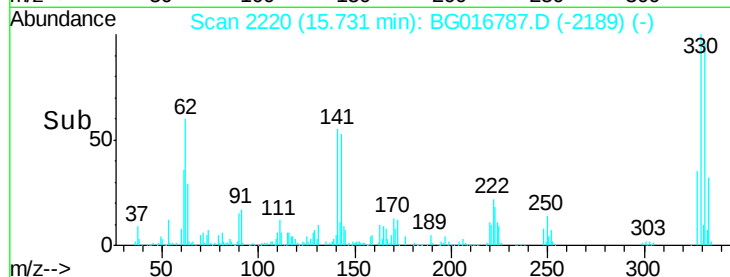
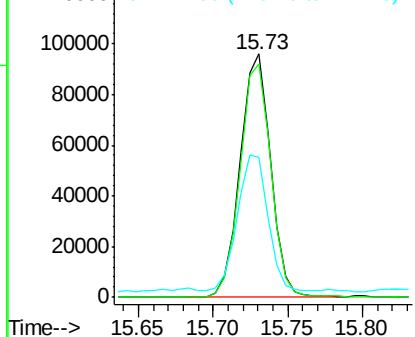



#44
 2-Fluorobiphenyl
 Concen: 71.62 ng
 RT: 12.84 min Scan# 1728
 Delta R.T. -0.03 min
 Lab File: BG016787.D
 Acq: 29 Apr 2015 6:46

Tgt Ion: 172 Resp: 910811
 Ion Ratio Lower Upper
 172 100
 171 37.8 29.9 44.9
 170 24.9 19.8 29.8

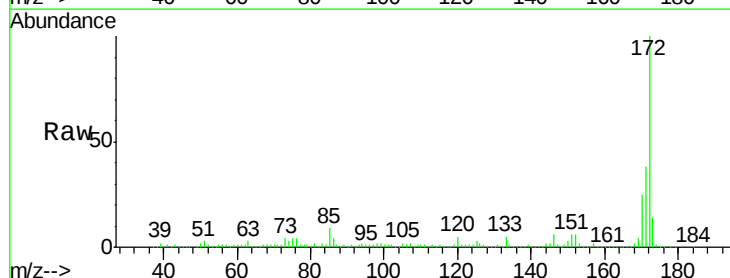

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



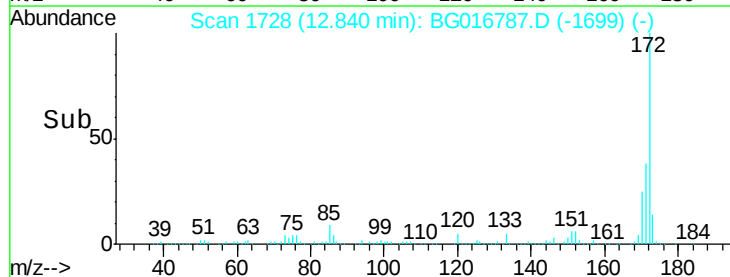
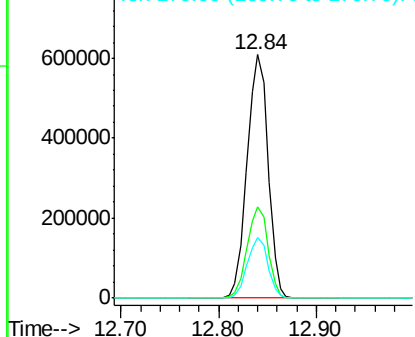


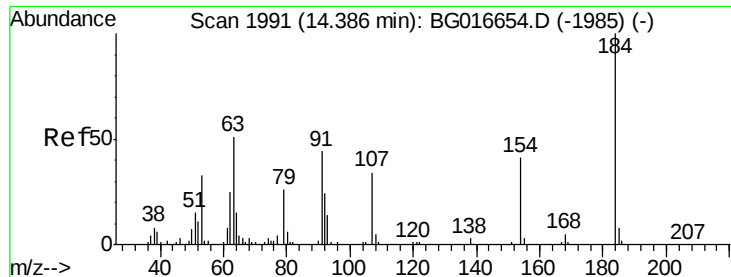

#53
 2,4-Dinitrophenol
 Concen: 7.71 ng
 RT: 14.39 min Scan# 1991
 Delta R.T. -0.00 min
 Lab File: BG016787.D
 Acq: 29 Apr 2015 6:46




Instrument :
 BNA_G
 ClientSampleId :
 MW-25


Tgt Ion:184 Resp: 234
 Ion Ratio Lower Upper
 184 100
 63 832.5 40.7 61.1#
 154 255.8 34.1 51.1#

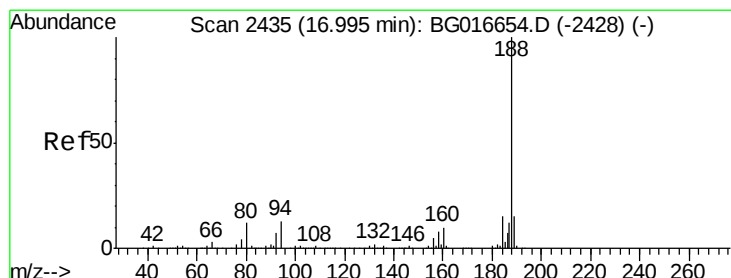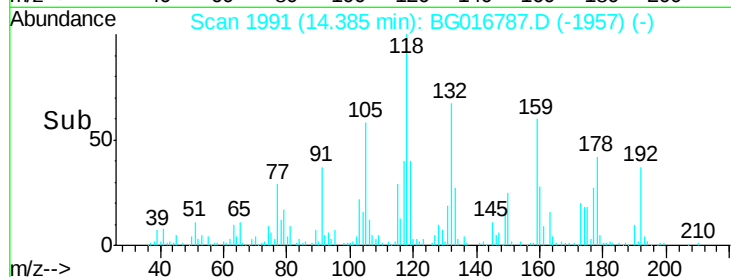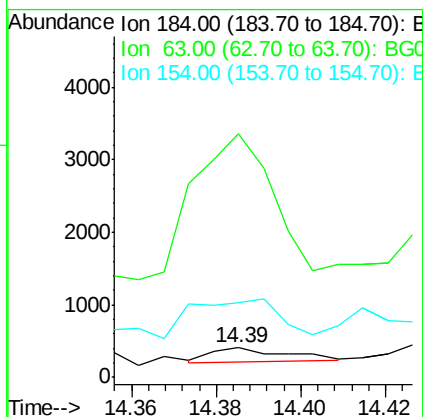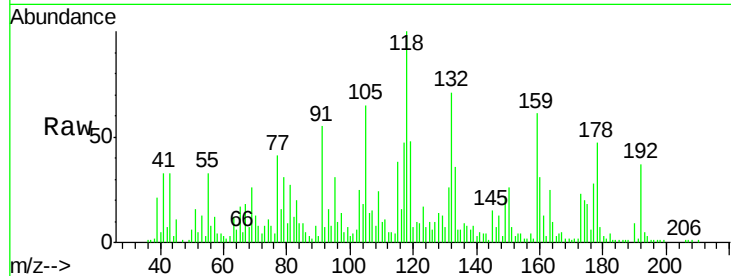

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 16.97 min Scan# 2431
 Delta R.T. -0.02 min
 Lab File: BG016787.D
 Acq: 29 Apr 2015 6:46

Tgt Ion:188 Resp: 365138
 Ion Ratio Lower Upper
 188 100
 94 15.7 10.7 16.1
 80 14.2 9.9 14.9


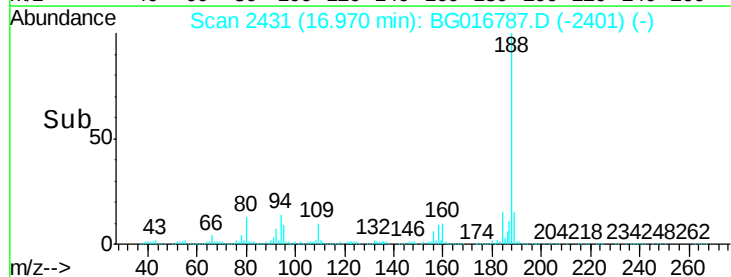
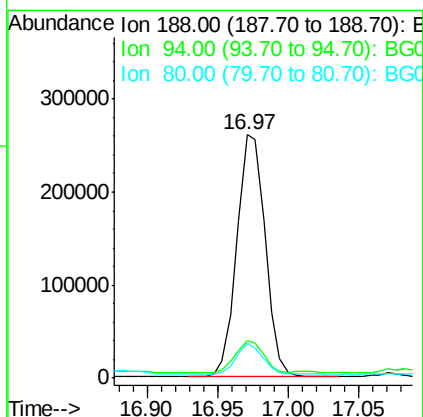
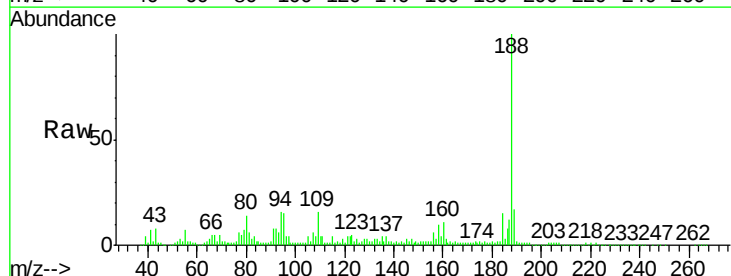


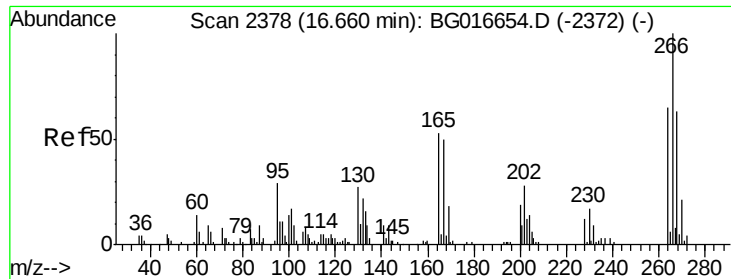

#69
 Pentachlorophenol
 Concen: 3.24 ng
 RT: 16.64 min Scan# 2375
 Delta R.T. -0.02 min
 Lab File: BG016787.D
 Acq: 29 Apr 2015 6:46




Instrument :
 BNA_G
 ClientSampleId :
 MW-25


Tgt Ion: 266 Resp: 4942
 Ion Ratio Lower Upper
 266 100
 268 58.9 50.6 76.0
 264 49.1 51.8 77.6#

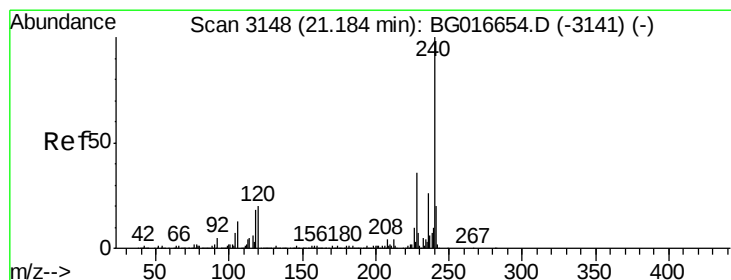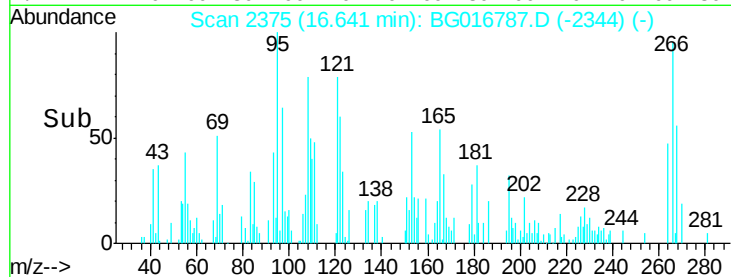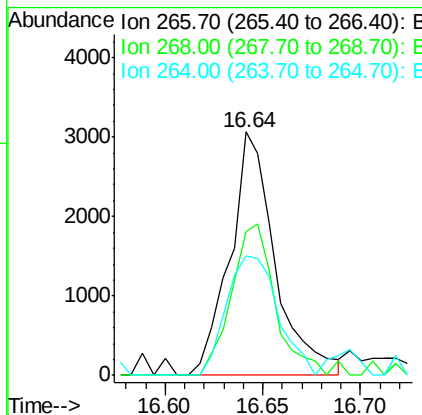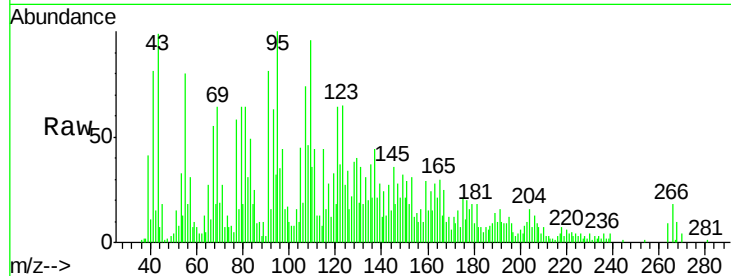

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 21.17 min Scan# 3145
 Delta R.T. -0.02 min
 Lab File: BG016787.D
 Acq: 29 Apr 2015 6:46

Tgt Ion: 240 Resp: 309102
 Ion Ratio Lower Upper
 240 100
 120 20.2 16.3 24.5
 236 27.7 21.1 31.7


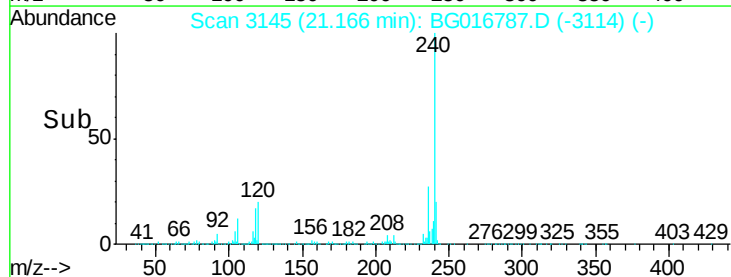
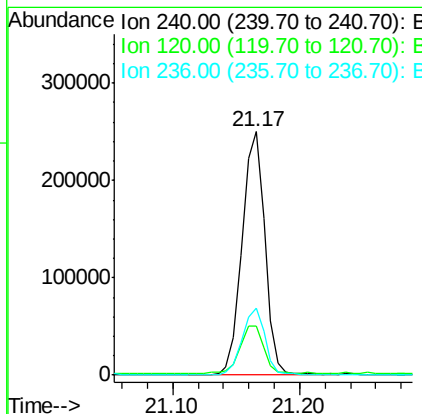
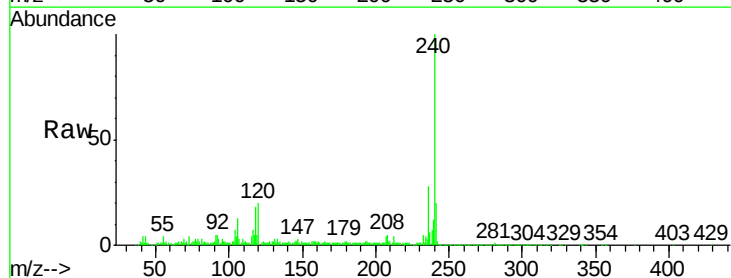


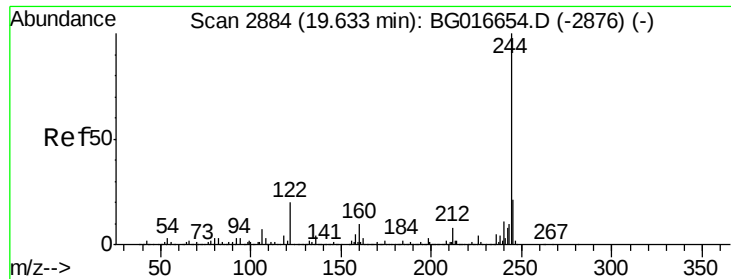

#78
 Terphenyl-d14
 Concen: 53.13 ng
 RT: 19.61 min Scan# 2881
 Delta R.T. -0.02 min
 Lab File: BG016787.D
 Acq: 29 Apr 2015 6:46

Instrument :
 BNA_G
 ClientSampleId :
 MW-25

Tgt Ion:244 Resp: 712965
 Ion Ratio Lower Upper
 244 100
 212 8.4 6.4 9.6
 122 19.7 15.9 23.9

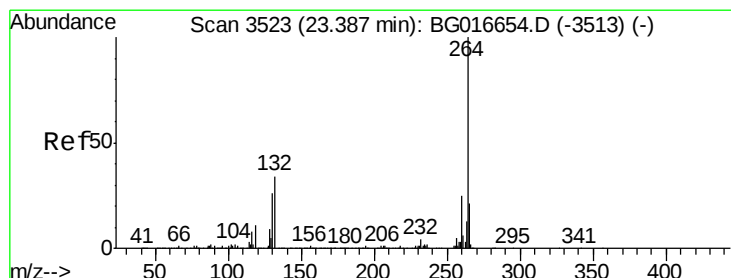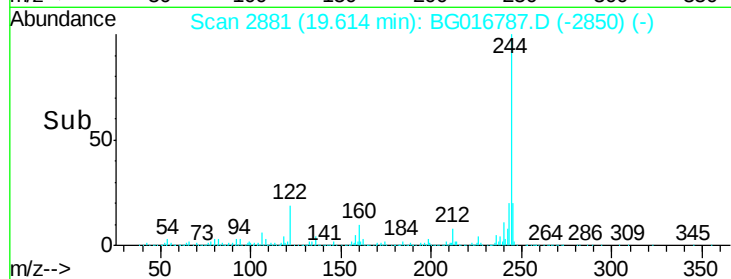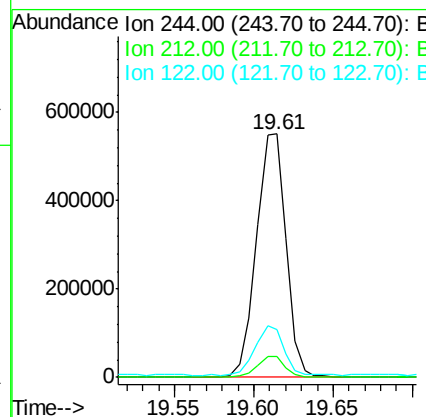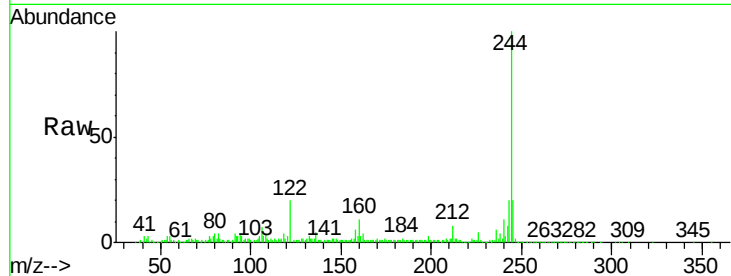

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 23.36 min Scan# 3519
 Delta R.T. -0.02 min
 Lab File: BG016787.D
 Acq: 29 Apr 2015 6:46

Tgt Ion:264 Resp: 296996
 Ion Ratio Lower Upper
 264 100
 260 25.0 20.0 30.0
 265 21.6 16.8 25.2

