


Data Path : Z:\HPCHEM1\BNA_G\Data\BG042815\
Data File : BG016782.D
Acq On : 29 Apr 2015 3:17
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 29 00:55:31 2015

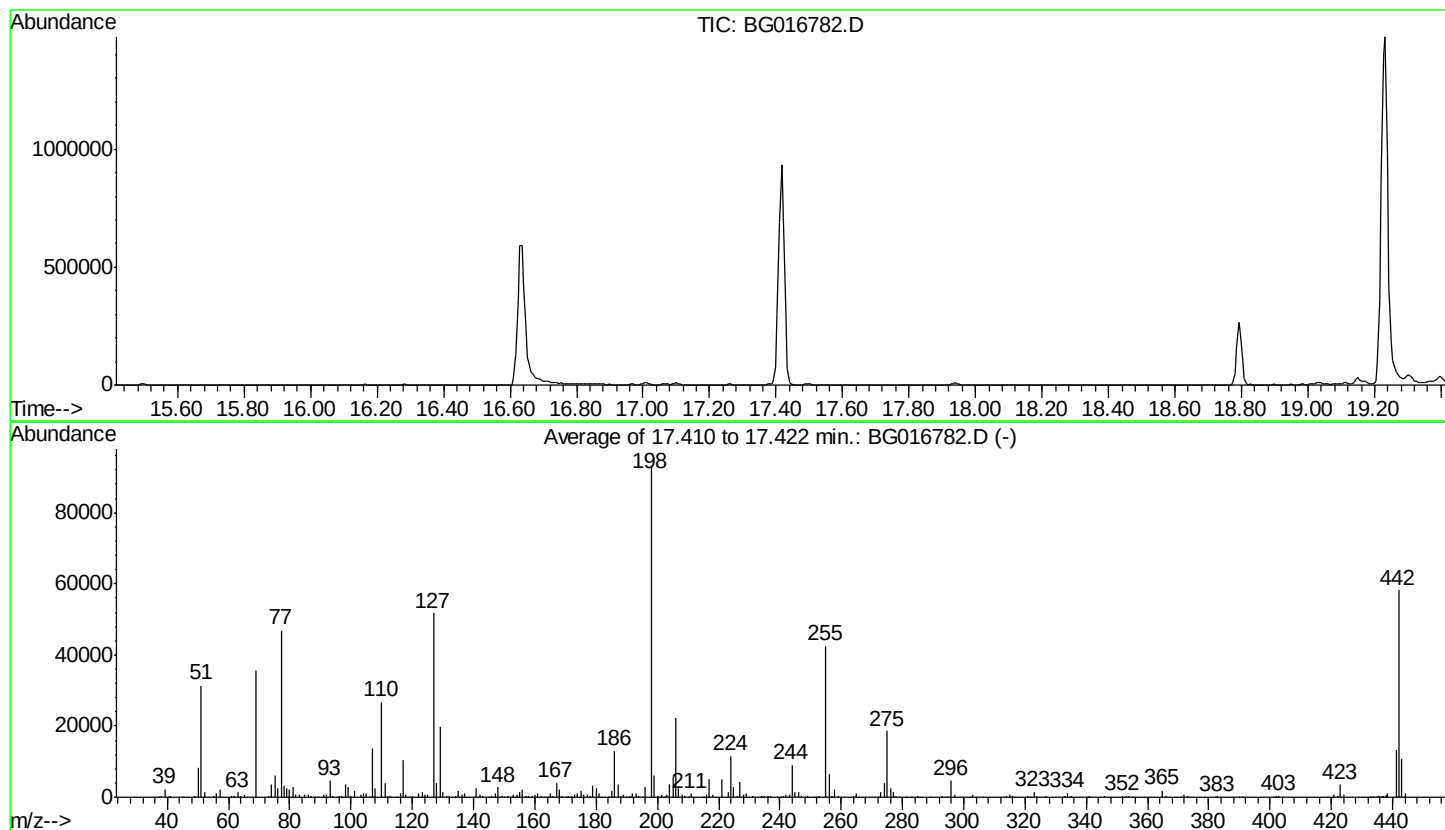

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	31461	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.1	35510	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.5	51757	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93226	PASS
199	198	5	9	6.7	6214	PASS
275	198	10	60	20.0	18683	PASS
365	198	1	100	2.0	1900	PASS
441	442	0.01	24	22.6	13190	PASS
442	198	50	100	62.5	58298	PASS
443	442	15	24	18.7	10886	PASS