
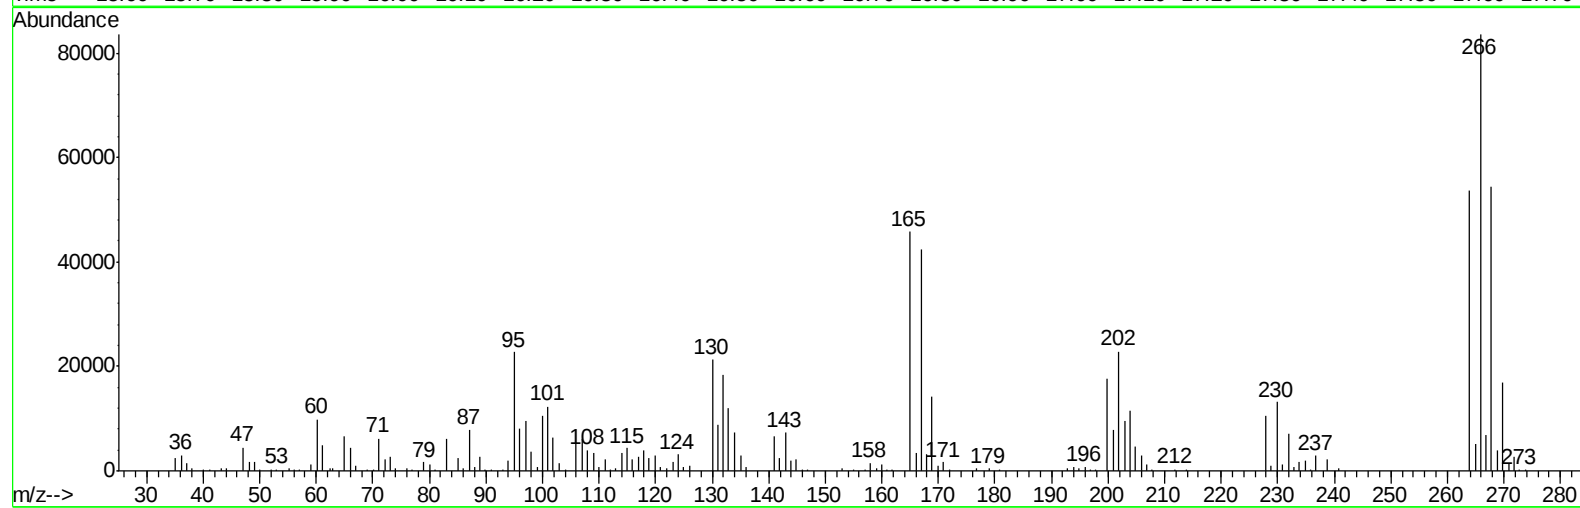


Data Path : Z:\HPCHEM1\BNA_G\Data\BG042815\
Data File : BG016764.D
Acq On : 28 Apr 2015 14:34
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 07:15:30 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 29 00:55:31 2015
Response via : Initial Calibration

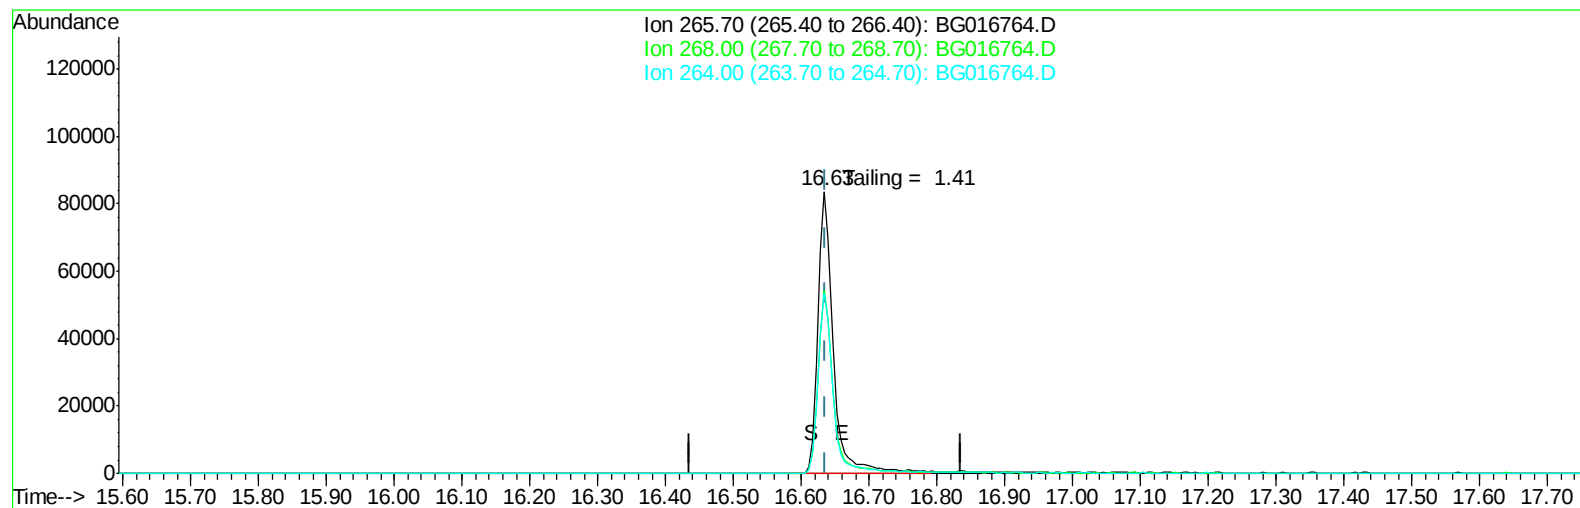

TIC: BG016764.D

(69) Pentachlorophenol (C)



16.634min (-0.003) 18418.20ng

response 128739

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	65.16
264.00	64.70	64.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042815\
Data File : BG016764.D
Acq On : 28 Apr 2015 14:34
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 07:15:30 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 29 00:55:31 2015
Response via : Initial Calibration

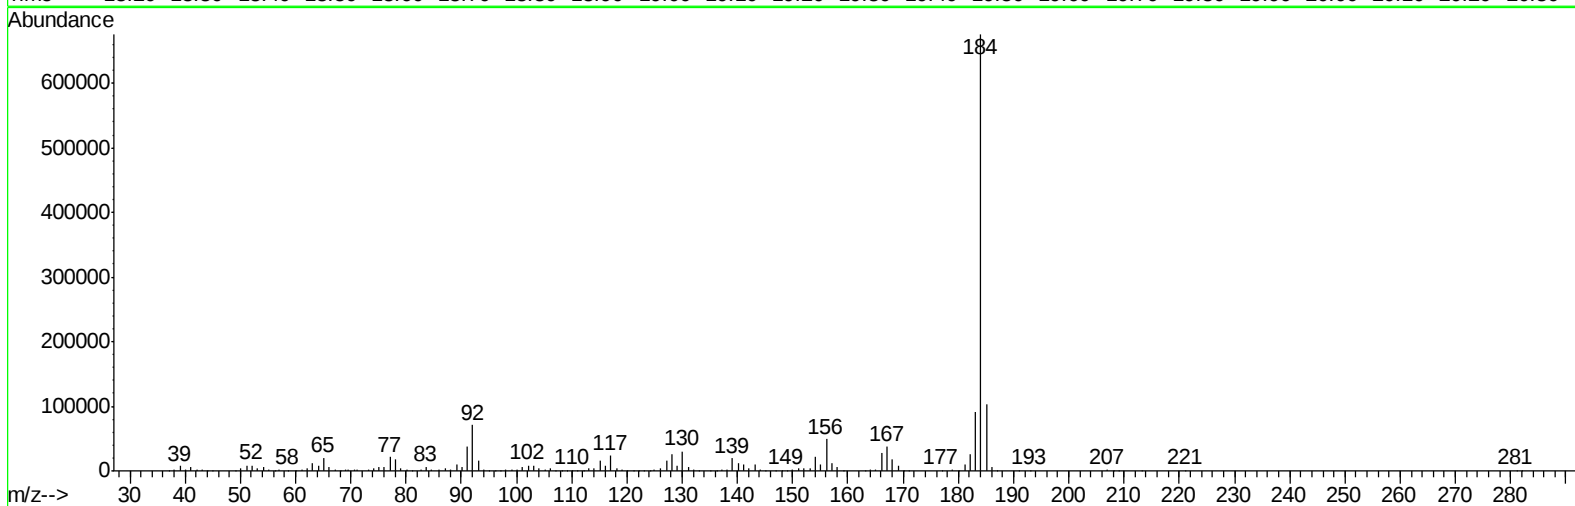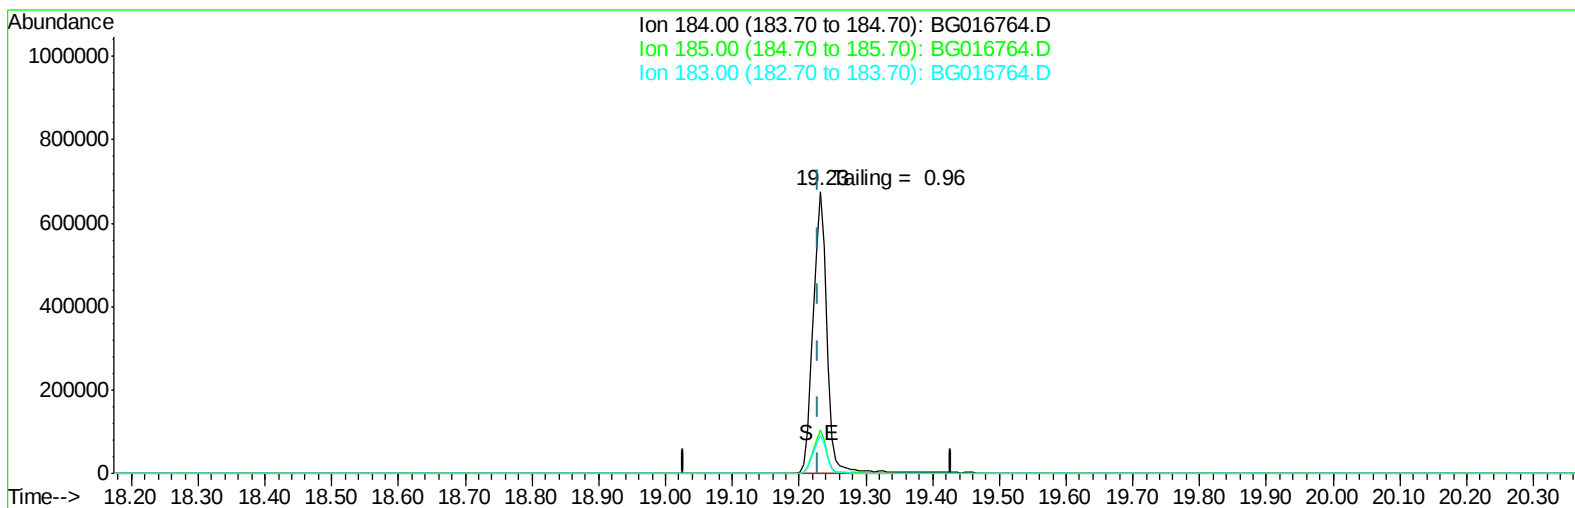

TIC: BG016764.D

(76) Benzidine

19.231min (+0.003) 511936.16ng

response 941543

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.34
183.00	12.60	13.64
0.00	0.00	0.00