
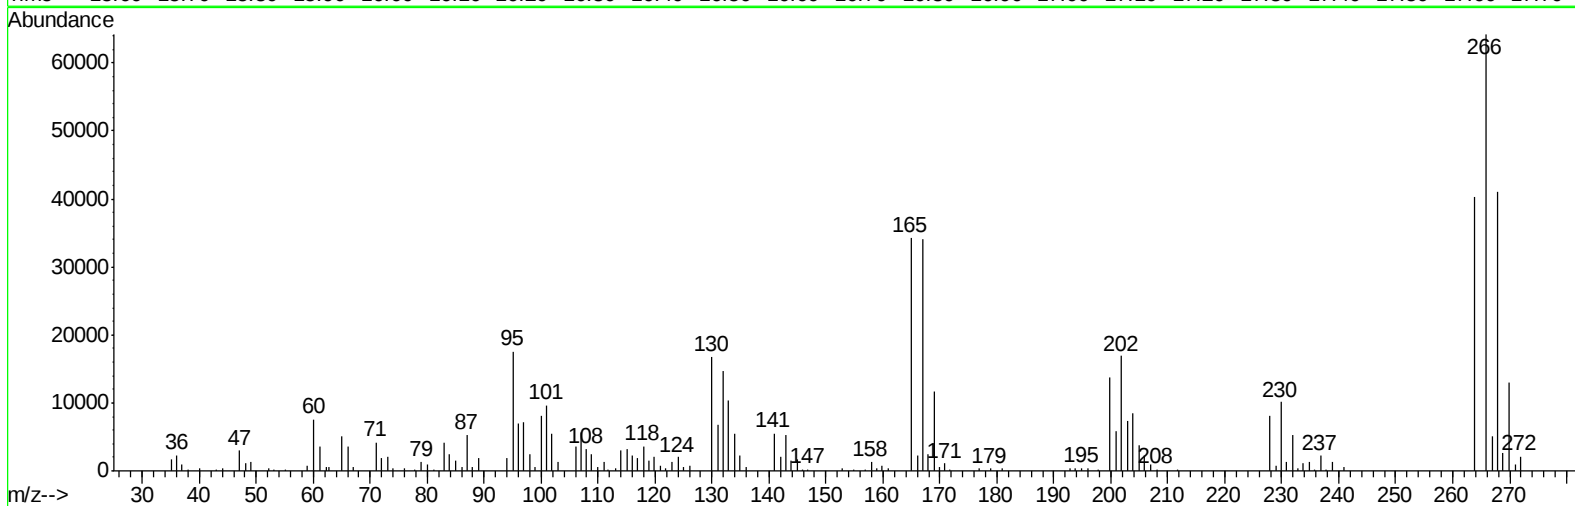


Data Path : Z:\HPCHEM1\BNA_G\Data\BG042815\
Data File : BG016782.D
Acq On : 29 Apr 2015 3:17
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 07:38:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 29 00:55:31 2015
Response via : Initial Calibration

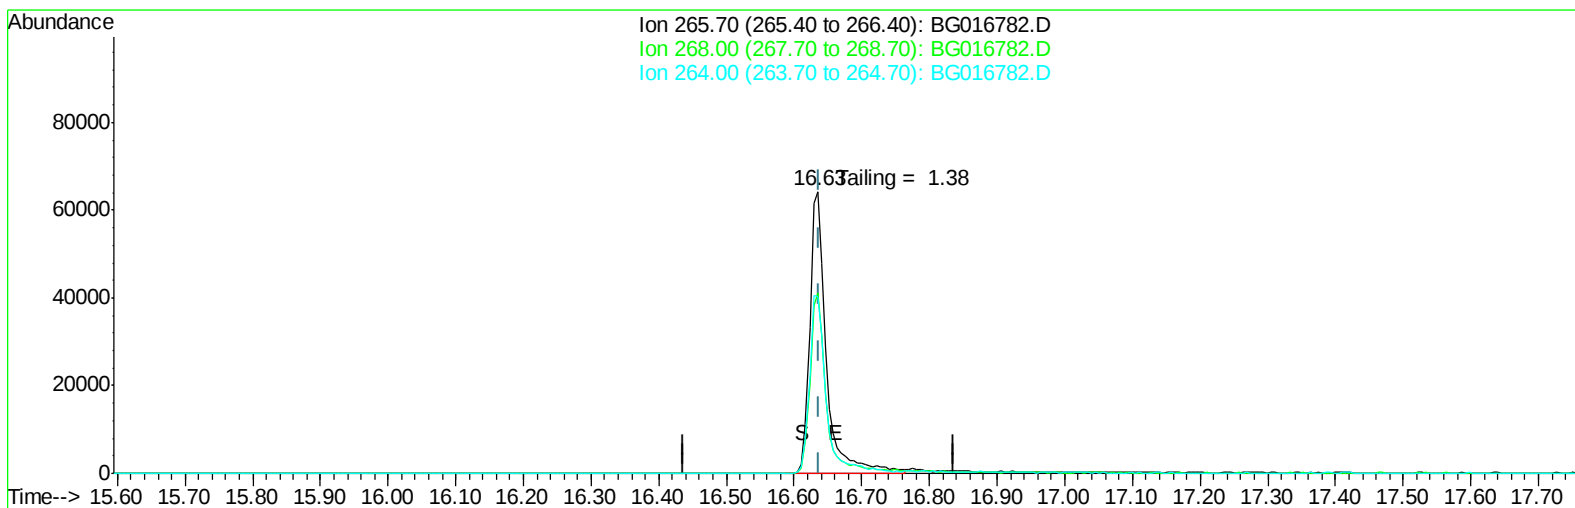

TIC: BG016782.D

(69) Pentachlorophenol (C)



16.635min (-0.003) 24570.06ng

response 109708

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	64.01
264.00	64.70	62.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042815\
Data File : BG016782.D
Acq On : 29 Apr 2015 3:17
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 07:38:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 29 00:55:31 2015
Response via : Initial Calibration

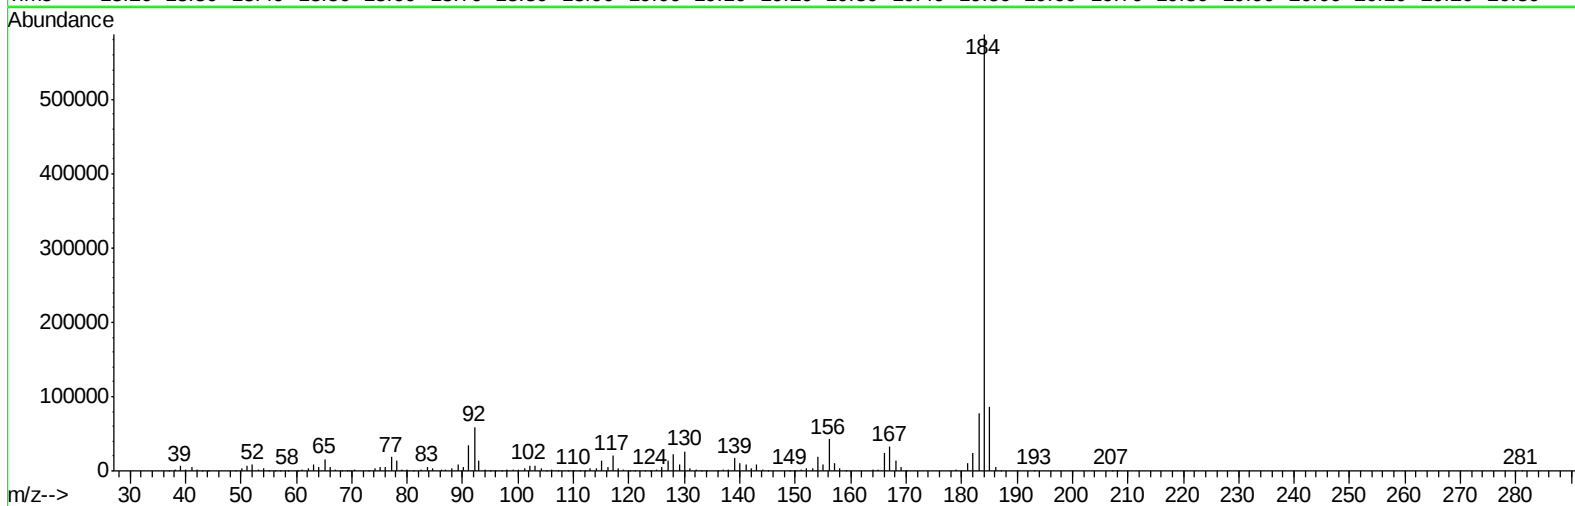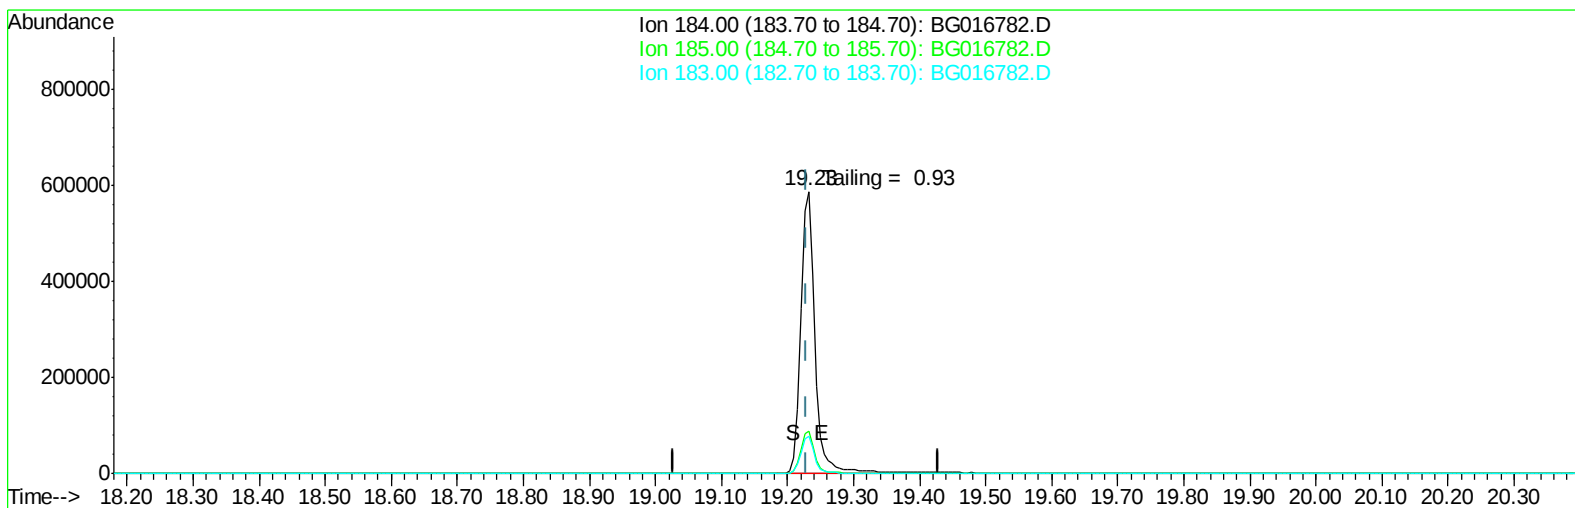

TIC: BG016782.D

(76) Benzidine

19.232min (+0.003) 16144.00ng

response 887453

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.80
183.00	12.60	13.25
0.00	0.00	0.00