

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
 Data File : BG016773.D
 Acq On : 28 Apr 2015 20:11
 Operator : TP/IZ
 Sample : G2022-06 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-02-COMP

Quant Time: Apr 29 01:45:41 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 29 00:55:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	65409	20.00	ng	0.00
21) Naphthalene-d8	10.35	136	291302	20.00	ng	0.00
38) Acenaphthene-d10	14.22	164	161497	20.00	ng	0.00
63) Phenanthrene-d10	16.98	188	289428	20.00	ng	0.00
75) Chrysene-d12	21.18	240	209821	20.00	ng	0.02
86) Perylene-d12	23.39	264	249657	20.00	ng	0.03

System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	91612	22.73	ng	0.00
7) Phenol-d6	6.77	99	128016	22.64	ng	0.00
23) Nitrobenzene-d5	8.72	82	65377	14.18	ng	0.00
41) 2,4,6-Tribromophenol	15.72	330	25236	21.06	ng	0.00
44) 2-Fluorobiphenyl	12.84	172	167108	16.62	ng	0.00
78) Terphenyl-d14	19.61	244	170139	18.68	ng	0.00


Target Compounds						Qvalue
31) Naphthalene	10.40	128	664115	43.24	ng	100
37) 2-Methylnaphthalene	12.02	142	297907	26.85	ng	99
45) 1,1'-Biphenyl	13.05	154	118604	9.35	ng	97
48) Acenaphthylene	13.95	152	260388	15.25	ng	97
51) Acenaphthene	14.29	154	658319	64.23	ng	99
54) Dibenzofuran	14.63	168	1045661	72.33	ng	98
57) Fluorene	15.28	166	1269693	100.48	ng	99
70) Phenanthrene	17.05	178	5665030	340.71	ng	# 54
71) Anthracene	17.12	178	2476455	149.74	ng	# 83
72) Carbazole	17.38	167	868486	52.42	ng	99
74) Fluoranthene	19.08	202	5923674	336.22	ng	63
77) Pylene	19.44	202	5255942	356.56	ng	# 58
80) Benzo(a)anthracene	21.17	228	3387338m	266.24	ng	
82) Chrysene	21.23	228	3312685m	271.59	ng	
85) Indeno(1,2,3-cd)pyrene	25.66	276	2247414	169.06	ng	91
87) Benzo(b)fluoranthene	22.74	252	4148623	273.57	ng	# 83
88) Benzo(k)fluoranthene	22.78	252	1590739m	107.49	ng	
89) Benzo(a)pyrene	23.32	252	3208551	224.53	ng	# 85
90) Dibenzo(a,h)anthracene	25.64	278	656265	47.23	ng	# 65
91) Benzo(a,h,i)perylene	26.35	276	1999856	141.45	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
Data File : BG016773.D
Acq On : 28 Apr 2015 20:11
Operator : TP/IZ
Sample : G2022-06 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-02-COMP

Quant Time: Apr 29 01:45:41 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 29 00:55:31 2015
Response via : Initial Calibration









#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.57 min Scan# 830
Delta R.T. -0.00 min
Lab File: BG016773.D
Acq: 28 Apr 2015 20:11

Instrument :
BNA_G
ClientSampleId :
SB-02-COMP




Tot Ion:152 Resp: 65409
Ion Ratio Lower Upper
152 100
150 152.0 129.6 194.4
115 51.6 43.0 64.6




#5

2-Fluorophenol
Concen: 22.73 ng
RT: 5.16 min Scan# 420
Delta R.T. -0.00 min
Lab File: BG016773.D
Acq: 28 Apr 2015 20:11

Tgt Ion:112 Resp: 91612
Ion Ratio Lower Upper
112 100
64 43.9 38.3 57.5
63 21.0 18.9 28.3





#7

Phenol-d6

Concen: 22.64 ng

RT: 6.77 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Instrument :

BNA_G

ClientSampleId :

SB-02-COMP


Tot Ion: 99 Resp: 128016

Ion Ratio Lower Upper




99 100

42 11.0 8.8 13.2

71 24.2 19.9 29.9



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

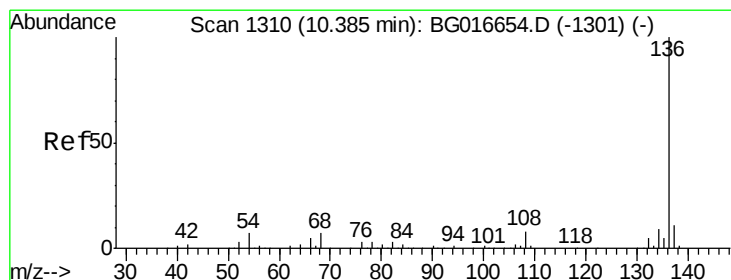

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.35 min Scan# 1304

Delta R.T. -0.00 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Tgt Ion: 136 Resp: 291302


Ion Ratio Lower Upper

136 100



137 10.8 8.5 12.7


54 5.3 5.4 8.2#

68 5.6 5.2 7.8



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC









#23
 Nitrobenzene-d5
 Concen: 14.18 ng
 RT: 8.72 min Scan# 1027
 Delta R.T. -0.01 min
 Lab File: BG016773.D
 Acq: 28 Apr 2015 20:11

Instrument :
 BNA_G
 ClientSampleId :
 SB-02-COMP

Tot Ion	82	Resp	65377
Ion Ratio	100	Lower	Upper
128	55.9	44.7	67.1
54	37.2	30.9	46.3




Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC






#31
 Naphthalene
 Concen: 43.24 ng
 RT: 10.40 min Scan# 1313
 Delta R.T. -0.00 min
 Lab File: BG016773.D
 Acq: 28 Apr 2015 20:11

Tgt Ion	128	Resp	664115
Ion Ratio	100	Lower	Upper
129	11.2	9.0	13.6
127	13.6	11.1	16.7



Abundance Ion 128.00 (127.70 to 128.70): BGC
 Ion 129.00 (128.70 to 129.70): BGC
 Ion 127.00 (126.70 to 127.70): BGC









#37
2-Methylnaphthalene
Concen: 26.85 ng
RT: 12.02 min Scan# 1589
Delta R.T. -0.00 min
Lab File: BG016773.D
Acq: 28 Apr 2015 20:11




Instrument :
BNA_G
ClientSampleId :
SB-02-COMP


Tot Ion:142 Resp: 297907
Ion Ratio Lower Upper
142 100
141 86.9 69.9 104.9
115 29.0 24.0 36.0



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.22 min Scan# 1963
Delta R.T. -0.01 min
Lab File: BG016773.D
Acq: 28 Apr 2015 20:11

Tgt Ion:164 Resp: 161497
Ion Ratio Lower Upper
164 100
162 96.7 77.3 115.9
160 42.9 33.7 50.5









#41
 2,4,6-Tribromophenol
 Concen: 21.06 ng
 RT: 15.72 min Scan# 2218
 Delta R.T. -0.01 min
 Lab File: BG016773.D
 Acq: 28 Apr 2015 20:11




Instrument :
 BNA_G
 ClientSampleId :
 SB-02-COMP


Tot Ion	Ratio	Lower	Upper
330	100		
332	94.1	76.2	114.4
141	53.4	43.0	64.6



#44
 2-Fluorobiphenyl
 Concen: 16.62 ng
 RT: 12.84 min Scan# 1727
 Delta R.T. -0.01 min
 Lab File: BG016773.D
 Acq: 28 Apr 2015 20:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	29.9	44.9
170	24.4	19.8	29.8









#45
 1,1'-Biphenyl
 Concen: 9.35 ng
 RT: 13.05 min Scan# 1763
 Delta R.T. -0.01 min
 Lab File: BG016773.D
 Acq: 28 Apr 2015 20:11




Instrument :
 BNA_G
 ClientSampleId :
 SB-02-COMP


Tot Ion	Ratio	Lower	Upper
154	100		
153	39.7	21.8	61.8
76	12.4	0.0	33.7



#48
 Acenaphthylene
 Concen: 15.25 ng
 RT: 13.95 min Scan# 1916
 Delta R.T. -0.00 min
 Lab File: BG016773.D
 Acq: 28 Apr 2015 20:11

Tgt Ion	Ratio	Lower	Upper
152	100		
151	21.2	16.7	25.1
153	16.1	11.0	16.6





#51

Acenaphthene

Concen: 64.23 ng

RT: 14.29 min Scan# 1974

Delta R.T. -0.01 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Instrument :

BNA_G

ClientSampleId :

SB-02-COMP


Tot Ion:154 Resp: 658319

Ion Ratio Lower Upper

154 100

153 107.7 87.0 130.6




152 53.5 41.6 62.4



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E



#54

Dibenzofuran

Concen: 72.33 ng

RT: 14.63 min Scan# 2032

Delta R.T. -0.00 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11


Tgt Ion:168 Resp: 1045661

Ion Ratio Lower Upper

168 100

139 38.4 29.8 44.8



169 15.0 11.0 16.4




Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E









#57
Fluorene
 Concen: 100.48 ng
 RT: 15.28 min Scan# 2143
 Delta R.T. 0.01 min
 Lab File: BG016773.D
 Acq: 28 Apr 2015 20:11

Instrument :
 BNA_G
 ClientSampleId :
 SB-02-COMP

Tot Ion:166 Resp: 1269693
 Ion Ratio Lower Upper
 166 100
 165 95.1 75.6 113.4
 167 15.4 10.7 16.1




Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E






#63
Phenanthrene-d10
 Concen: 20.00 ng
 RT: 16.98 min Scan# 2432
 Delta R.T. 0.01 min
 Lab File: BG016773.D
 Acq: 28 Apr 2015 20:11

Tgt Ion:188 Resp: 289428
 Ion Ratio Lower Upper
 188 100
 94 11.2 10.7 16.1
 80 11.4 9.9 14.9



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC





#70

Phenanthrene

Concen: 340.71 ng

RT: 17.05 min Scan# 2444

Delta R.T. 0.03 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Instrument :

BNA_G

ClientSampleId :

SB-02-COMP


Tot Ion:178 Resp: 5665030

Ion Ratio Lower Upper

178 100

176 41.9 15.8 23.6#




179 33.9 12.8 19.2#



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



#71

Anthracene

Concen: 149.74 ng

RT: 17.12 min Scan# 2456

Delta R.T. 0.01 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11


Tgt Ion:178 Resp: 2476455

Ion Ratio Lower Upper

178 100

176 28.1 16.0 24.0#



179 22.9 12.9 19.3#




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E





#72

Carbazole

Concen: 52.42 ng

RT: 17.38 min Scan# 2501

Delta R.T. -0.00 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Instrument :

BNA_G

ClientSampleId :

SB-02-COMP


Tot Ion:167 Resp: 868486

Ion Ratio Lower Upper

167 100

166 23.4 18.4 27.6




139 14.1 11.1 16.7



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E



#74

Fluoranthene

Concen: 336.22 ng

RT: 19.08 min Scan# 2789

Delta R.T. 0.04 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11


Tgt Ion:202 Resp: 5923674

Ion Ratio Lower Upper

202 100

101 32.8 0.0 38.1



203 36.9 0.0 38.4




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E





#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.18 min Scan# 3148

Delta R.T. 0.02 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Instrument :

BNA_G

ClientSampleId :

SB-02-COMP


Tot Ion:240 Resp: 209821

Ion Ratio Lower Upper

240 100

120 20.2 16.3 24.5




236 27.1 21.1 31.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



#77

Pyrene

Concen: 356.56 ng

RT: 19.44 min Scan# 2851

Delta R.T. 0.04 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11


Tgt Ion:202 Resp: 5255942

Ion Ratio Lower Upper

202 100

200 42.7 18.0 27.0#



203 37.6 14.9 22.3#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E





#78

Terphenyl-d14

Concen: 18.68 ng

RT: 19.61 min Scan# 2880

Delta R.T. -0.00 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Instrument :

BNA_G

ClientSampleId :

SB-02-COMP


Tot Ion:244 Resp: 170139

Ion Ratio Lower Upper

244 100

212 7.5 6.4 9.6




122 15.9 15.9 23.9#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



#80

Benzo(a)anthracene

Concen: 266.24 ng m

RT: 21.17 min Scan# 3145

Delta R.T. 0.02 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11


Tgt Ion:228 Resp: 3387338

Ion Ratio Lower Upper

228 100

226 43.9 23.8 35.6#



229 32.0 17.0 25.4#




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E





#82

Chrysene

Concen: 271.59 ng/mL

RT: 21.23 min Scan# 3155

Delta R.T. 0.03 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Instrument :

BNA_G

ClientSampleId :

SB-02-COMP


Tot Ion:228 Resp: 3312685

Ion Ratio Lower Upper




228 100

226 45.5 25.4 38.0#

229 34.0 16.5 24.7#



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E



#85

Indeno(1,2,3-cd)pyrene

Concen: 169.06 ng/mL

RT: 25.66 min Scan# 3909

Delta R.T. 0.06 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11


Tgt Ion:276 Resp: 2247414

Ion Ratio Lower Upper



276 100


138 41.4 38.2 57.2

277 23.0 21.4 32.2



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E









#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.39 min Scan# 3523
Delta R.T. 0.03 min
Lab File: BG016773.D
Acq: 28 Apr 2015 20:11

Instrument :
BNA_G
ClientSampleId :
SB-02-COMP

Tot Ion:264 Resp: 249657




Ion	Ratio	Lower	Upper
264	100		
260	25.0	20.0	30.0
265	27.2	16.8	25.2#




#87
Benzo(b)fluoranthene
Concen: 273.57 ng
RT: 22.74 min Scan# 3413
Delta R.T. 0.04 min
Lab File: BG016773.D
Acq: 28 Apr 2015 20:11

Tgt Ion:252 Resp: 4148623

Ion	Ratio	Lower	Upper
252	100		
253	29.7	17.9	26.9#
125	28.4	15.8	23.8#





#88

Benzo(k)fluoranthene

Concen: 107.49 ng

RT: 22.78 min Scan# 3419

Delta R.T. 0.03 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11

Instrument :

BNA_G

ClientSampleId :

SB-02-COMP


Tot Ion:252 Resp: 1590739

Ion Ratio Lower Upper

252 100

253 28.6 17.6 26.4#




125 25.1 15.5 23.3#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#89

Benzo(a)pyrene

Concen: 224.53 ng

RT: 23.32 min Scan# 3511

Delta R.T. 0.05 min

Lab File: BG016773.D

Acq: 28 Apr 2015 20:11


Tgt Ion:252 Resp: 3208551

Ion Ratio Lower Upper

252 100

253 29.3 17.2 25.8#



125 27.0 16.3 24.5#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E









#90
Dibenzo(a,h)anthracene
Concen: 47.23 ng
RT: 25.64 min Scan# 3907
Delta R.T. 0.05 min
Lab File: BG016773.D
Acq: 28 Apr 2015 20:11

Instrument :
BNA_G
ClientSampleId :
SB-02-COMP

Tot Ion:278 Resp: 656265
Ion Ratio Lower Upper
278 100
139 0.0 24.2 36.2#
279 27.6 18.9 28.3



#91
Benzo(g,h,i)perylene
Concen: 141.45 ng
RT: 26.35 min Scan# 4027
Delta R.T. 0.08 min
Lab File: BG016773.D
Acq: 28 Apr 2015 20:11

Tgt Ion:276 Resp: 1999856
Ion Ratio Lower Upper
276 100
277 26.6 19.3 28.9
138 42.2 32.8 49.2

