

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
 Data File : BG016778.D
 Acq On : 28 Apr 2015 23:05
 Operator : TP/IZ
 Sample : G2022-04 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-04-COMP

Quant Time: Apr 29 01:59:12 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 29 00:55:31 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	71731	20.00	ng	0.00
21) Naphthalene-d8	10.35	136	300209	20.00	ng	0.00
38) Acenaphthene-d10	14.22	164	162692	20.00	ng	0.00
63) Phenanthrene-d10	16.97	188	298172	20.00	ng	0.00
75) Chrysene-d12	21.16	240	247470	20.00	ng	0.00
86) Perylene-d12	23.36	264	242605	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	223779	50.62	ng	0.00
7) Phenol-d6	6.76	99	304795	49.15	ng	0.00
23) Nitrobenzene-d5	8.73	82	158563	33.37	ng	0.00
41) 2,4,6-Tribromophenol	15.72	330	59954	49.67	ng	0.00
44) 2-Fluorobiphenyl	12.84	172	352899	34.85	ng	0.00
78) Terphenyl-d14	19.60	244	326086	30.35	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	10.40	128	166699	10.53	ng	96
37) 2-Methylnaphthalene	12.02	142	95676	8.37	ng	100
70) Phenanthrene	17.01	178	145009	8.47	ng	98
74) Fluoranthene	19.03	202	245005	13.50	ng	97
77) Pyrene	19.40	202	247102	14.21	ng	97
80) Benzo(a)anthracene	21.14	228	124856	8.32	ng	99
82) Chrysene	21.19	228	116686	8.11	ng	96
83) Bis(2-ethylhexyl)phthalate	21.08	149	155862	13.40	ng	100
85) Indeno(1,2,3-cd)pyrene	25.58	276	67989	4.34	ng	# 85
87) Benzo(b)fluoranthene	22.70	252	149685	10.16	ng	96
88) Benzo(k)fluoranthene	22.73	252	55523m	3.86	ng	
89) Benzo(a)pyrene	23.26	252	116636	8.40	ng	94
91) Benzo(a,h,i)perylene	26.27	276	62877	4.58	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
Data File : BG016778.D
Acq On : 28 Apr 2015 23:05
Operator : TP/IZ
Sample : G2022-04 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-04-COMP

Quant Time: Apr 29 01:59:12 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 29 00:55:31 2015
Response via : Initial Calibration

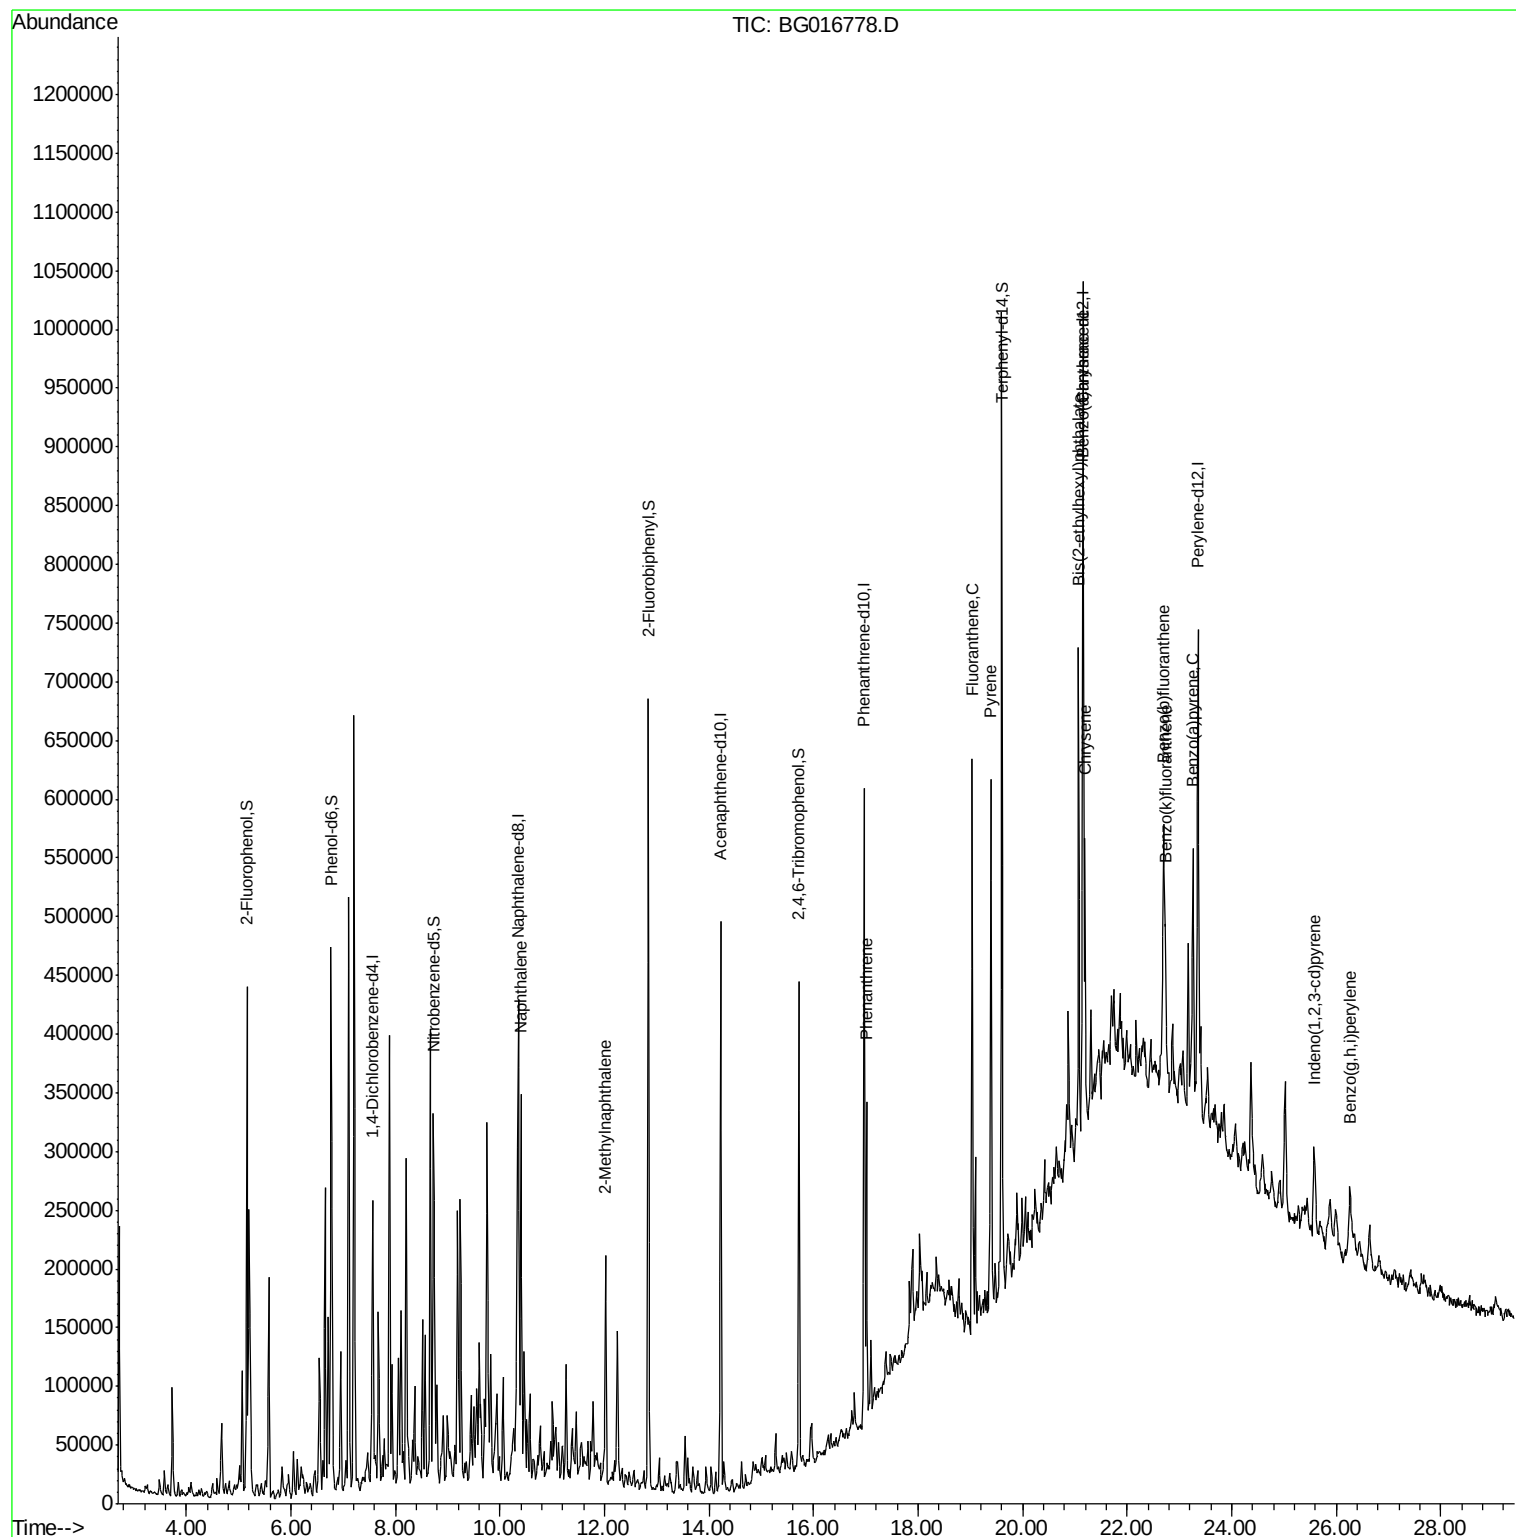



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.56 min Scan# 830

Delta R.T. -0.00 min

Lab File: BG016778.D

Acq: 28 Apr 2015 23:05

Instrument :

BNA_G

ClientSampleId :

SB-04-COMP


Tot Ion:152 Resp: 71731

Ion Ratio Lower Upper

152 100

150 150.0 129.6 194.4




115 53.1 43.0 64.6

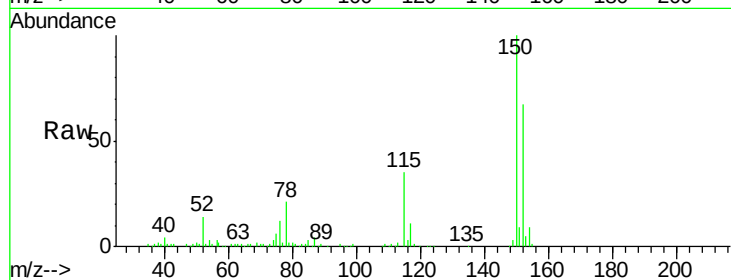

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

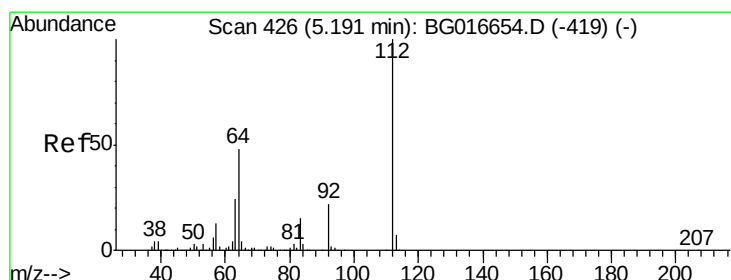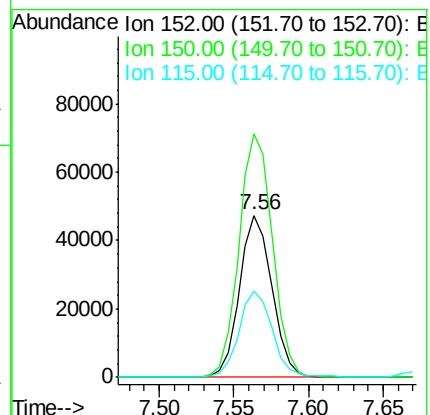

#5

2-Fluorophenol

Concen: 50.62 ng

RT: 5.16 min Scan# 421

Delta R.T. 0.00 min

Lab File: BG016778.D

Acq: 28 Apr 2015 23:05


Tgt Ion:112 Resp: 223779

Ion Ratio Lower Upper

112 100

64 44.3 38.3 57.5



63 21.6 18.9 28.3

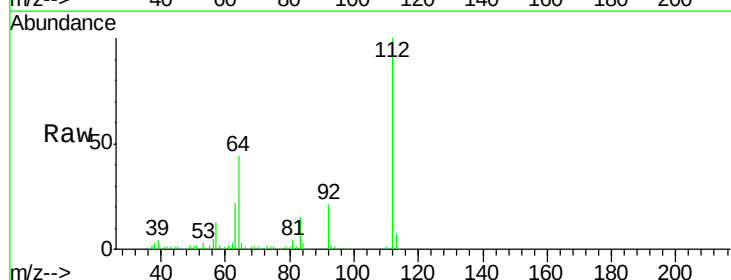


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

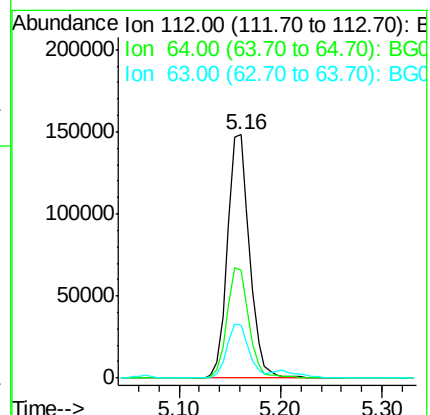



#7

Phenol-d6

Concen: 49.15 ng

RT: 6.76 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG016778.D

Acq: 28 Apr 2015 23:05

Instrument :

BNA_G

ClientSampleId :

SB-04-COMP


Tot Ion: 99 Resp: 304795

Ion Ratio Lower Upper




99 100

42 11.2 8.8 13.2

71 24.5 19.9 29.9

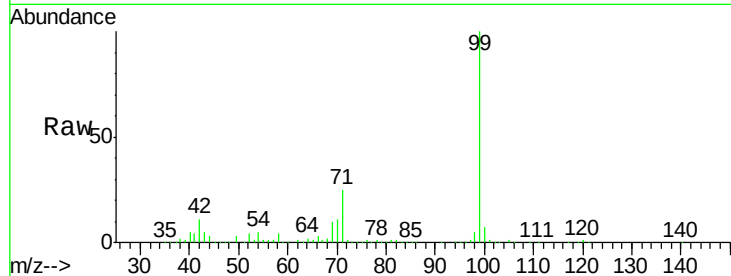

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

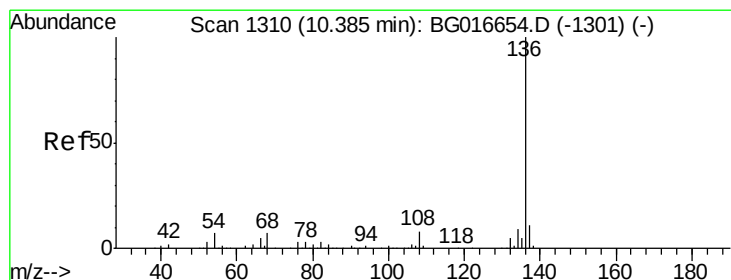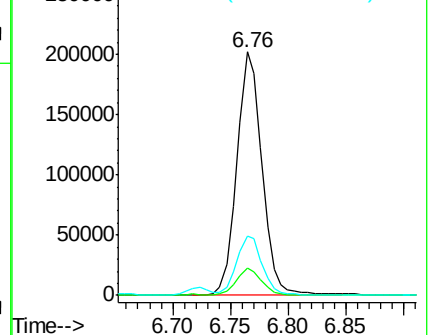

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.35 min Scan# 1304

Delta R.T. -0.00 min

Lab File: BG016778.D

Acq: 28 Apr 2015 23:05

Tgt Ion: 136 Resp: 300209


Ion Ratio Lower Upper

136 100



137 11.6 8.5 12.7


54 6.0 5.4 8.2

68 6.2 5.2 7.8



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




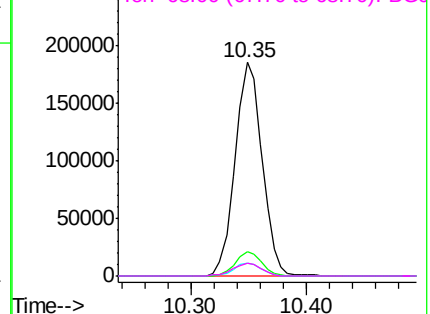




#23
 Nitrobenzene-d5
 Concen: 33.37 ng
 RT: 8.73 min Scan# 1028
 Delta R.T. -0.00 min
 Lab File: BG016778.D
 Acq: 28 Apr 2015 23:05




Instrument :
 BNA_G
 ClientSampleId :
 SB-04-COMP


Tot Ion: 82 Resp: 158563
 Ion Ratio Lower Upper
 82 100
 128 56.0 44.7 67.1
 54 36.5 30.9 46.3

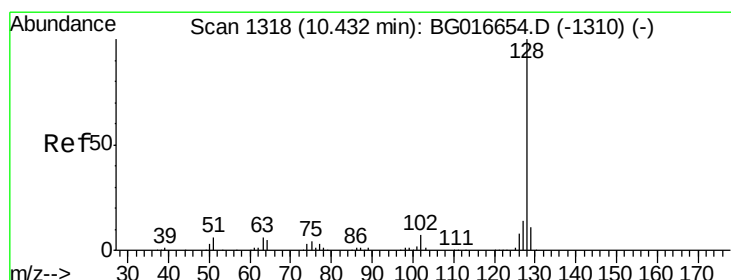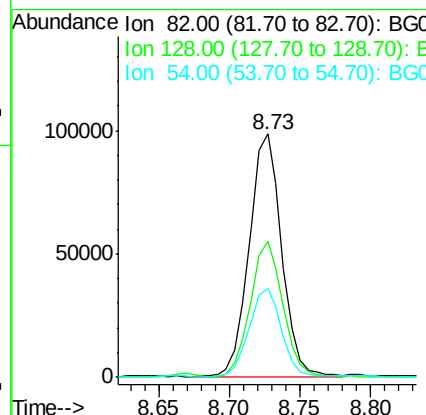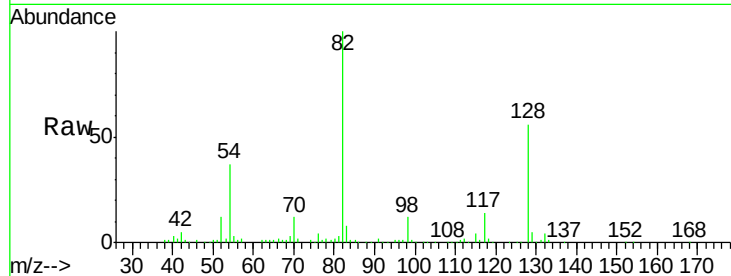

#31
 Naphthalene
 Concen: 10.53 ng
 RT: 10.40 min Scan# 1313
 Delta R.T. -0.00 min
 Lab File: BG016778.D
 Acq: 28 Apr 2015 23:05

Tgt Ion: 128 Resp: 166699
 Ion Ratio Lower Upper
 128 100
 129 13.5 9.0 13.6
 127 13.0 11.1 16.7


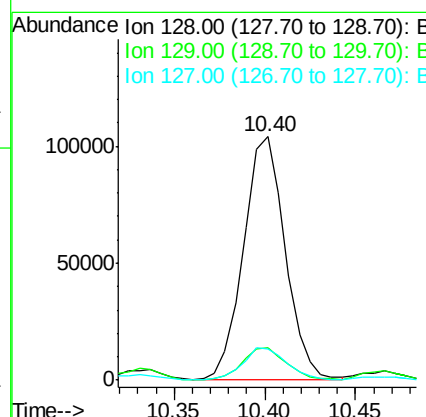




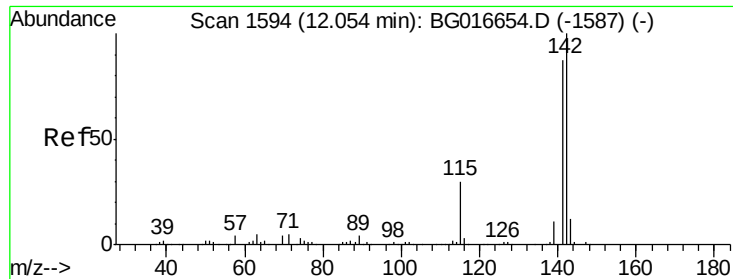

#37
2-Methylnaphthalene
Concen: 8.37 ng
RT: 12.02 min Scan# 1589
Delta R.T. -0.00 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05




Instrument :
BNA_G
ClientSampleId :
SB-04-COMP


Tot Ion:142 Resp: 95676
Ion Ratio Lower Upper
142 100
141 87.4 69.9 104.9
115 29.2 24.0 36.0

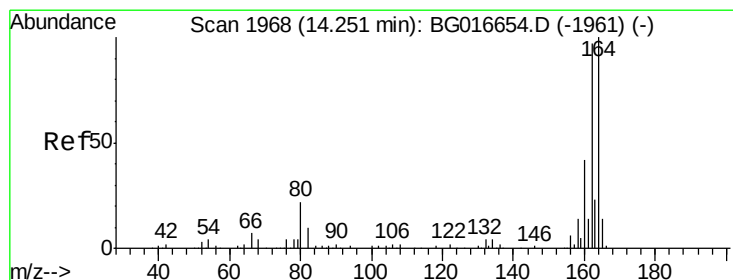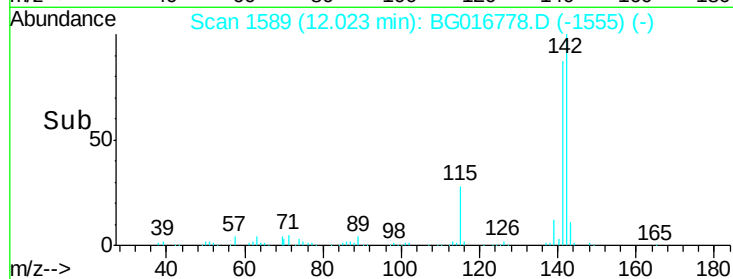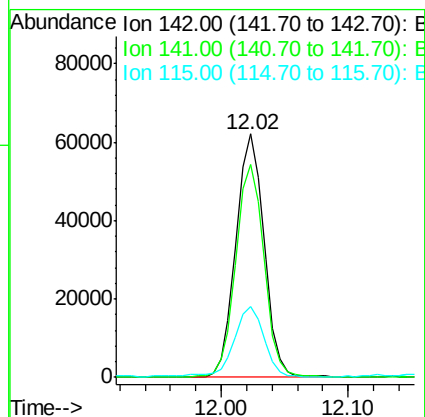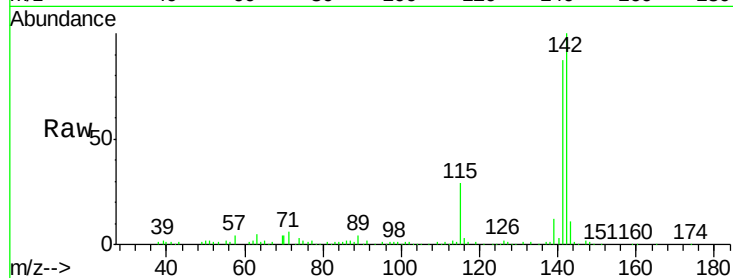

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.22 min Scan# 1963
Delta R.T. -0.01 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05

Tgt Ion:164 Resp: 162692
Ion Ratio Lower Upper
164 100
162 94.9 77.3 115.9
160 43.7 33.7 50.5

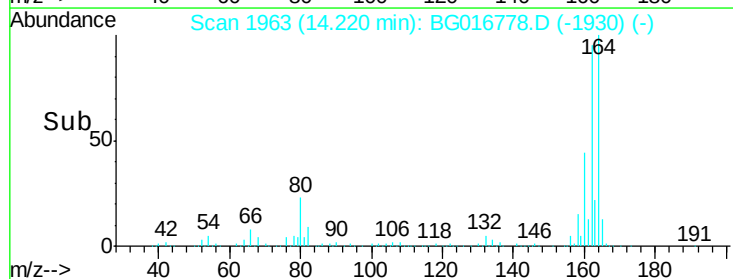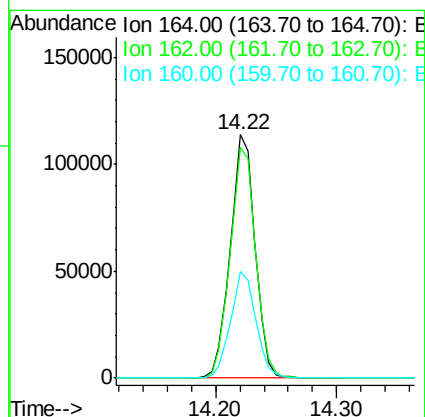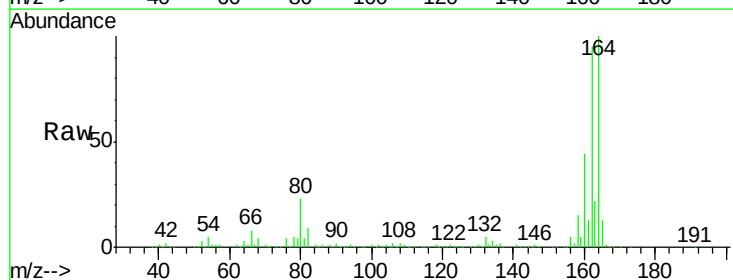


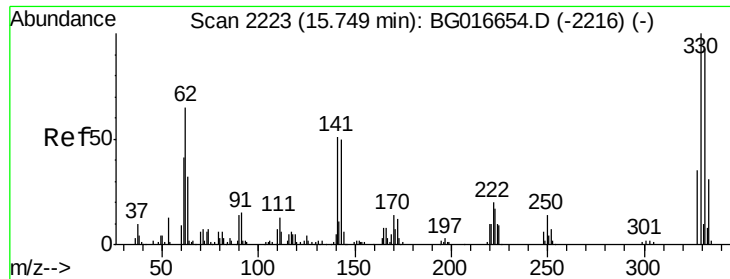




#41
 2,4,6-Tribromophenol
 Concen: 49.67 ng
 RT: 15.72 min Scan# 2218
 Delta R.T. -0.01 min
 Lab File: BG016778.D
 Acq: 28 Apr 2015 23:05

Instrument :
 BNA_G
 ClientSampleId :
 SB-04-COMP

Tot Ion:330 Resp: 59954
 Ion Ratio Lower Upper
 330 100
 332 96.3 76.2 114.4
 141 51.3 43.0 64.6

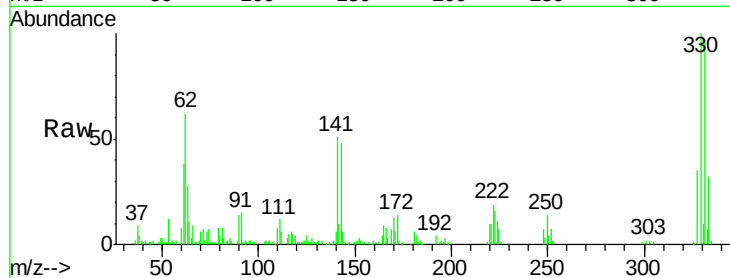


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

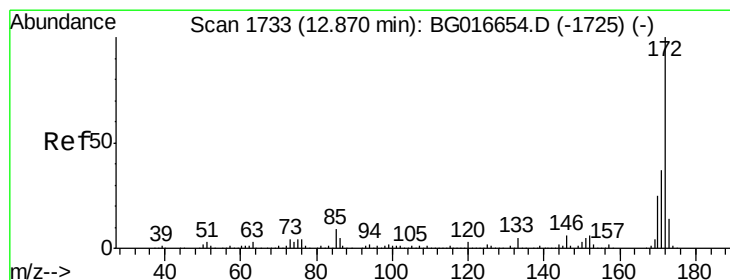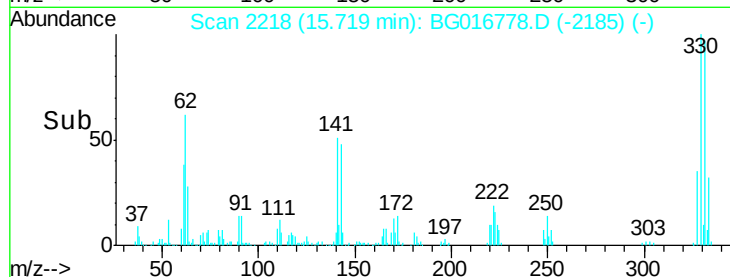
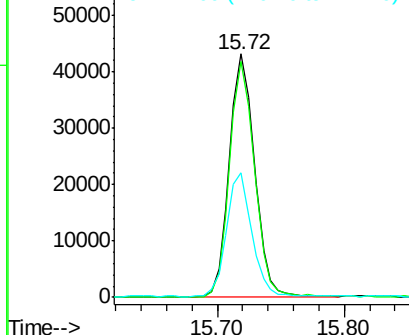



#44
 2-Fluorobiphenyl
 Concen: 34.85 ng
 RT: 12.84 min Scan# 1728
 Delta R.T. -0.00 min
 Lab File: BG016778.D
 Acq: 28 Apr 2015 23:05

Tgt Ion:172 Resp: 352899
 Ion Ratio Lower Upper
 172 100
 171 35.6 29.9 44.9
 170 24.2 19.8 29.8

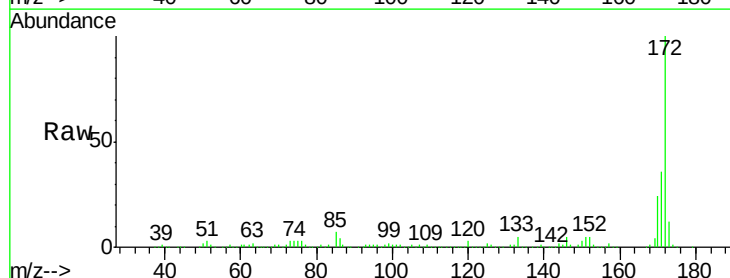

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



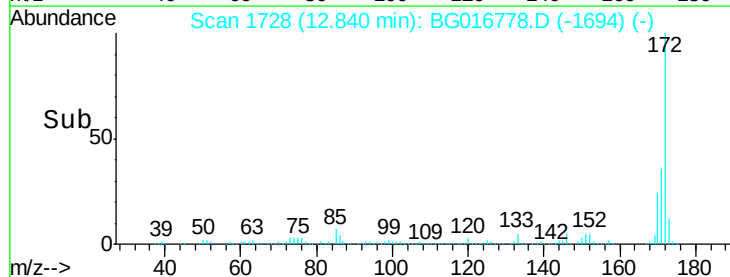
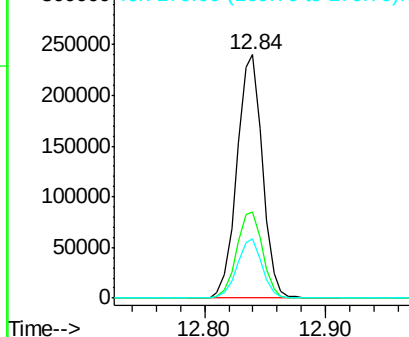




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.97 min Scan# 2431
Delta R.T. -0.00 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05




Instrument :
BNA_G
ClientSampleId :
SB-04-COMP


Tot Ion:188 Resp: 298172
Ion Ratio Lower Upper
188 100
94 11.6 10.7 16.1
80 11.5 9.9 14.9

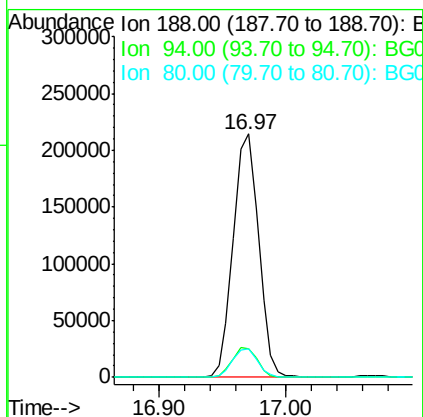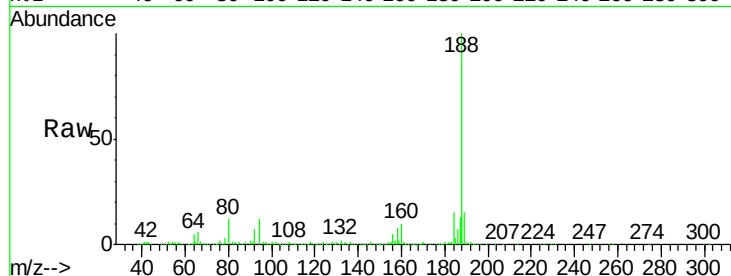

#70
Phenanthrene
Concen: 8.47 ng
RT: 17.01 min Scan# 2438
Delta R.T. -0.00 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05

Tgt Ion:178 Resp: 145009
Ion Ratio Lower Upper
178 100
176 20.4 15.8 23.6
179 15.2 12.8 19.2

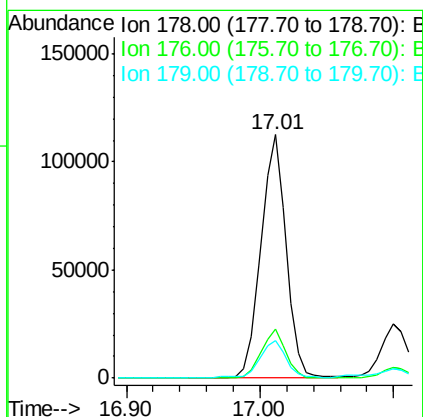



#74

Fluoranthene

Concen: 13.50 ng

RT: 19.03 min Scan# 2782

Delta R.T. -0.00 min

Lab File: BG016778.D

Acq: 28 Apr 2015 23:05


Instrument :

BNA_G




ClientSampleId :

SB-04-COMP

Tot Ion:	202	Resp:	245005
Ion	Ratio	Lower	Upper
202	100		
101	16.0	0.0	38.1
203	18.5	0.0	38.4

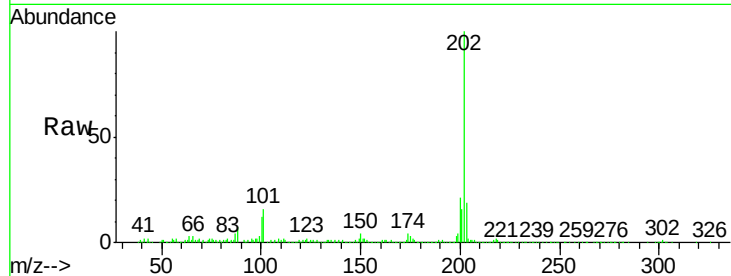

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

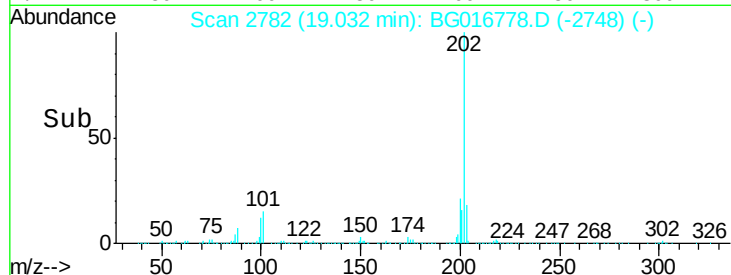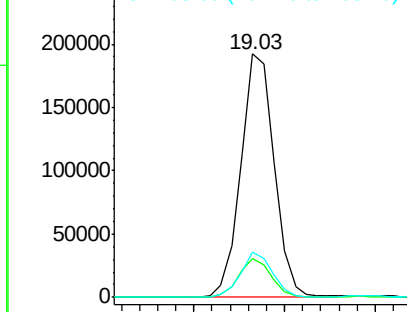

#75

Chrysene-d12

Concen: 20.00 ng


RT: 21.16 min Scan# 3144

Delta R.T. -0.00 min



Lab File: BG016778.D


Acq: 28 Apr 2015 23:05

Tgt Ion:	240	Resp:	247470
Ion	Ratio	Lower	Upper
240	100		
120	20.0	16.3	24.5
236	27.8	21.1	31.7



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E




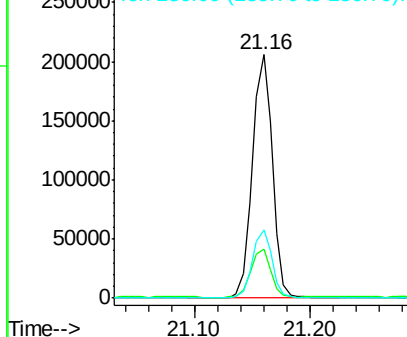


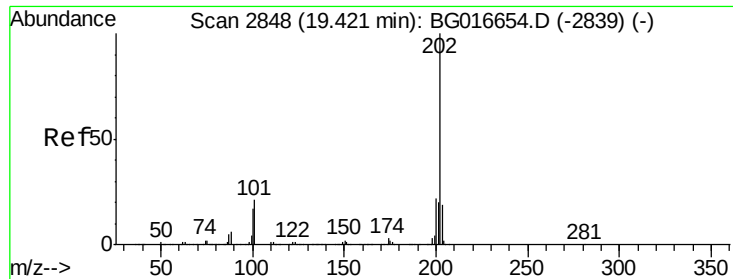

#77
Pvrene
Concen: 14.21 ng
RT: 19.40 min Scan# 2844
Delta R.T. -0.00 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05




Instrument :
BNA_G
ClientSampleId :
SB-04-COMP


Tot Ion	Ratio	Lower	Upper
202	100		
200	20.4	18.0	27.0
203	17.7	14.9	22.3

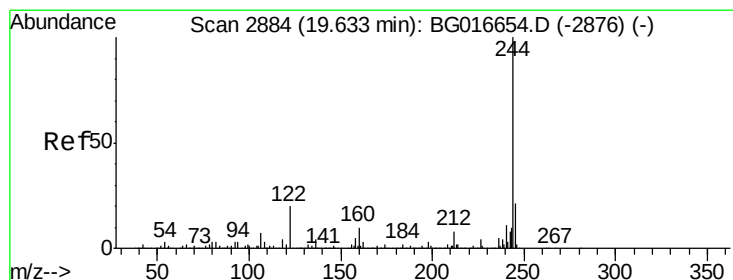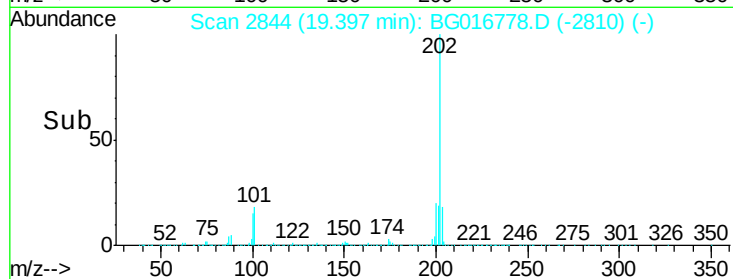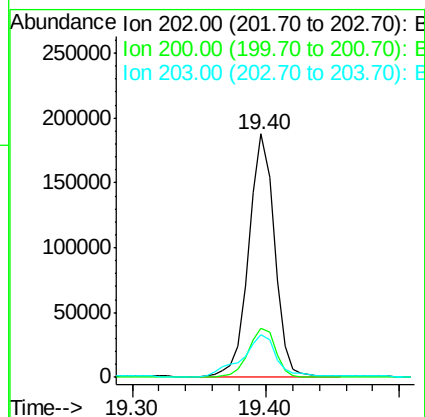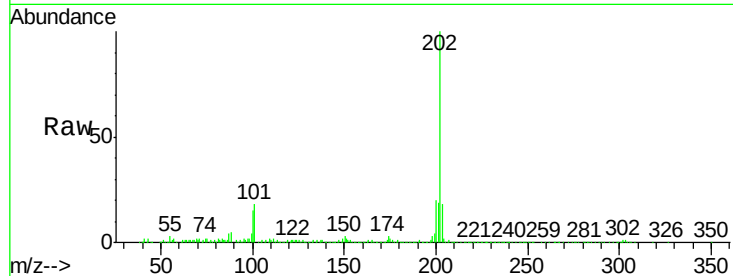

#78
Terphenyl-d14
Concen: 30.35 ng
RT: 19.60 min Scan# 2879
Delta R.T. -0.01 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.6	6.4	9.6
122	19.1	15.9	23.9


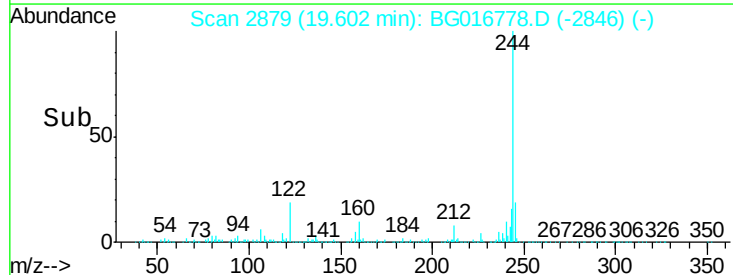
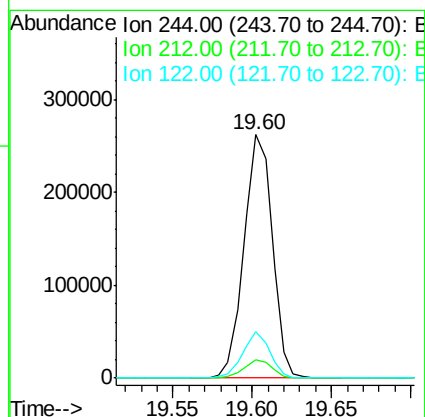
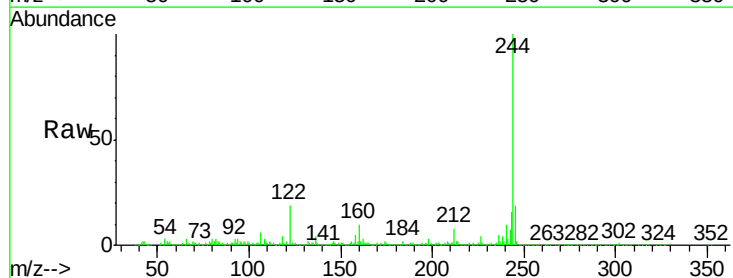


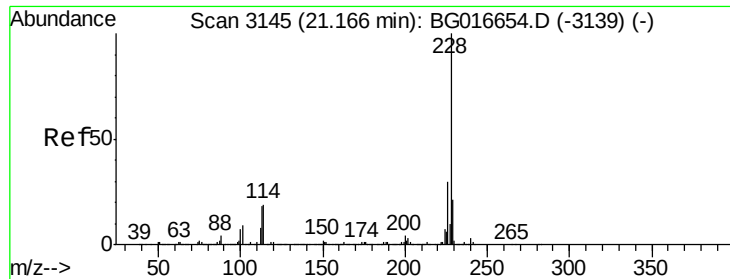

#80
Benzo(a)anthracene
Concen: 8.32 ng
RT: 21.14 min Scan# 3141
Delta R.T. -0.00 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05




Instrument :
BNA_G
ClientSampleId :
SB-04-COMP


Tot Ion	Ratio	Lower	Upper
228	100		
226	29.0	23.8	35.6
229	21.4	17.0	25.4

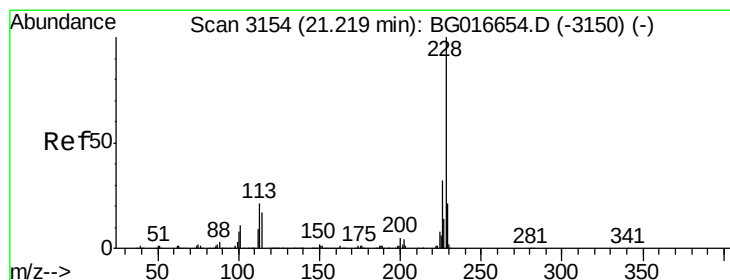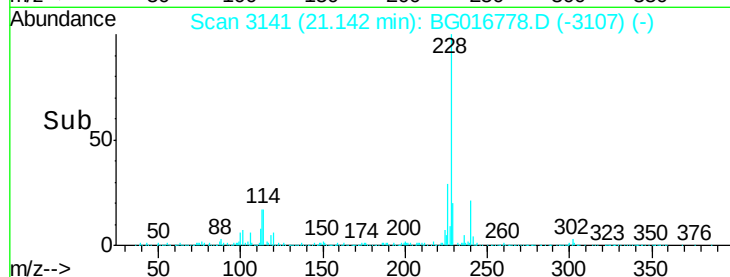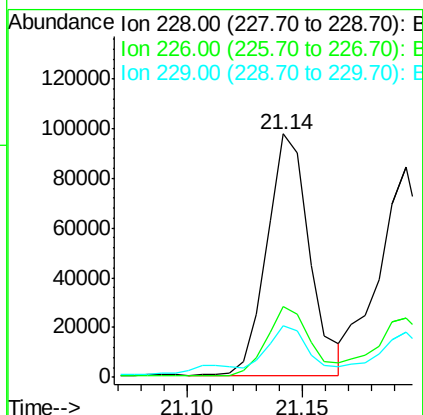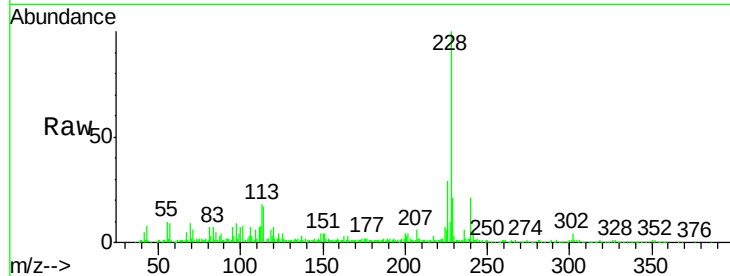

#82
Chrysene
Concen: 8.11 ng
RT: 21.19 min Scan# 3150
Delta R.T. -0.00 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.5	25.4	38.0
229	21.4	16.5	24.7


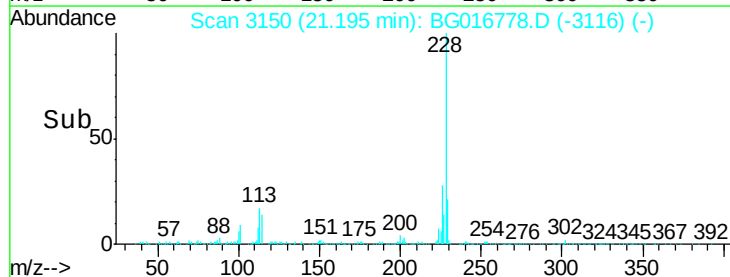
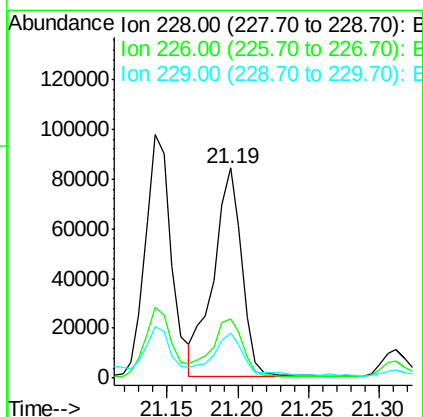
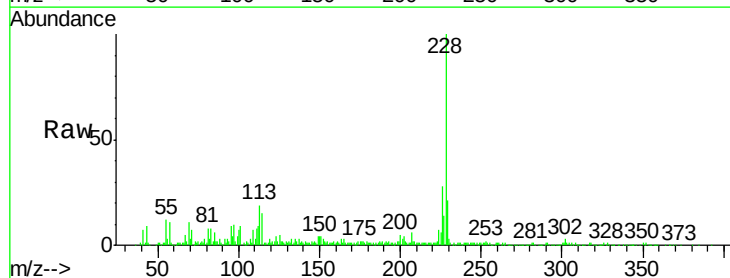




#83
 Bis(2-ethylhexyl)phthalate
 Concen: 13.40 ng
 RT: 21.08 min Scan# 3130
 Delta R.T. 0.00 min
 Lab File: BG016778.D
 Acq: 28 Apr 2015 23:05




Instrument :
 BNA_G
 ClientSampleId :
 SB-04-COMP


Tot Ion:149 Resp: 155862
 Ion Ratio Lower Upper
 149 100
 167 33.0 26.6 39.8
 279 6.5 5.1 7.7

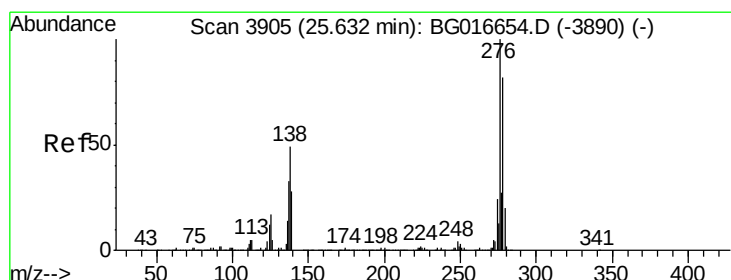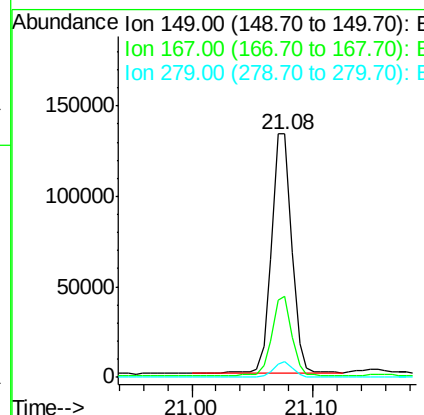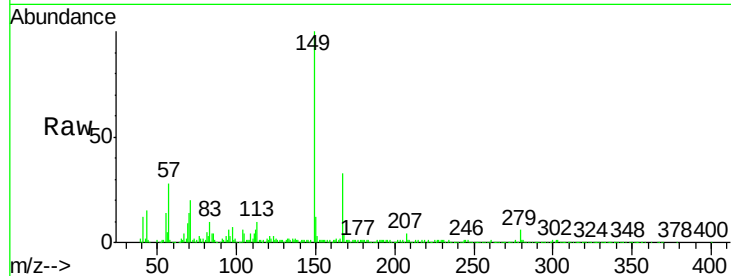

#85
 Indeno(1,2,3-cd)pyrene
 Concen: 4.34 ng
 RT: 25.58 min Scan# 3896
 Delta R.T. -0.01 min
 Lab File: BG016778.D
 Acq: 28 Apr 2015 23:05

Tgt Ion:276 Resp: 67989
 Ion Ratio Lower Upper
 276 100
 138 35.7 38.2 57.2#
 277 21.6 21.4 32.2



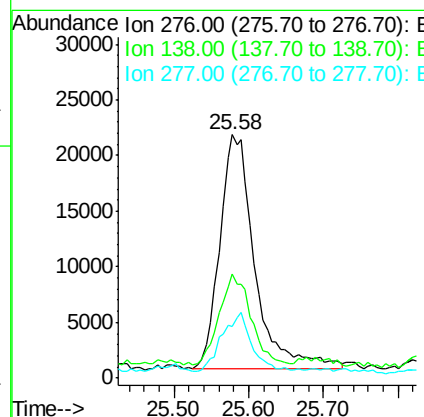





#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.36 min Scan# 3518
Delta R.T. 0.00 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05




Instrument :
BNA_G
ClientSampleId :
SB-04-COMP


Tot Ion	Ratio	Lower	Upper
264	100		
260	24.8	20.0	30.0
265	22.8	16.8	25.2

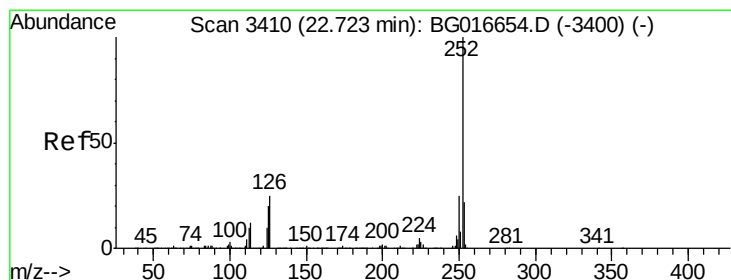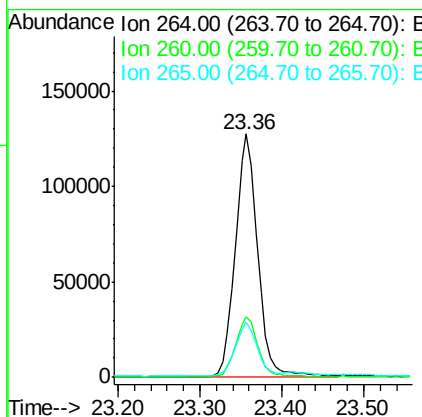

#87
Benzo(b)fluoranthene
Concen: 10.16 ng
RT: 22.70 min Scan# 3406
Delta R.T. -0.00 min
Lab File: BG016778.D
Acq: 28 Apr 2015 23:05

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.0	17.9	26.9
125	22.8	15.8	23.8

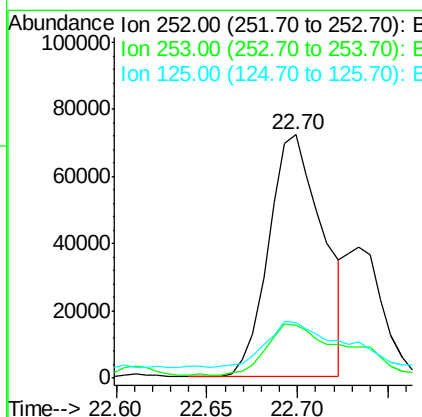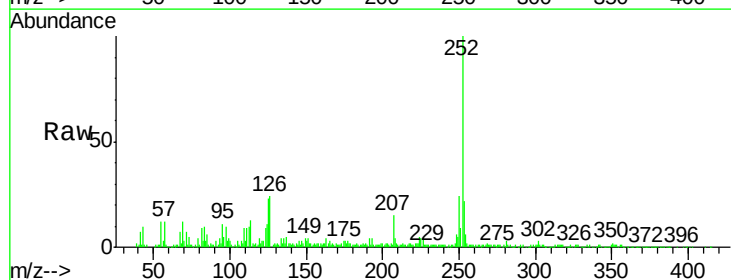



#88

Benzo(k)fluoranthene

Concen: 3.86 ng

RT: 22.73 min Scan# 3412

Delta R.T. -0.01 min

Lab File: BG016778.D

Acq: 28 Apr 2015 23:05

Instrument :

BNA_G

ClientSampleId :

SB-04-COMP


Tot Ion:252 Resp: 55523

Ion Ratio Lower Upper




252 100

253 23.9 17.6 26.4

125 27.7 15.5 23.3#

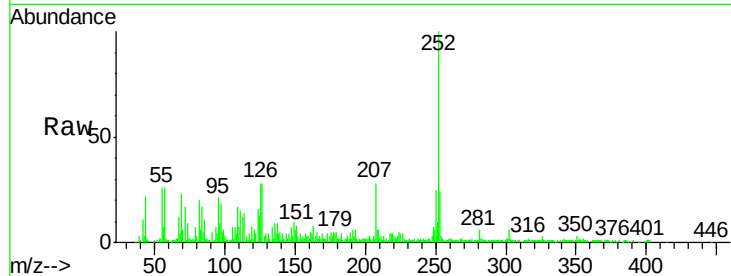

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

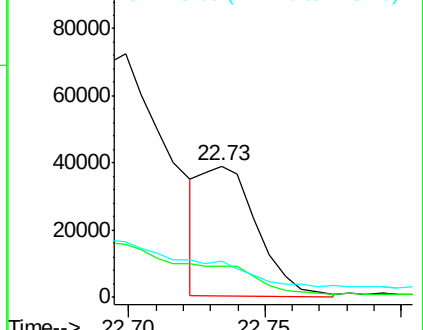

#89

Benzo(a)pyrene

Concen: 8.40 ng

RT: 23.26 min Scan# 3502

Delta R.T. -0.00 min

Lab File: BG016778.D

Acq: 28 Apr 2015 23:05


Tgt Ion:252 Resp: 116636

Ion Ratio Lower Upper



252 100


253 23.7 17.2 25.8

125 23.4 16.3 24.5



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

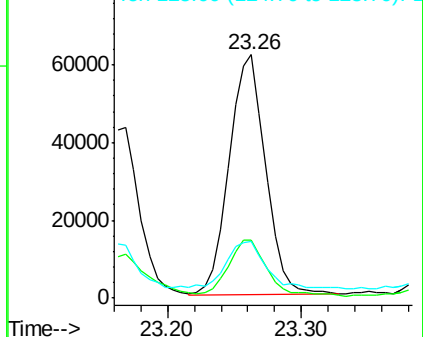



#91
 Benzo(a,h,i)perylene
 Concen: 4.58 ng
 RT: 26.27 min Scan# 4013
 Delta R.T. -0.01 min
 Lab File: BG016778.D
 Acq: 28 Apr 2015 23:05

Instrument :
 BNA_G
 ClientSampleId :
 SB-04-COMP

Tot Ion	Ratio	Lower	Upper
276	100		
277	25.9	19.3	28.9
138	44.1	32.8	49.2

