

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
 Data File : BG016767.D
 Acq On : 28 Apr 2015 16:40
 Operator : TP/IZ
 Sample : G2024-10 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-05-0-2.0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.671	333	337	345	rVB	17321	25919	2.82%	0.365%
2	5.158	412	420	429	rBV	133744	207550	22.55%	2.924%
3	6.768	688	694	705	rBV	132540	231415	25.14%	3.260%
4	7.103	743	751	761	rBV	155315	245488	26.67%	3.459%
5	7.567	823	830	837	rBV	219933	344428	37.42%	4.853%
6	7.884	877	884	891	rBV	118953	193959	21.07%	2.733%
7	8.725	1021	1027	1037	rBV	74174	134768	14.64%	1.899%
8	10.352	1295	1304	1320	rBV	313853	539652	58.63%	7.603%
9	12.837	1718	1727	1739	rBV	223849	350552	38.09%	4.939%
10	14.224	1956	1963	1970	rBV2	488471	717585	77.96%	10.110%
11	14.453	1996	2002	2009	rVB5	10498	20072	2.18%	0.283%
12	15.722	2212	2218	2224	rBV	118613	178118	19.35%	2.509%
13	15.957	2252	2258	2263	rVB8	9856	20687	2.25%	0.291%
14	16.427	2334	2338	2341	rBV	40603	54668	5.94%	0.770%
15	16.463	2341	2344	2348	rVB	37276	41441	4.50%	0.584%
16	16.786	2396	2399	2403	rVB4	12580	17860	1.94%	0.252%
17	16.968	2424	2430	2434	rBV2	555326	767131	83.34%	10.808%
18	17.009	2434	2437	2442	rVB	99511	135723	14.75%	1.912%
19	17.103	2449	2453	2457	rVB	25671	31892	3.46%	0.449%
20	17.843	2576	2579	2582	rBV2	15056	19417	2.11%	0.274%
21	17.890	2584	2587	2592	rVB2	31179	47037	5.11%	0.663%
22	18.037	2608	2612	2615	rBV4	27508	39819	4.33%	0.561%
23	18.349	2663	2665	2670	rVB3	17682	18650	2.03%	0.263%
24	19.030	2777	2781	2786	rBV	228746	311573	33.85%	4.390%
25	19.394	2839	2843	2848	rVB	237387	294885	32.04%	4.155%
26	19.600	2874	2878	2883	rVB	319268	370816	40.29%	5.224%
27	21.157	3139	3143	3147	rBV2	656018	816386	88.70%	11.502%
28	23.360	3515	3518	3533	rVB2	474019	920439	100.00%	12.968%


Sum of corrected areas: 7097930

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
Data File : BG016767.D
Acq On : 28 Apr 2015 16:40
Operator : TP/IZ
Sample : G2024-10 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-05-0-2.0

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

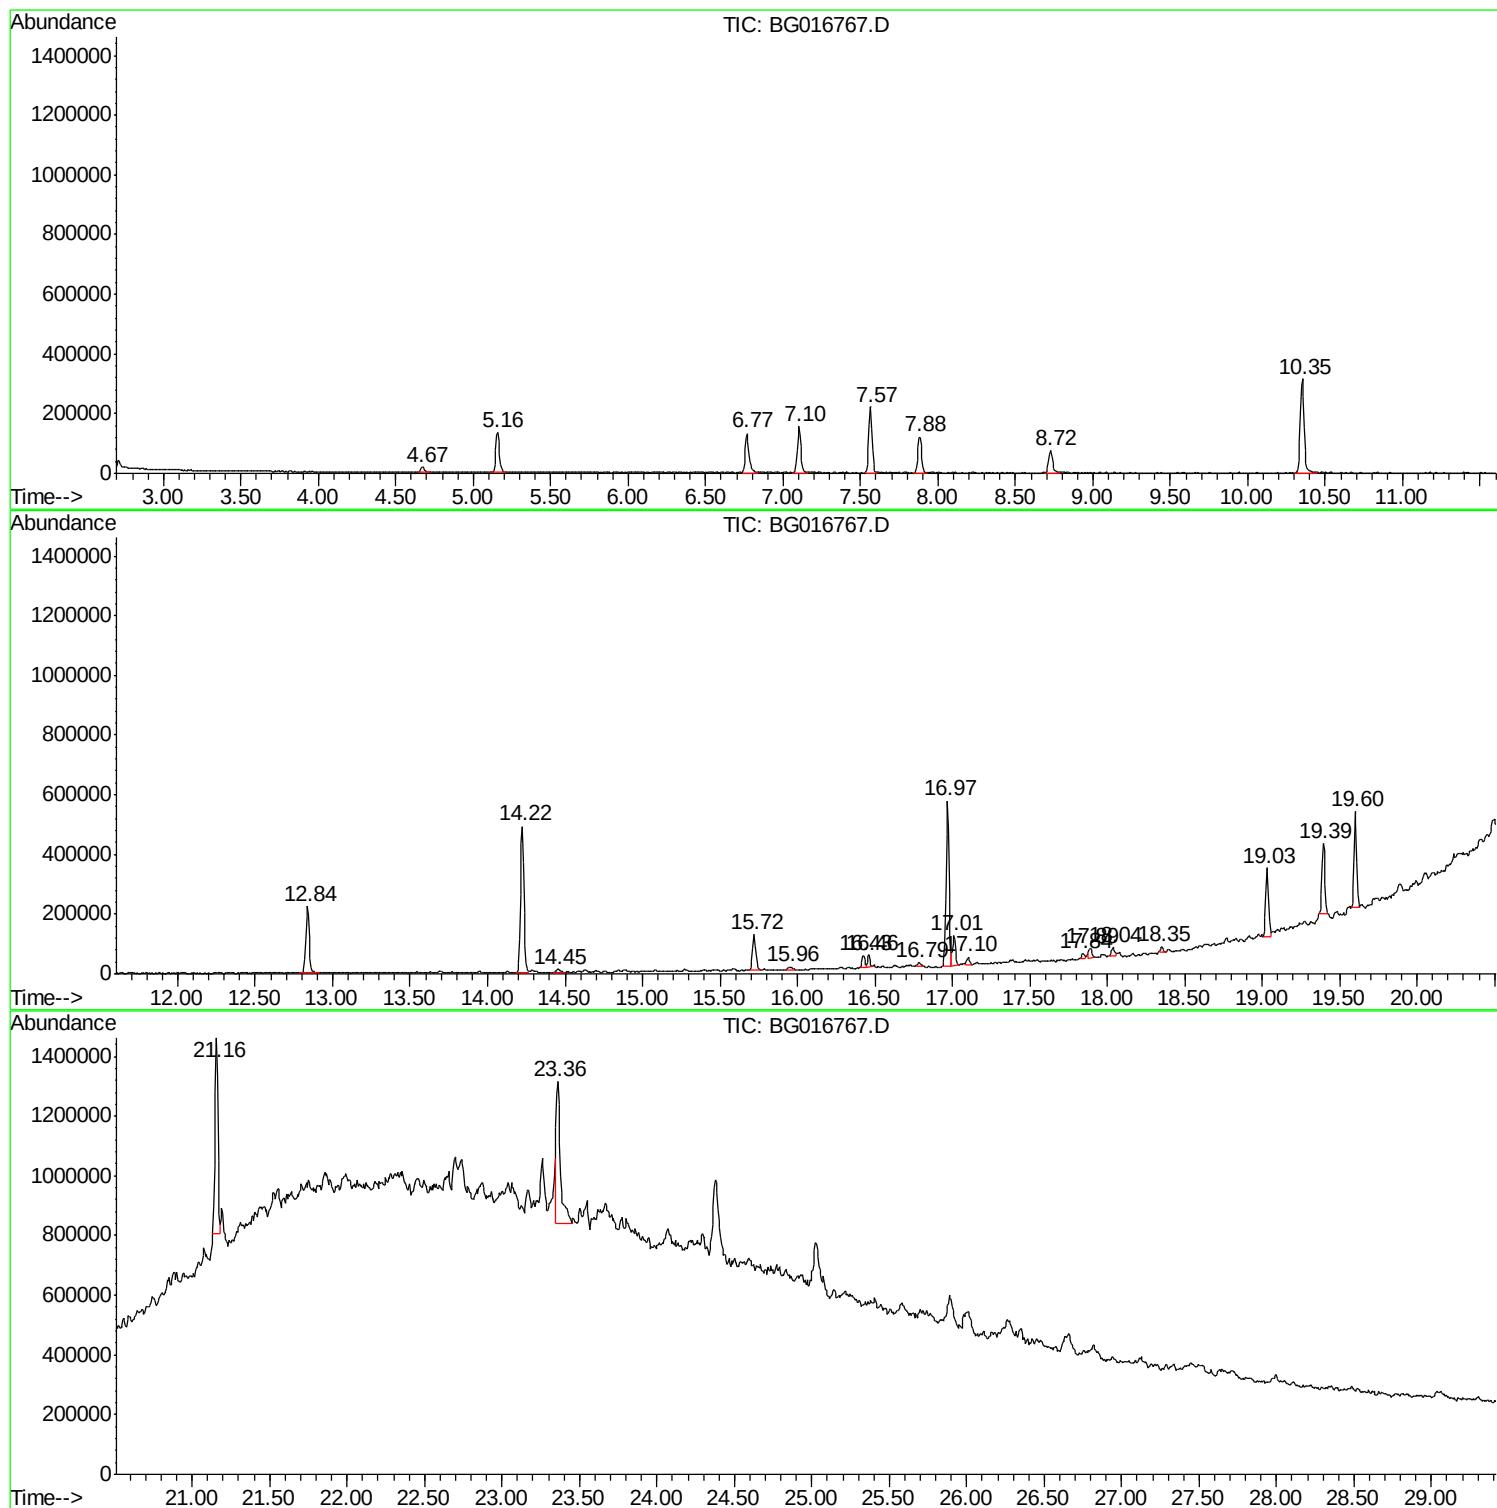

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
Data File : BG016767.D
Acq On : 28 Apr 2015 16:40
Operator : TP/IZ
Sample : G2024-10 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-05-0-2.0










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.10 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.10	14.25 ng	245488	1,4-Dichlorobenzene-d4	7.56

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		Xenon	132	Xe	007440-63-3	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

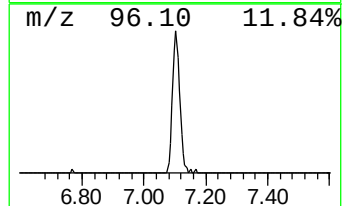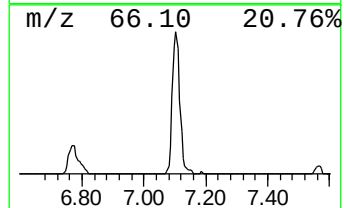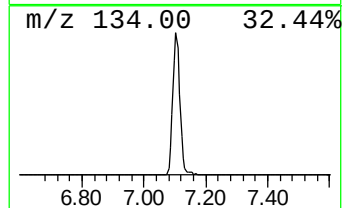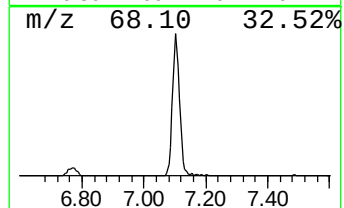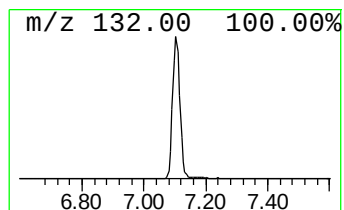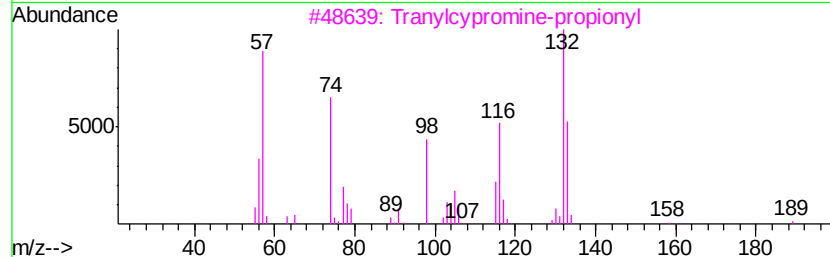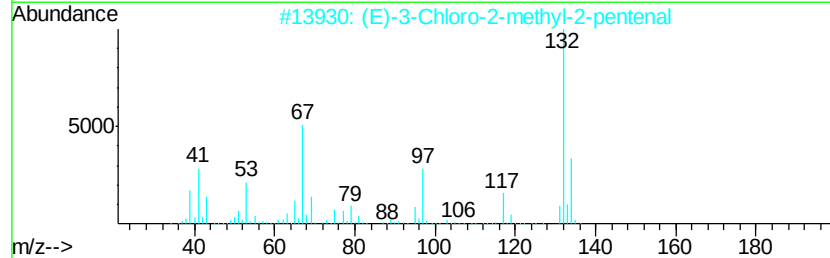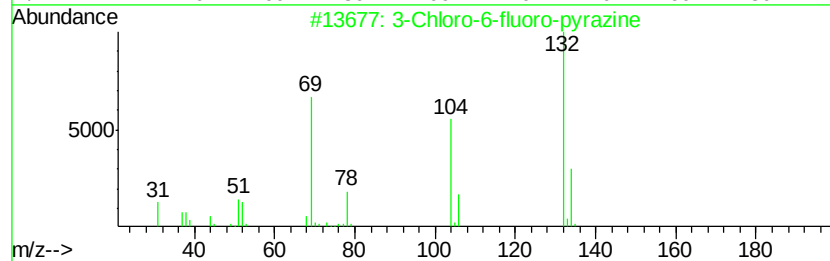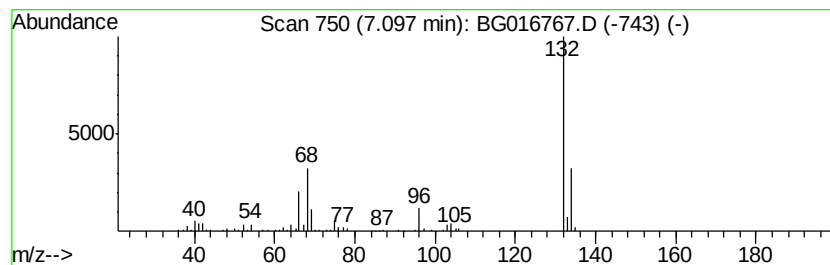

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042815\
Data File : BG016767.D
Acq On : 28 Apr 2015 16:40
Operator : TP/IZ
Sample : G2024-10 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-05-0-2.0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.10	7.10	14.3	ng	245488	1	7.56	344428	20.0