

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
 Data File : BG016770.D
 Acq On : 28 Apr 2015 18:26
 Operator : TP/IZ
 Sample : G1991-13DL 25X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-63SDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.160	416	421	428	rBV2	31004	48355	2.01%	0.211%
2	6.770	690	695	707	rBV	25168	50336	2.09%	0.220%
3	7.105	747	752	761	rBV	33519	55076	2.29%	0.241%
4	7.563	822	830	839	rBV	227943	361701	15.03%	1.582%
5	7.881	877	884	891	rBV	28524	46425	1.93%	0.203%
6	8.733	1024	1029	1035	rBV	16225	28452	1.18%	0.124%
7	10.348	1297	1304	1310	rBV	337364	563423	23.41%	2.464%
8	10.395	1310	1312	1320	rVB	20328	32078	1.33%	0.140%
9	12.840	1721	1728	1740	rBV	48483	77059	3.20%	0.337%
10	14.220	1956	1963	1970	rBV2	497819	737950	30.66%	3.227%
11	14.285	1970	1974	1983	rVB	69349	101212	4.21%	0.443%
12	14.626	2027	2032	2038	rBV	44817	64730	2.69%	0.283%
13	15.272	2137	2142	2155	rBV	63419	99423	4.13%	0.435%
14	15.572	2188	2193	2199	rVB	24728	36956	1.54%	0.162%
15	15.724	2209	2219	2228	rBV3	47644	86576	3.60%	0.379%
16	16.277	2303	2313	2319	rBV4	18116	49991	2.08%	0.219%
17	16.506	2343	2352	2355	rBV5	18559	32685	1.36%	0.143%
18	16.629	2369	2373	2381	rVB	30100	45741	1.90%	0.200%
19	16.723	2381	2389	2393	rVV5	30092	67141	2.79%	0.294%
20	16.788	2396	2400	2409	rVB	59782	87164	3.62%	0.381%
21	16.970	2425	2431	2434	rBV	555077	771430	32.05%	3.373%
22	17.011	2434	2438	2445	rVV	1172197	1551177	64.45%	6.783%
23	17.099	2445	2453	2459	rVV	252724	366495	15.23%	1.603%
24	17.164	2459	2464	2470	rVB2	22231	39187	1.63%	0.171%
25	17.352	2490	2496	2497	rBV	19957	26886	1.12%	0.118%
26	17.381	2497	2501	2515	rVV	78204	142007	5.90%	0.621%
27	17.487	2515	2519	2525	rVV3	28497	41526	1.73%	0.182%
28	17.552	2525	2530	2538	rVV7	20148	36488	1.52%	0.160%
29	17.846	2571	2580	2584	rBV	130901	211910	8.80%	0.927%
30	17.893	2584	2588	2594	rVB	206975	274640	11.41%	1.201%
31	17.969	2594	2601	2607	rBV	85162	122722	5.10%	0.537%
32	18.039	2607	2613	2617	rVV2	178066	332788	13.83%	1.455%
33	18.075	2617	2619	2628	rVB	103014	120053	4.99%	0.525%
34	18.157	2628	2633	2636	rBV3	17617	24842	1.03%	0.109%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
 Data File : BG016770.D
 Acq On : 28 Apr 2015 18:26
 Operator : TP/IZ
 Sample : G1991-13DL 25X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-63SDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	18.351	2661	2666	2670	rVV	126315	170210	7.07%	0.744%
36	18.392	2670	2673	2678	rVB	56255	75639	3.14%	0.331%
37	18.598	2704	2708	2713	rVB	36003	43946	1.83%	0.192%
38	18.645	2713	2716	2720	rVV	26167	31482	1.31%	0.138%
39	18.686	2720	2723	2728	rVB	33629	40971	1.70%	0.179%
40	18.768	2728	2737	2741	rBV	71048	135779	5.64%	0.594%
41	18.833	2743	2748	2751	rVV4	51185	95051	3.95%	0.416%
42	18.862	2751	2753	2756	rVV	37492	39954	1.66%	0.175%
43	18.915	2756	2762	2770	rVB3	64563	131481	5.46%	0.575%
44	19.038	2776	2783	2790	rBV	1810215	2406877	100.00%	10.525%
45	19.097	2790	2793	2796	rVV	26688	30834	1.28%	0.135%
46	19.132	2796	2799	2804	rVB	44597	55550	2.31%	0.243%
47	19.232	2811	2816	2819	rBV5	23233	49856	2.07%	0.218%
48	19.279	2820	2824	2828	rVB	62111	84729	3.52%	0.371%
49	19.367	2834	2839	2840	rBV	303921	345294	14.35%	1.510%
50	19.397	2840	2844	2852	rVV	1595912	2187803	90.90%	9.567%
51	19.467	2852	2856	2864	rVB2	84908	134681	5.60%	0.589%
52	19.579	2870	2875	2877	rBV	94507	131835	5.48%	0.577%
53	19.602	2877	2879	2882	rVV	81064	89179	3.71%	0.390%
54	19.643	2882	2886	2891	rVB	77235	111699	4.64%	0.488%
55	19.732	2894	2901	2907	rBV4	97033	251946	10.47%	1.102%
56	19.855	2917	2922	2924	rBV3	78717	113925	4.73%	0.498%
57	19.896	2925	2929	2933	rVB	148856	216176	8.98%	0.945%
58	19.996	2942	2946	2949	rVV2	76443	92211	3.83%	0.403%
59	20.055	2949	2956	2959	rVV2	139264	239695	9.96%	1.048%
60	20.090	2959	2962	2966	rVB2	35325	46908	1.95%	0.205%
61	20.131	2966	2969	2973	rVB3	30113	39467	1.64%	0.173%
62	20.190	2975	2979	2983	rBV	66490	88746	3.69%	0.388%
63	20.237	2983	2987	2991	rVV	83362	107315	4.46%	0.469%
64	20.448	3019	3023	3027	rBV4	21030	44483	1.85%	0.195%
65	20.601	3045	3049	3052	rBV6	22257	36640	1.52%	0.160%
66	20.642	3052	3056	3062	rVB	115605	158208	6.57%	0.692%
67	20.807	3079	3084	3087	rBV2	92137	137175	5.70%	0.600%
68	20.842	3087	3090	3094	rVV	132274	151017	6.27%	0.660%
69	20.883	3094	3097	3102	rVV2	95184	166305	6.91%	0.727%
70	20.936	3102	3106	3114	rVB2	101250	168189	6.99%	0.735%
71	21.153	3133	3143	3147	rBV2	924184	1982462	82.37%	8.669%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
Data File : BG016770.D
Acq On : 28 Apr 2015 18:26
Operator : TP/IZ
Sample : G1991-13DL 25X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-63SDL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	21.195	3147	3150	3160	rVB	677785	875257	36.36%	3.827%
73	21.312	3166	3170	3176	rBV	81235	115009	4.78%	0.503%
74	21.471	3192	3197	3201	rBV3	71589	121931	5.07%	0.533%
75	21.694	3232	3235	3239	rVB	106122	138910	5.77%	0.607%
76	21.747	3242	3244	3251	rVB	60013	73227	3.04%	0.320%
77	21.888	3265	3268	3271	rBV2	45594	66069	2.75%	0.289%
78	22.699	3400	3406	3411	rBV	452043	1051253	43.68%	4.597%
79	22.863	3430	3434	3438	rVB	77662	116562	4.84%	0.510%
80	23.163	3480	3485	3493	rVB	269285	515819	21.43%	2.256%
81	23.257	3495	3501	3508	rVV	425699	739677	30.73%	3.235%
82	23.357	3511	3518	3522	rVV	433855	800875	33.27%	3.502%
83	23.404	3523	3526	3535	rVB2	120340	222405	9.24%	0.973%
84	25.578	3889	3896	3906	rVB	183312	492881	20.48%	2.155%
85	26.265	4006	4013	4025	rVB	122375	369853	15.37%	1.617%


Sum of corrected areas: 22868071

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
Data File : BG016770.D
Acq On : 28 Apr 2015 18:26
Operator : TP/IZ
Sample : G1991-13DL 25X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-63SDL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

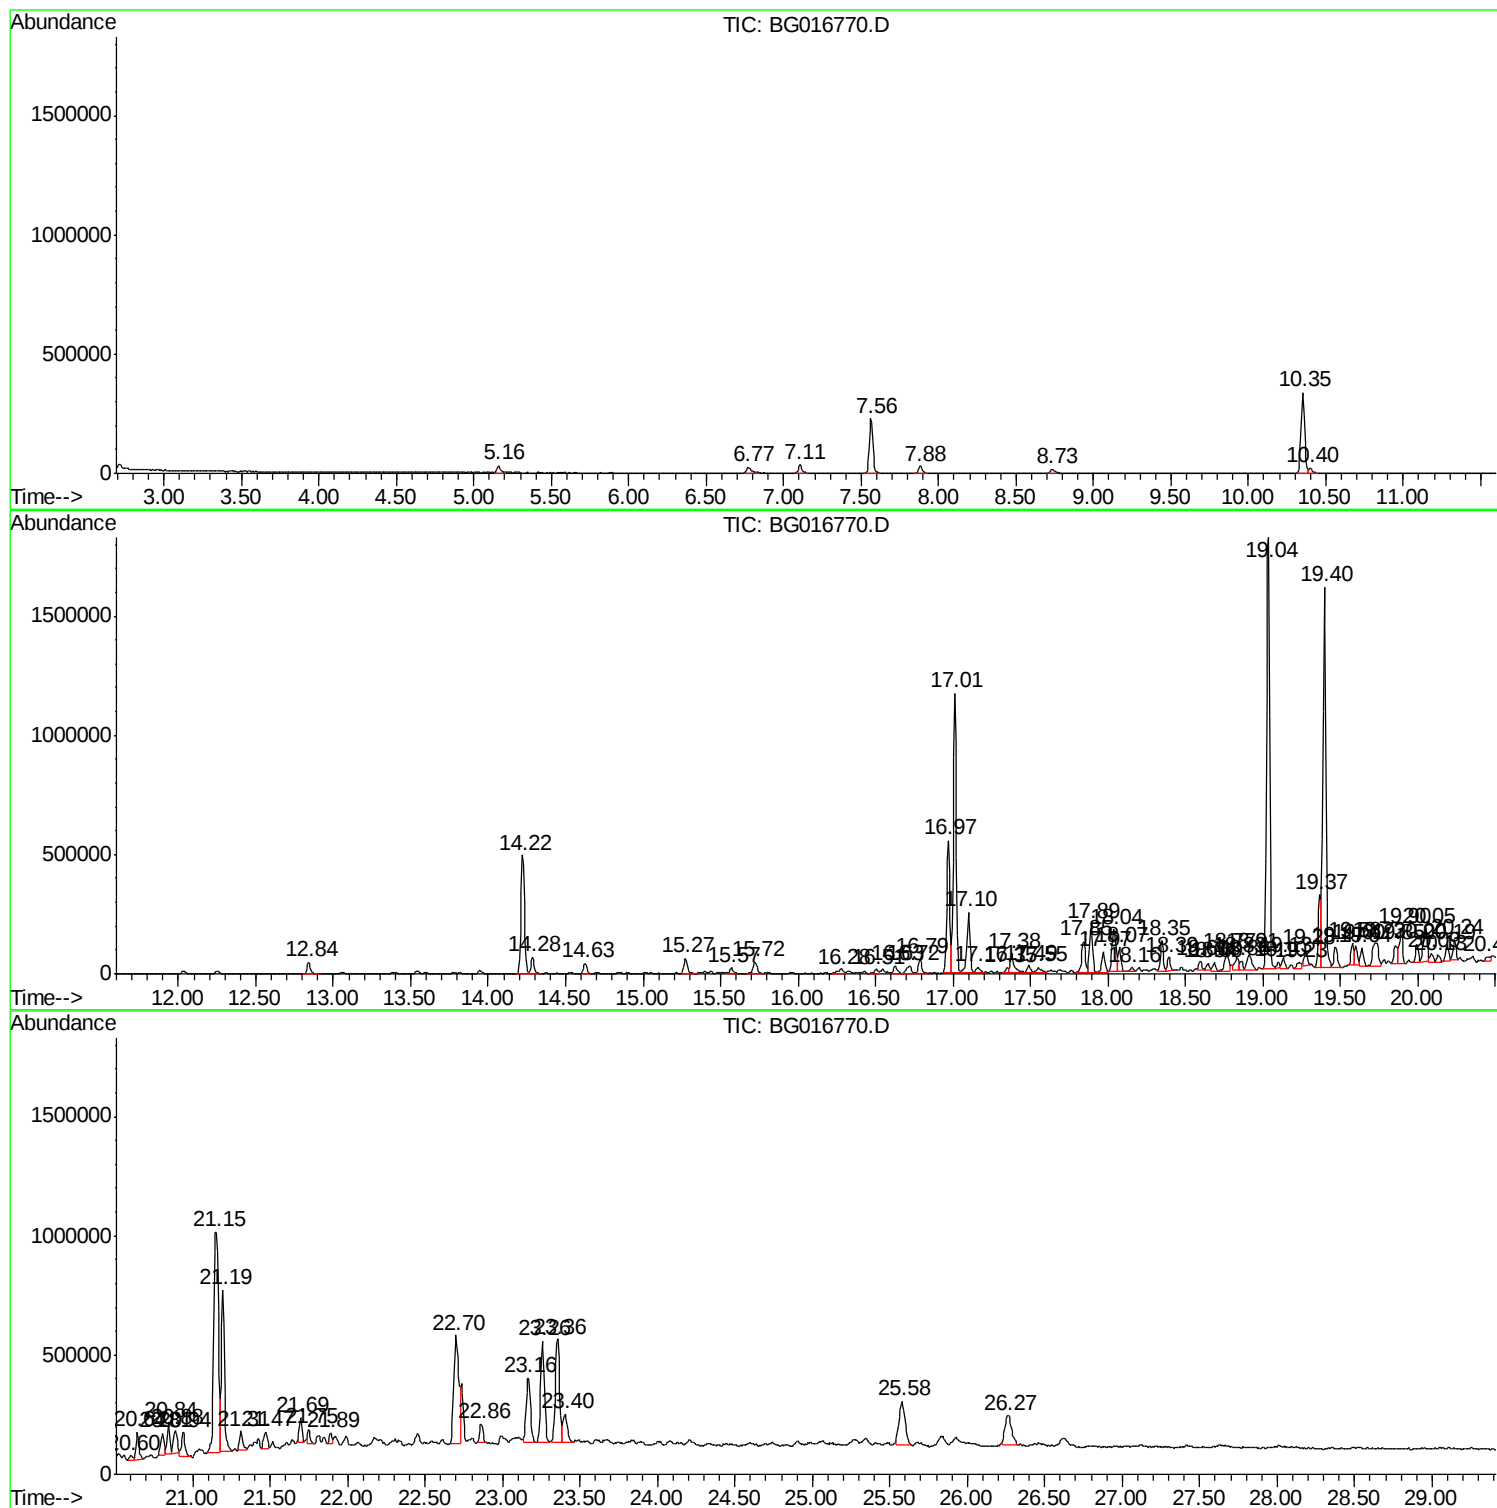

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG042815\
Data_File : BG016770.D
Acq_On : 28 Apr 2015 18:266
Operator : TP/IZZ
Sample : G1991-13DL_25XX
Misc :
ALS_Vial : 7 Sample Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SB-63SDL

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
