


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042815\
 Data File : BG016764.D
 Acq On : 28 Apr 2015 14:34
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 23 19:19:11 2015

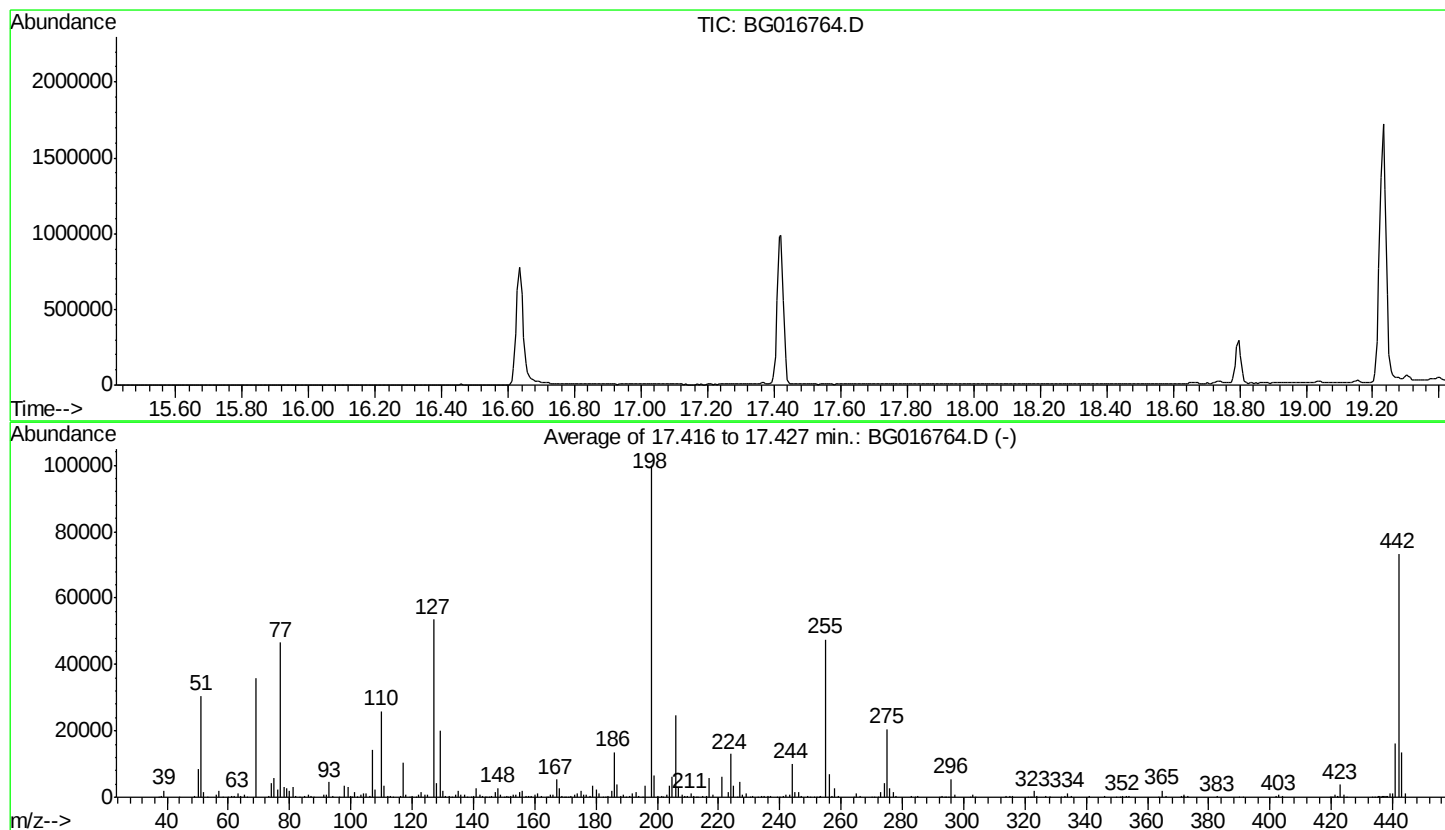

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	30613	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.0	36004	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.6	53562	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99912	PASS
199	198	5	9	6.7	6669	PASS
275	198	10	60	20.5	20513	PASS
365	198	1	100	2.1	2102	PASS
441	442	0.01	24	22.3	16374	PASS
442	198	50	100	73.5	73482	PASS
443	442	15	24	18.4	13531	PASS