
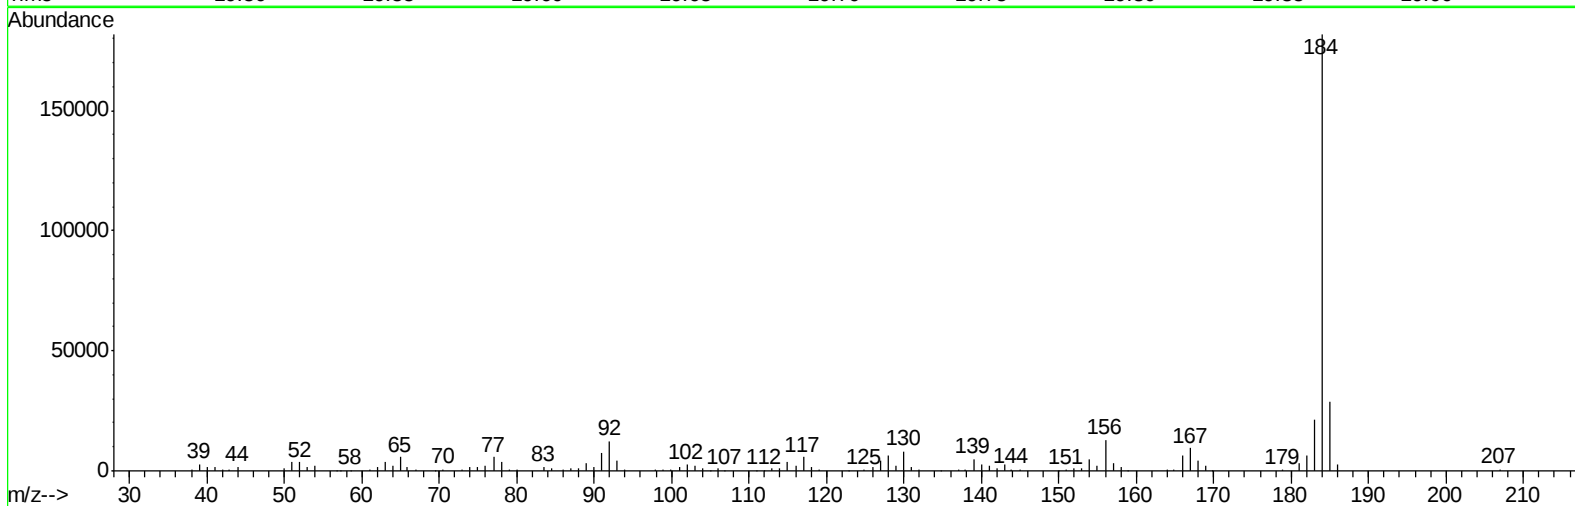


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120118\
Data File : BG038285.D
Acq On : 1 Dec 2018 13:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 04:13:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

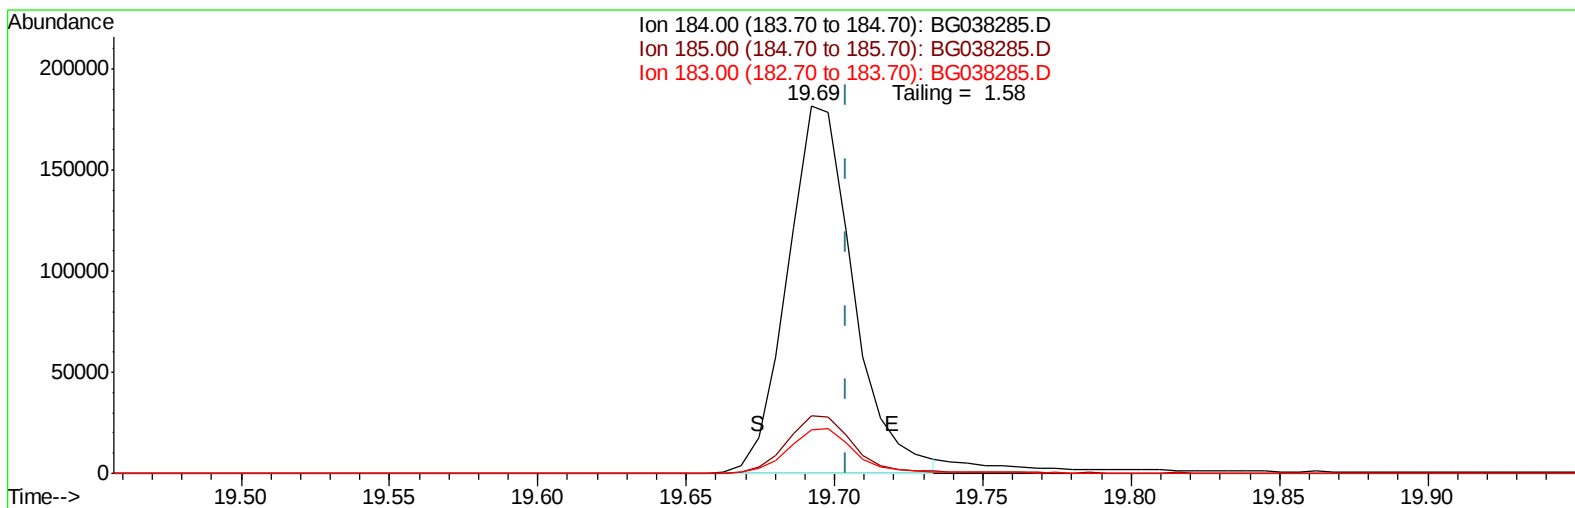

TIC: BG038285.D

(77) Benzidine



19.692min (-0.012) 0.00ng

response 292408

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.82
183.00	12.70	11.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120118\
Data File : BG038285.D
Acq On : 1 Dec 2018 13:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 04:13:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

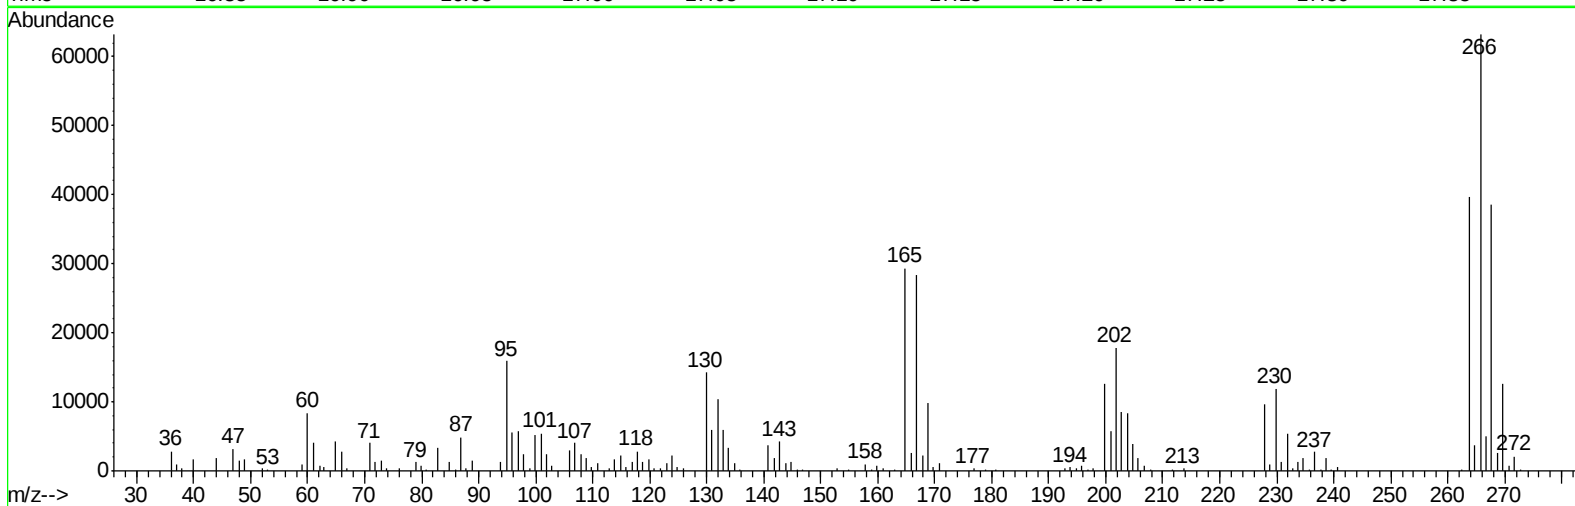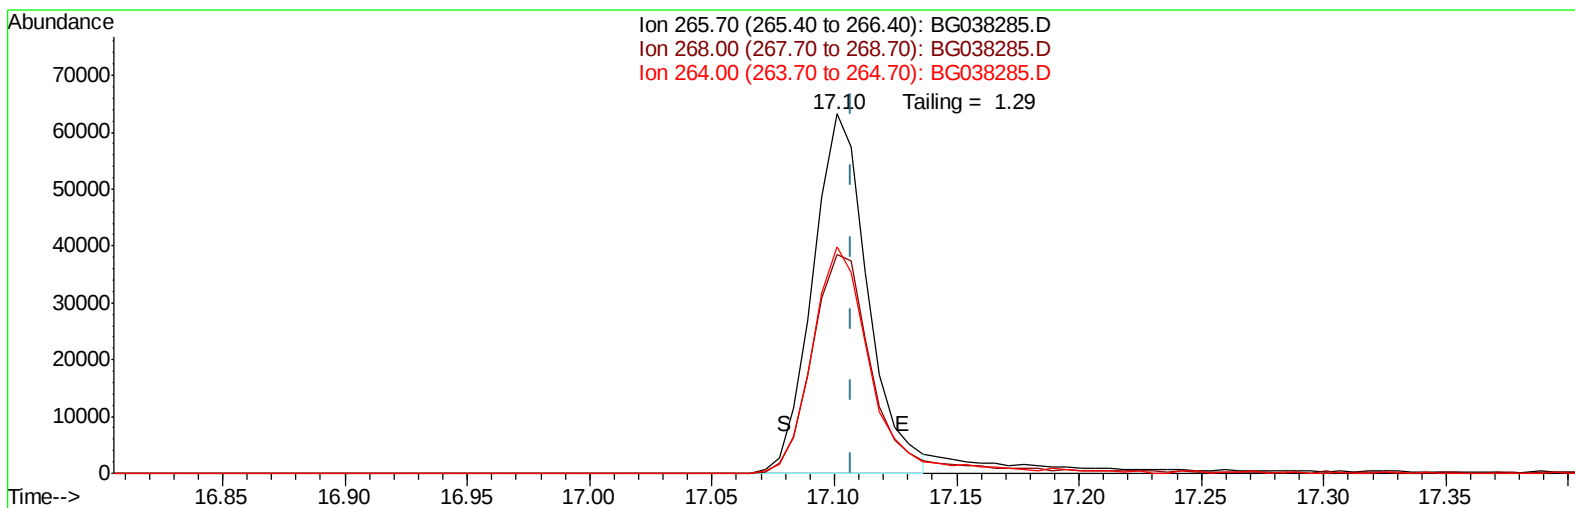

TIC: BG038285.D

(70) Pentachlorophenol (C)

17.101min (-0.006) 97514.69ng

response 107296

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	64.89
264.00	73.60	68.63
0.00	0.00	0.00