

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120118\
 Data File : BG038288.D
 Acq On : 1 Dec 2018 15:27
 Operator : JU/SJ
 Sample : PB115178BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB115178BL

Quant Time: Dec 03 02:44:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	27078	20.00	ng	-0.02
21) Naphthalene-d8	10.90	136	108133	20.00	ng	-0.01
39) Acenaphthene-d10	14.71	164	69153	20.00	ng	-0.01
64) Phenanthrene-d10	17.46	188	193289	20.00	ng	-0.01
76) Chrysene-d12	21.74	240	193478	20.00	ng	-0.01
87) Perylene-d12	25.06	264	194406	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	177748	113.34	ng	-0.01
7) Phenol-d6	7.23	99	243057	108.57	ng	0.00
23) Nitrobenzene-d5	9.25	82	153201	75.84	ng	-0.01
42) 2,4,6-Tribromophenol	16.20	330	98661	125.10	ng	-0.01
45) 2-Fluorobiphenyl	13.34	172	357419	75.30	ng	-0.01
79) Terphenyl-d14	20.06	244	714180	86.86	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120118\
Data File : BG038288.D
Acq On : 1 Dec 2018 15:27
Operator : JU/SJ
Sample : PB115178BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB115178BL

Quant Time: Dec 03 02:44:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

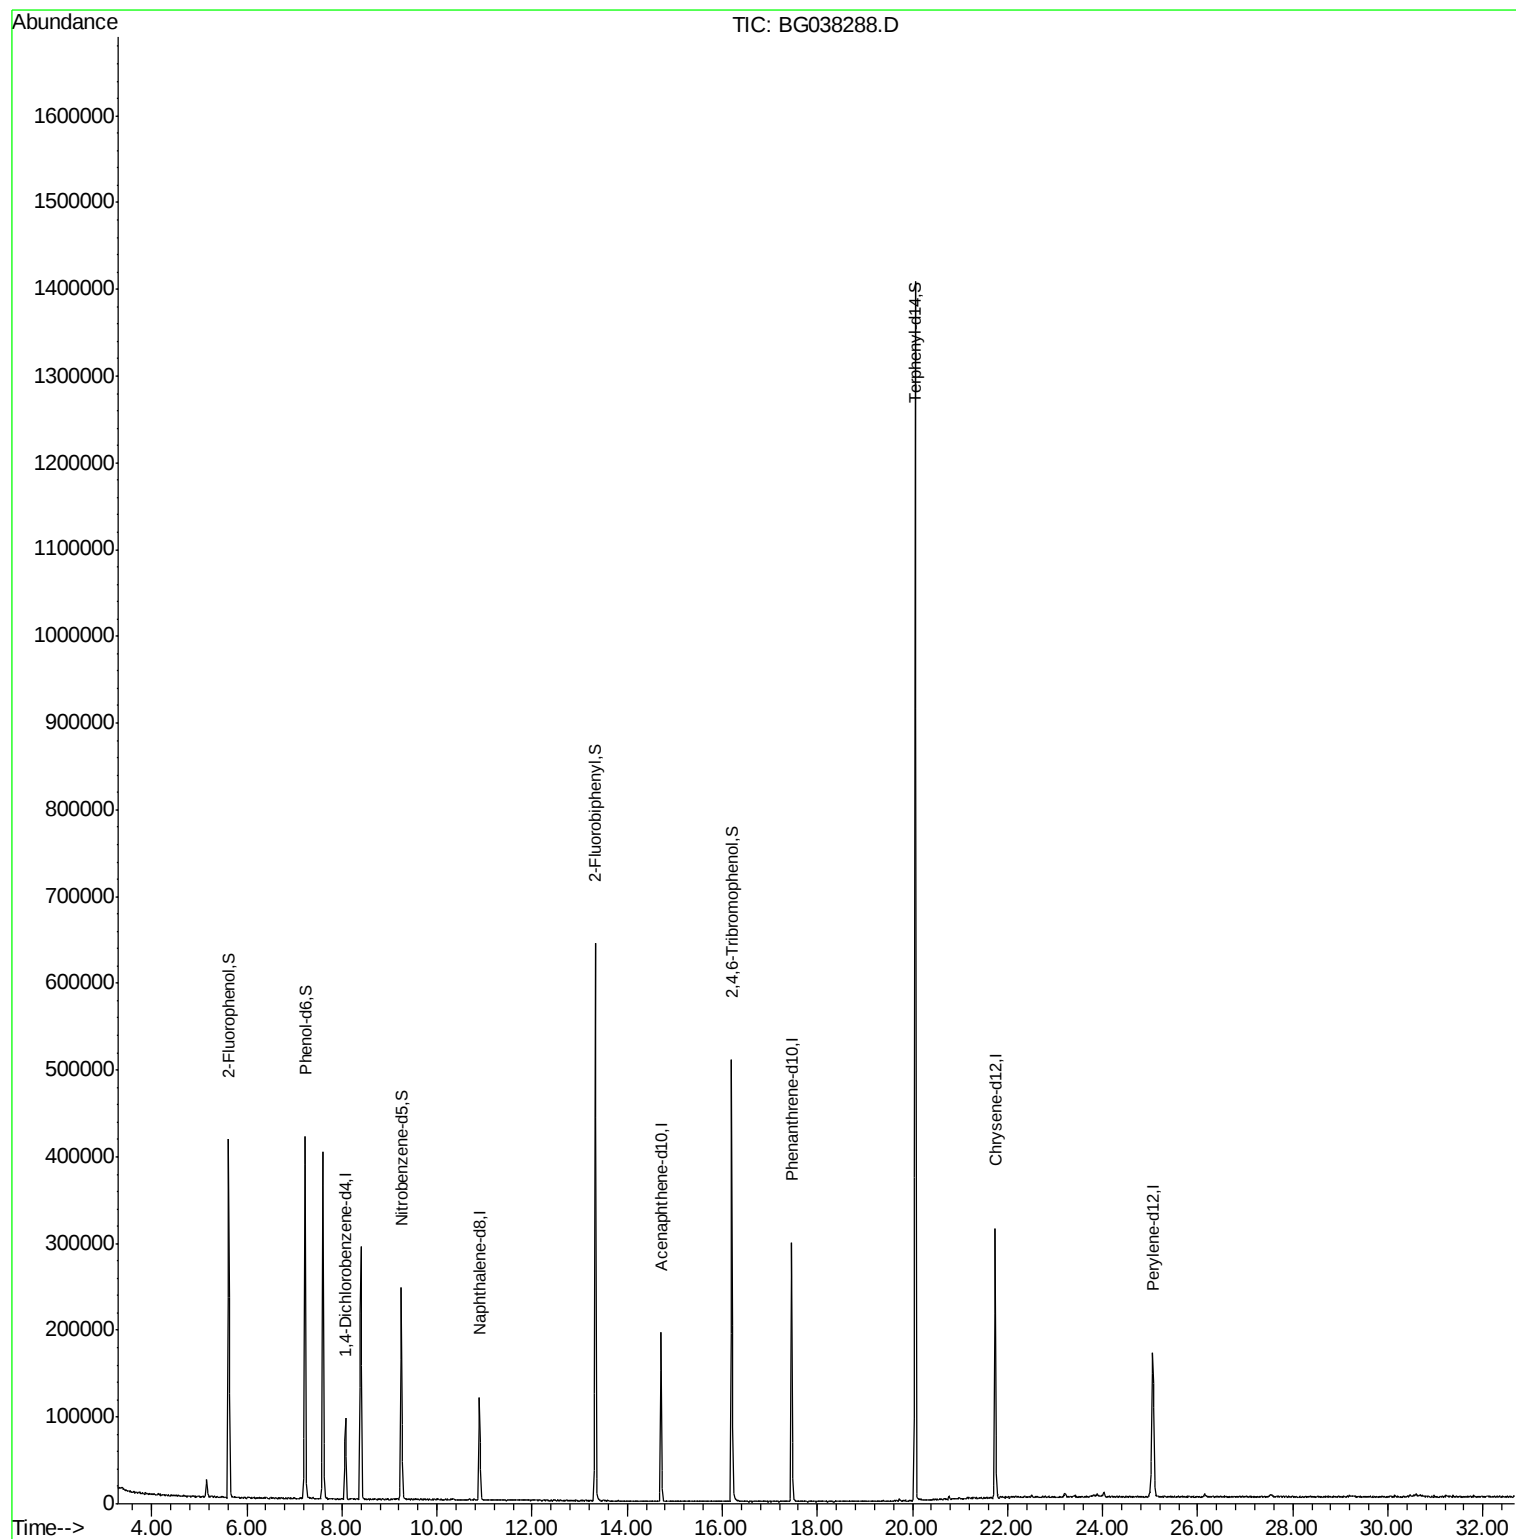

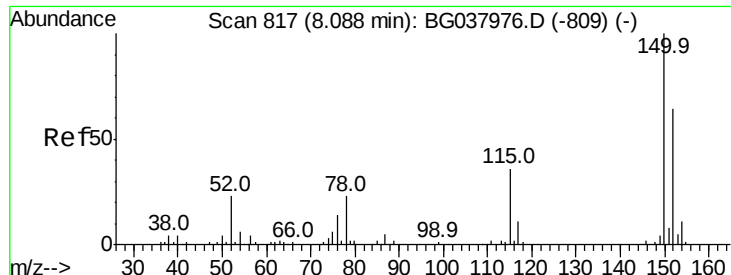


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 814
Delta R.T. -0.02 min
Lab File: BG038288.D
Acq: 1 Dec 2018 15:27

Instrument :
BNA_G
ClientSampleId :
PB115178BL

Tot Ion:152 Resp: 27078
Ion Ratio Lower Upper
152 100
150 153.5 126.0 189.0
115 65.1 45.5 68.3

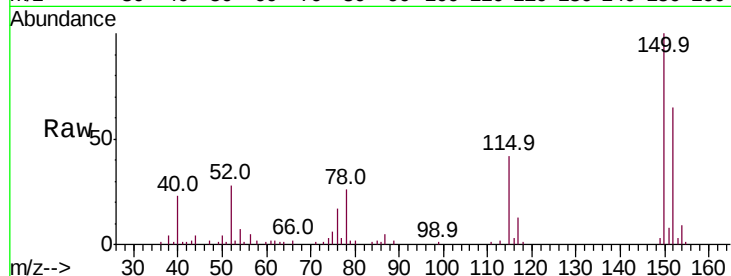


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

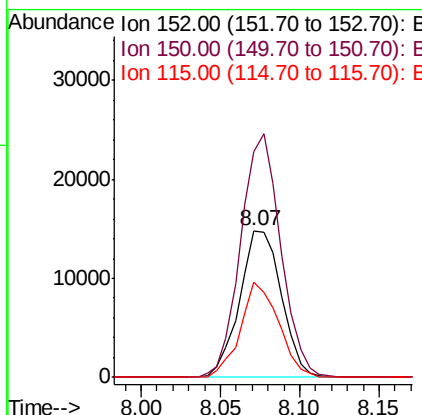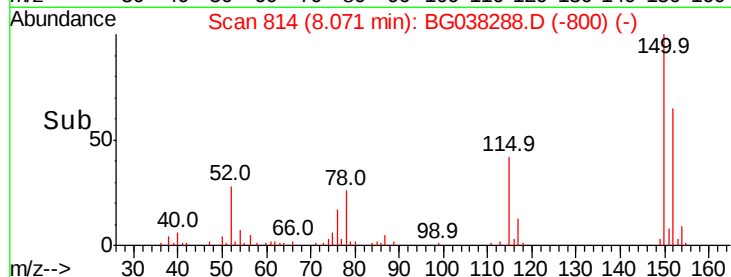



#5


2-Fluorophenol
Concen: 113.337 ng
RT: 5.62 min Scan# 397
Delta R.T. -0.01 min
Lab File: BG038288.D
Acq: 1 Dec 2018 15:27

Tgt Ion:112 Resp: 177748
Ion Ratio Lower Upper
112 100
64 68.7 53.1 79.7
63 36.9 27.3 40.9

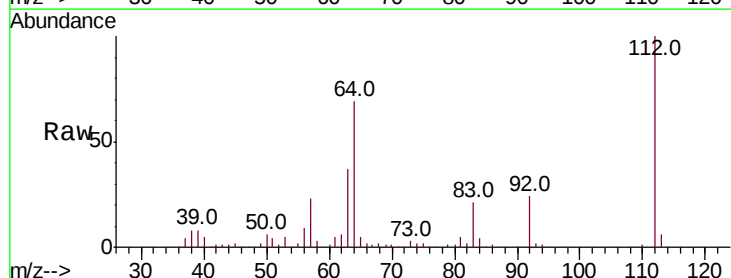

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

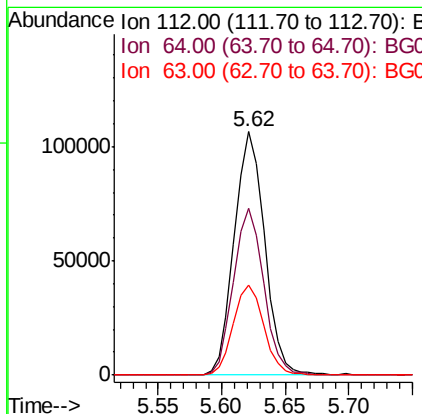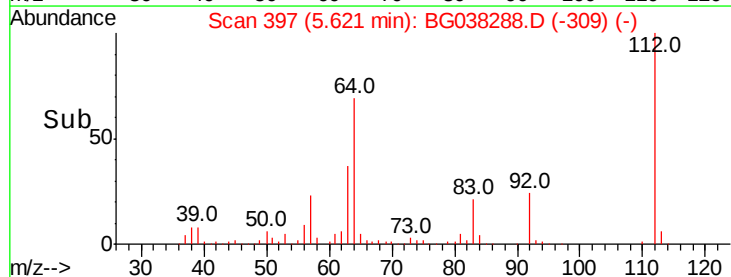

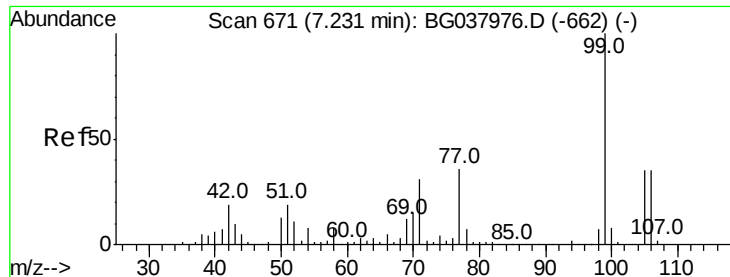

#7

Phenol-d6

Concen: 108.572 ng

RT: 7.23 min Scan# 670

Delta R.T. -0.01 min

Lab File: BG038288.D

Acq: 1 Dec 2018 15:27

Instrument :

BNA_G

ClientSampleId :

PB115178BL


Tot Ion: 99 Resp: 243057

Ion Ratio Lower Upper




99 100

42 22.8 15.0 22.4#

71 35.5 25.5 38.3

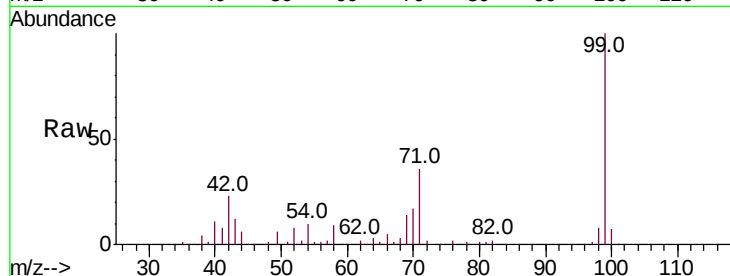

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

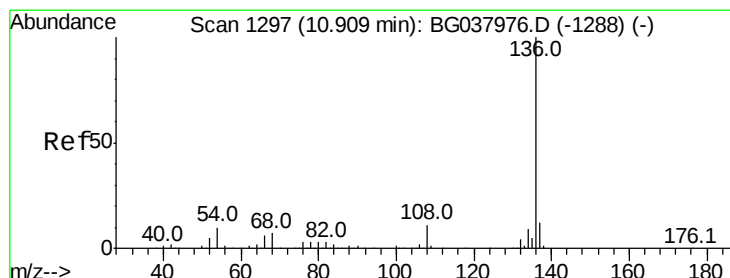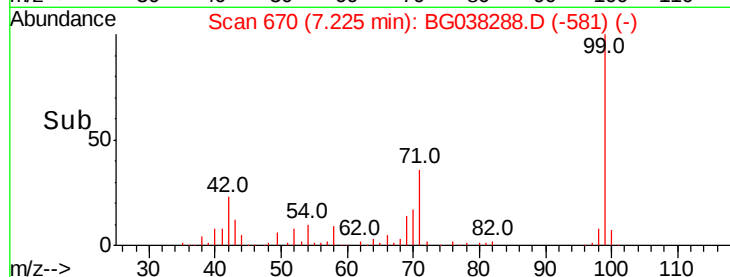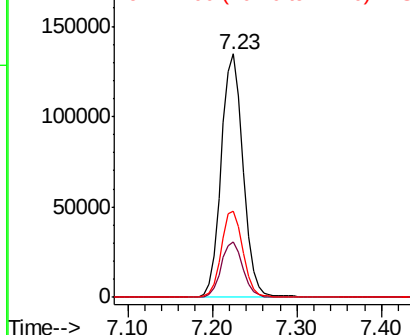

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.90 min Scan# 1295

Delta R.T. -0.01 min

Lab File: BG038288.D

Acq: 1 Dec 2018 15:27

Tgt Ion:136 Resp: 108133


Ion Ratio Lower Upper

136 100



137 11.3 9.6 14.4


54 10.6 7.9 11.9

68 5.4 4.8 7.2

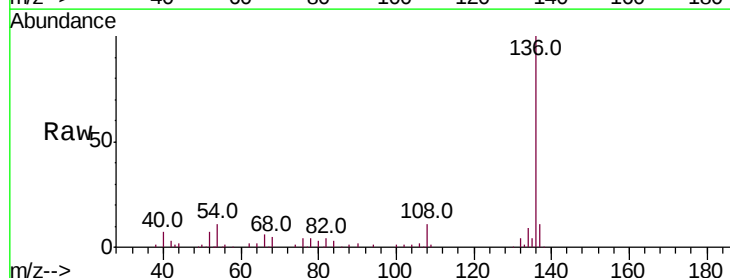

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



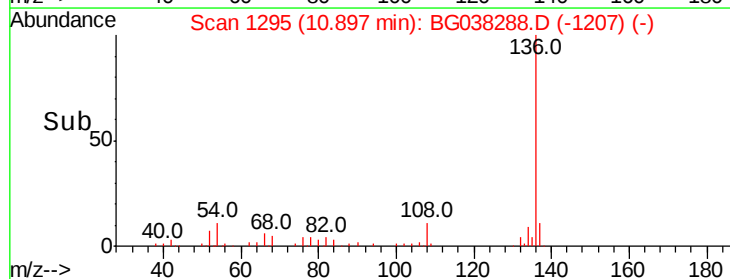
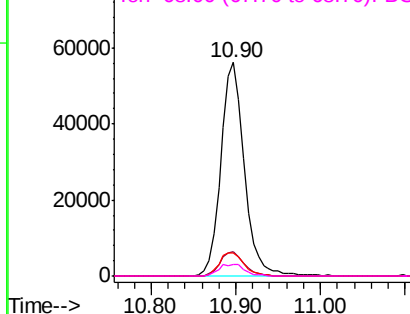


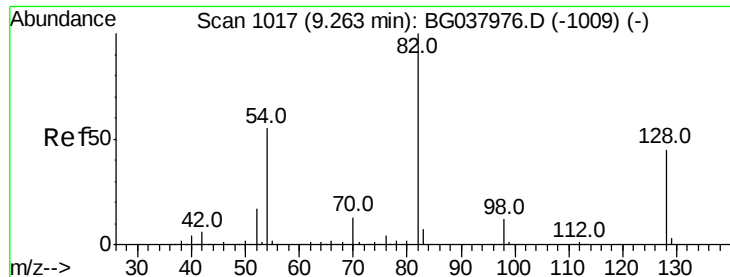

#23
Nitrobenzene-d5
Concen: 75.841 ng
RT: 9.25 min Scan# 1015
Delta R.T. -0.01 min
Lab File: BG038288.D
Acq: 1 Dec 2018 15:27




Instrument :
BNA_G
ClientSampleId :
PB115178BL


Tot Ion: 82 Resp: 153201
Ion Ratio Lower Upper
82 100
128 43.2 34.6 51.8
54 61.4 45.3 67.9

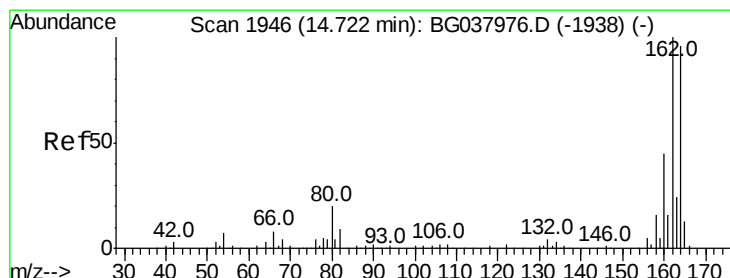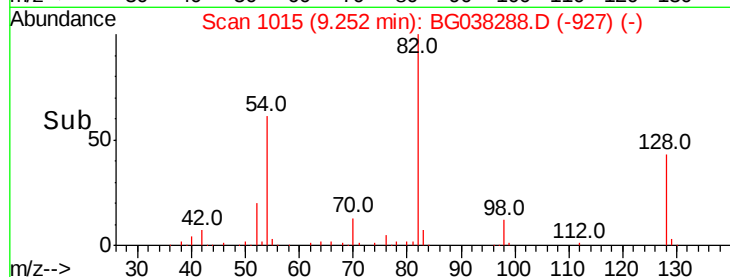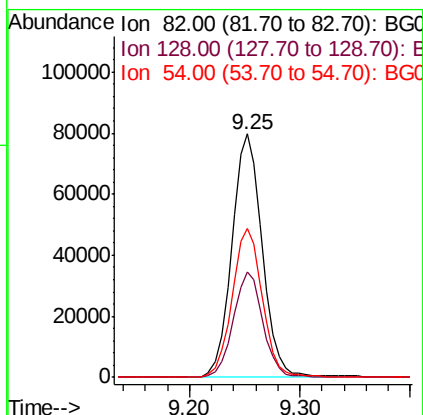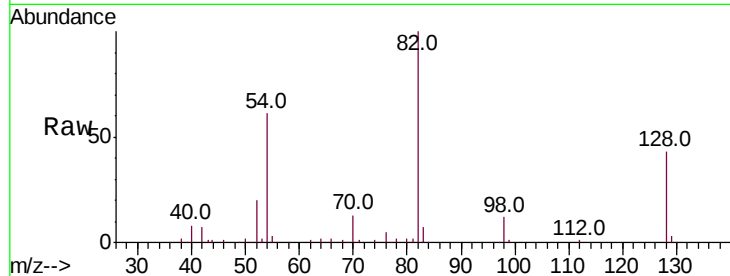

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.71 min Scan# 1944
Delta R.T. -0.01 min
Lab File: BG038288.D
Acq: 1 Dec 2018 15:27

Tgt Ion:164 Resp: 69153
Ion Ratio Lower Upper
164 100
162 103.9 81.3 121.9
160 43.3 36.3 54.5

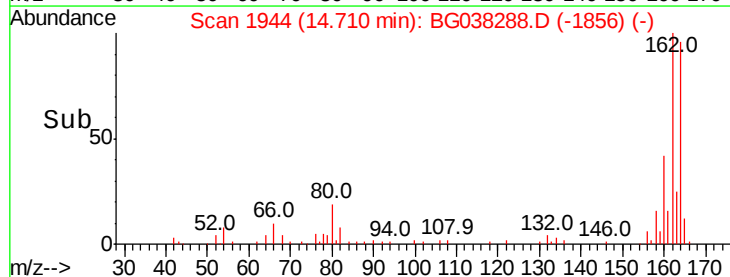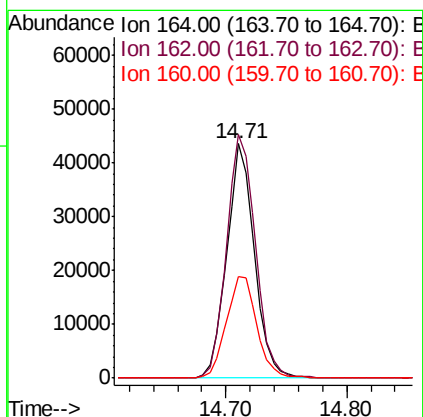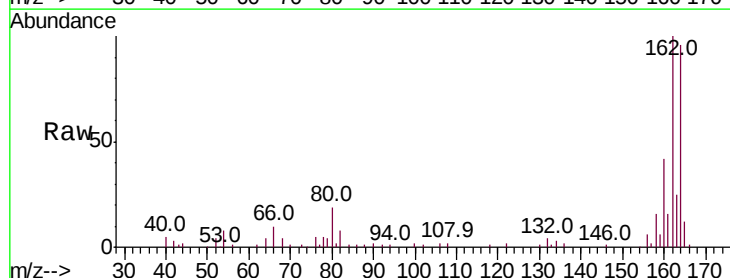


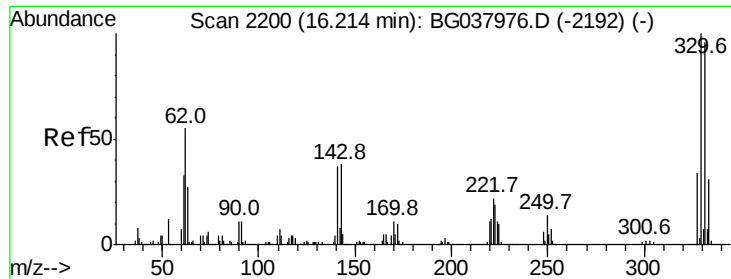

#42
 2,4,6-Tribromophenol
 Concen: 125.097 ng
 RT: 16.20 min Scan# 2198
 Delta R.T. -0.01 min
 Lab File: BG038288.D
 Acq: 1 Dec 2018 15:27

Instrument :
 BNA_G
 ClientSampleId :
 PB115178BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.3	78.4	117.6
141	40.9	32.2	48.2



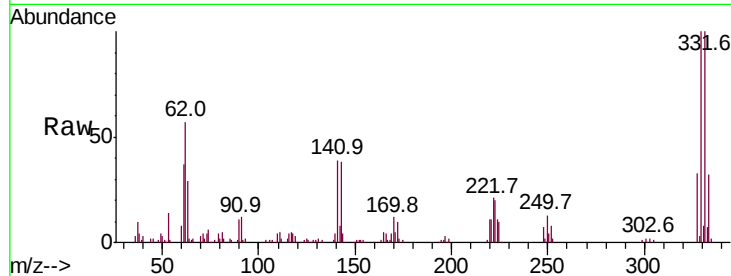


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

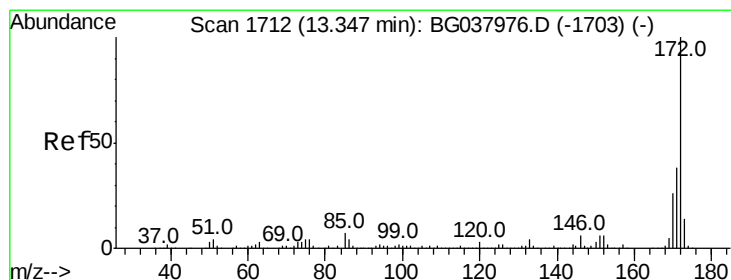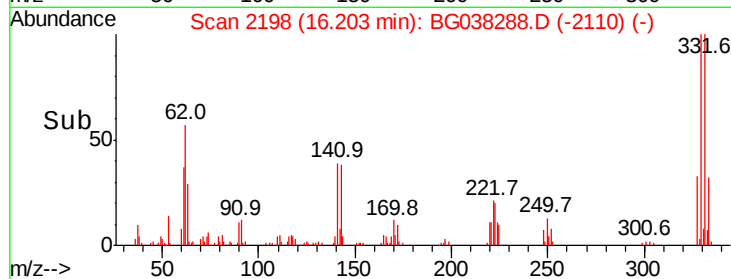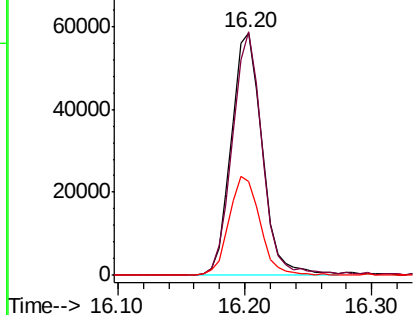

#45
 2-Fluorobiphenyl
 Concen: 75.298 ng
 RT: 13.34 min Scan# 1710
 Delta R.T. -0.01 min
 Lab File: BG038288.D
 Acq: 1 Dec 2018 15:27

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.0	31.0	46.4
170	24.2	20.2	30.2


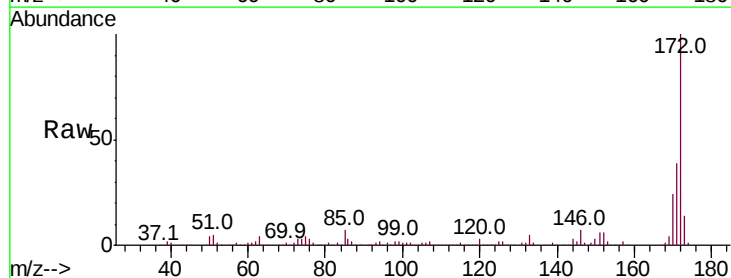



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

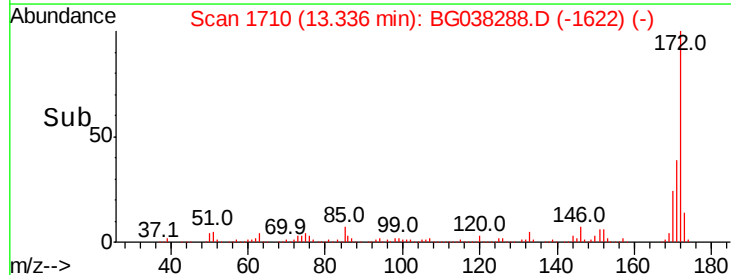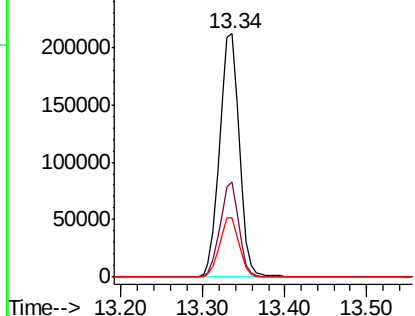

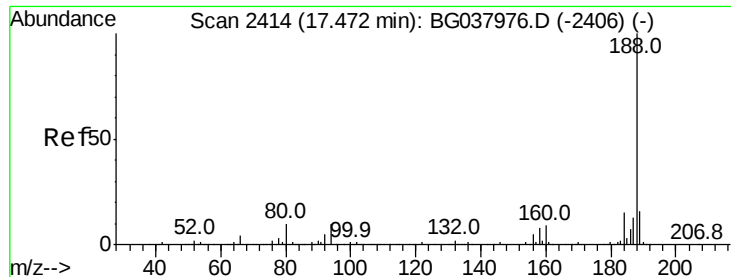

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.46 min Scan# 2412

Delta R.T. -0.01 min

Lab File: BG038288.D

Acq: 1 Dec 2018 15:27

Instrument :

BNA_G

ClientSampleId :

PB115178BL



Tot Ion:188 Resp: 193289

Ion Ratio Lower Upper

188 100

94 8.6 7.2 10.8



80 8.9 7.7 11.5

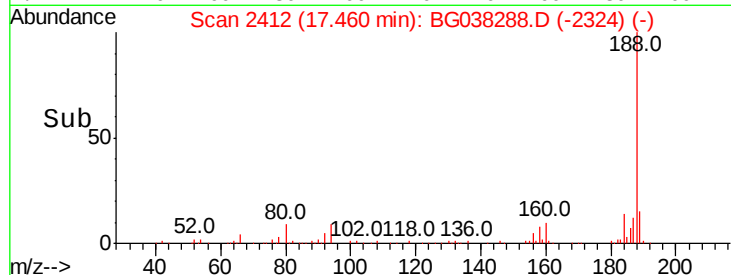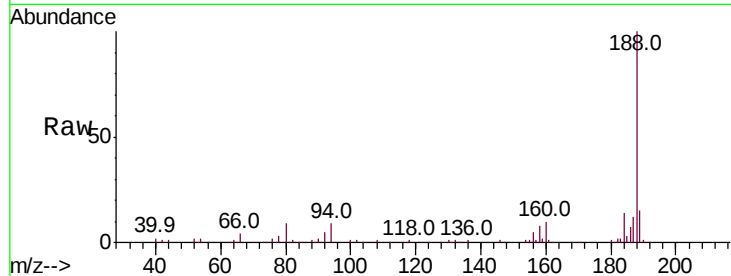

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

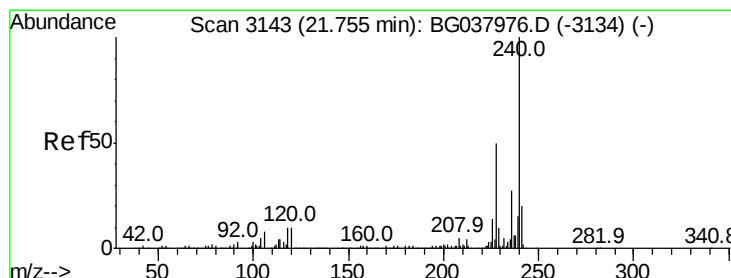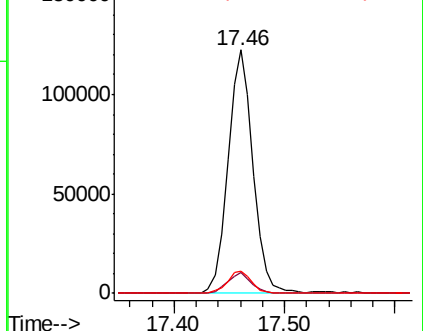

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.74 min Scan# 3141

Delta R.T. -0.01 min

Lab File: BG038288.D

Acq: 1 Dec 2018 15:27



Tgt Ion:240 Resp: 193478

Ion Ratio Lower Upper

240 100

120 9.4 8.1 12.1


236 26.9 21.4 32.0

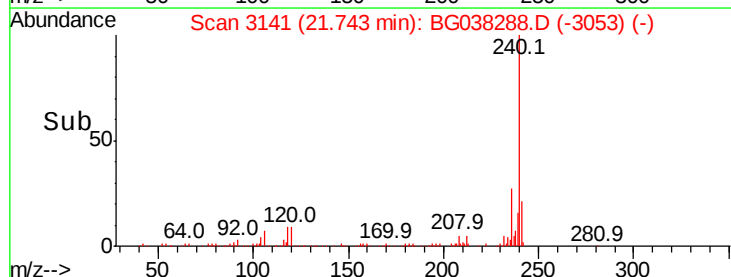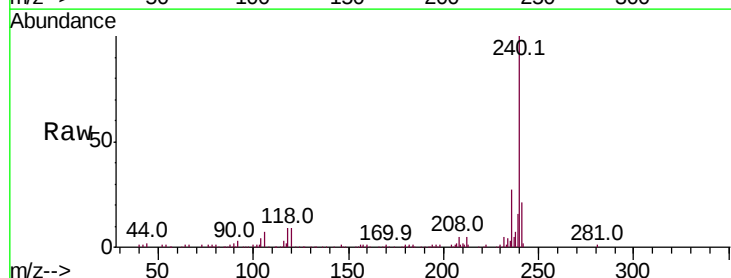

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

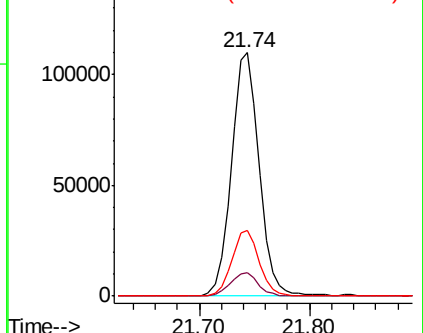



#79

Terphenyl-d14

Concen: 86.856 ng

RT: 20.06 min Scan# 2856

Delta R.T. -0.01 min

Lab File: BG038288.D

Acq: 1 Dec 2018 15:27

Instrument :

BNA_G

ClientSampleId :

PB115178BL


Tot Ion:244 Resp: 714180

Ion Ratio Lower Upper

244 100

212 7.9 6.5 9.7




122 8.9 9.0 13.4#

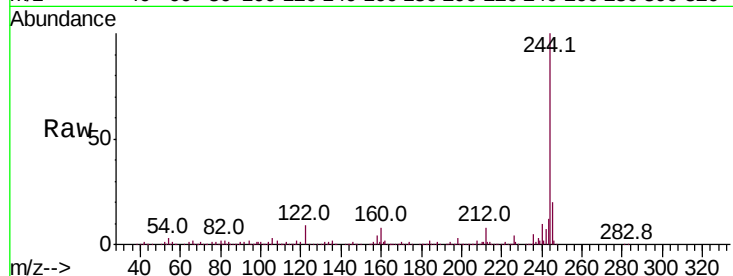

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

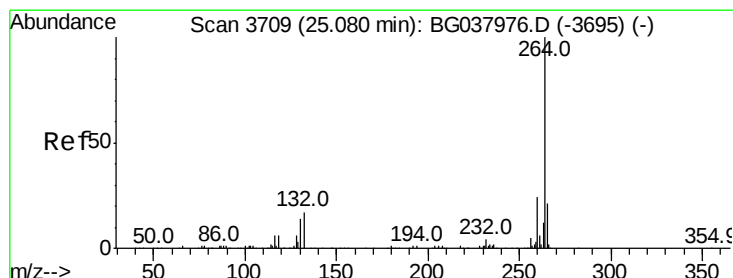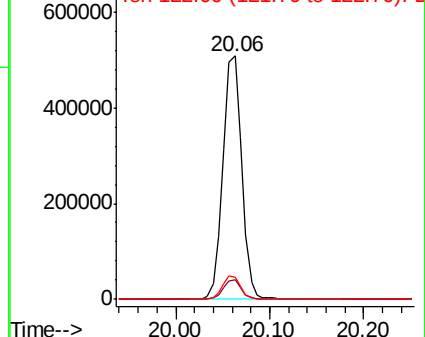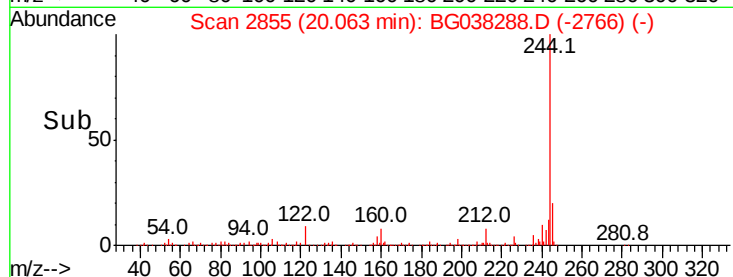

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.06 min Scan# 3705

Delta R.T. -0.02 min

Lab File: BG038288.D

Acq: 1 Dec 2018 15:27


Tgt Ion:264 Resp: 194406

Ion Ratio Lower Upper

264 100

260 22.8 18.2 27.4

265 21.5 17.9 26.9

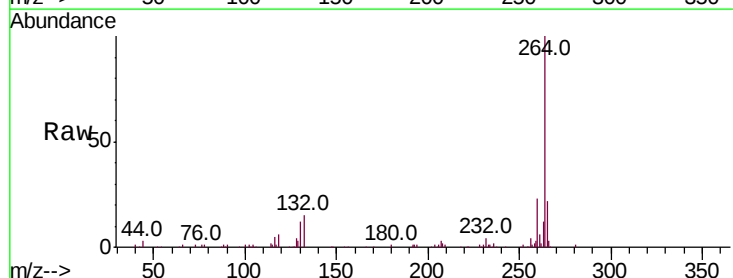

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

