


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120118\
 Data File : BG038285.D
 Acq On : 1 Dec 2018 13:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

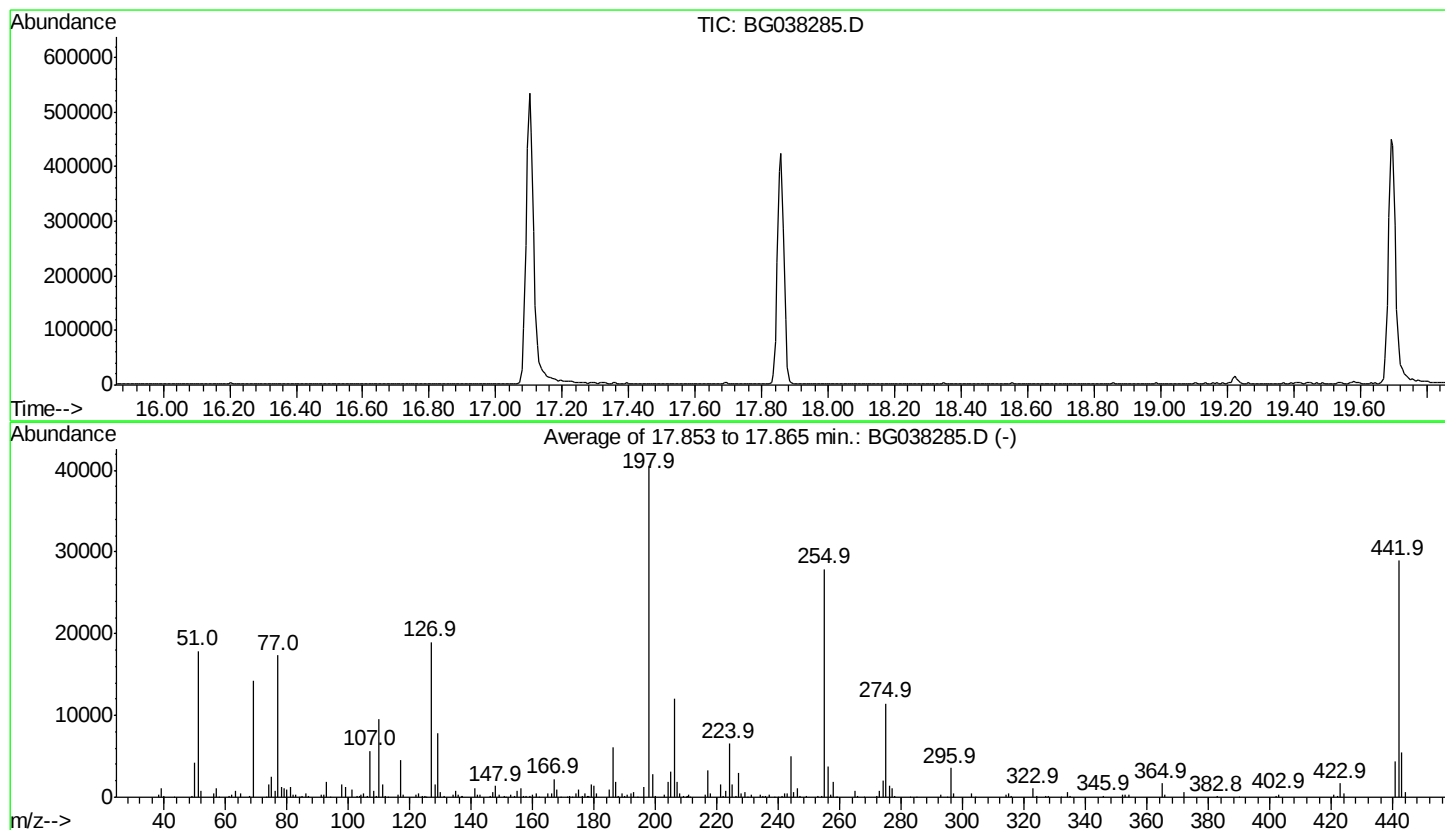

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	17899	PASS
68	69	0.00	2	1.4	201	PASS
69	198	0.00	100	35.0	14218	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	18992	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40573	PASS
199	198	5	9	7.1	2899	PASS
275	198	10	60	28.2	11457	PASS
365	198	1	100	4.1	1676	PASS
441	198	0.01	100	11.0	4457	PASS
442	198	50	100	71.4	28970	PASS
443	442	15	24	18.7	5420	PASS