
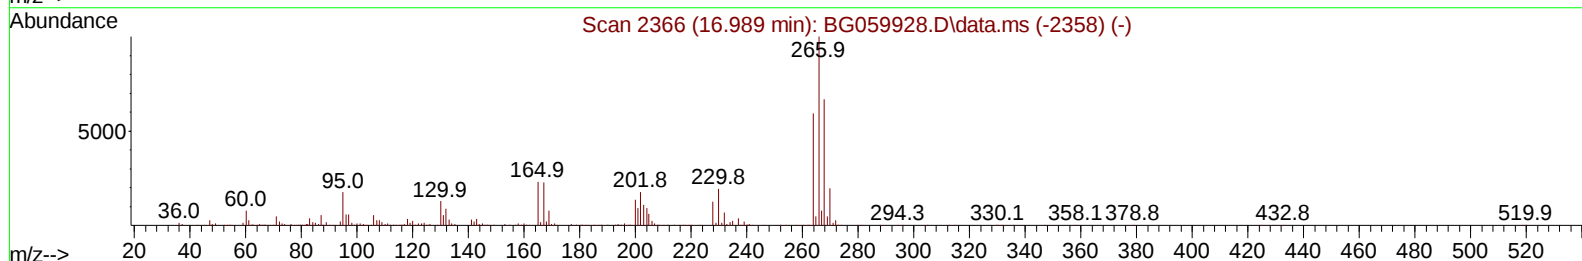
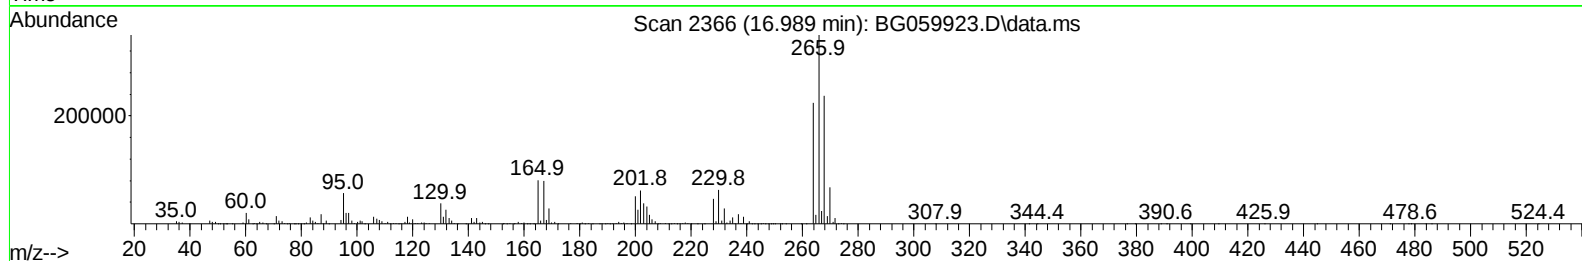


Quant Time: Dec 02 03:44:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 03:28:09 2023
Response via : Initial Calibration

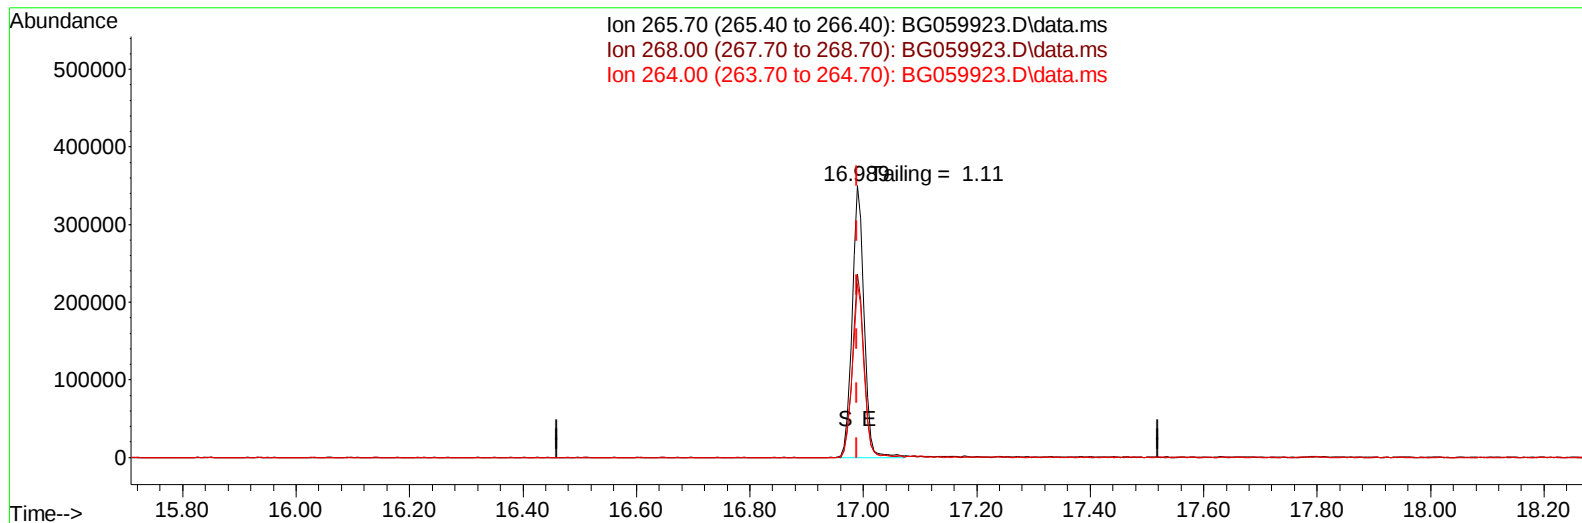

TIC: BG059923.D\data.ms

(70) Pentachlorophenol (C)




16.989min (+ 0.000) 310586.10 ng

response 514435

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.80	67.66
264.00	59.40	63.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120123\
Data File : BG059923.D
Acq On : 1 Dec 2023 18:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 03:44:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 03:28:09 2023
Response via : Initial Calibration

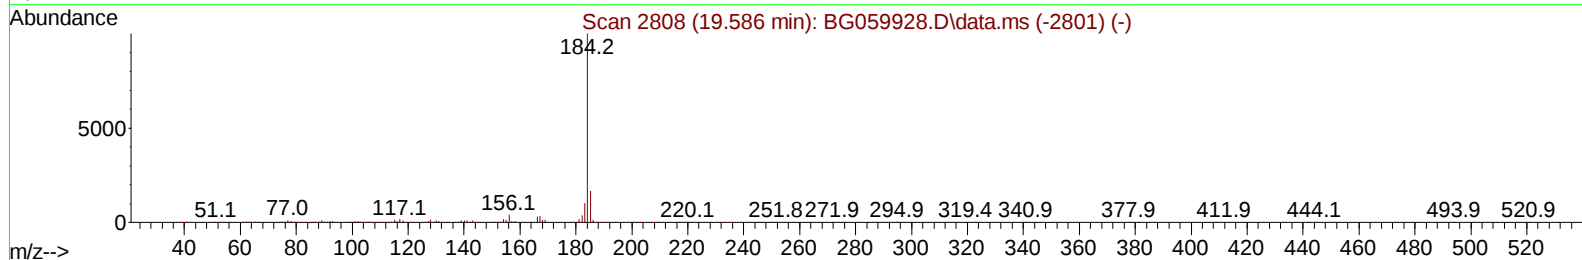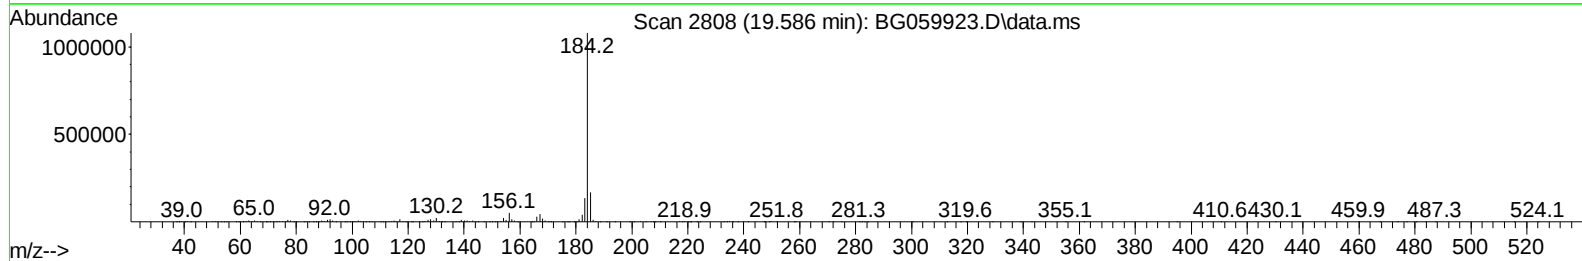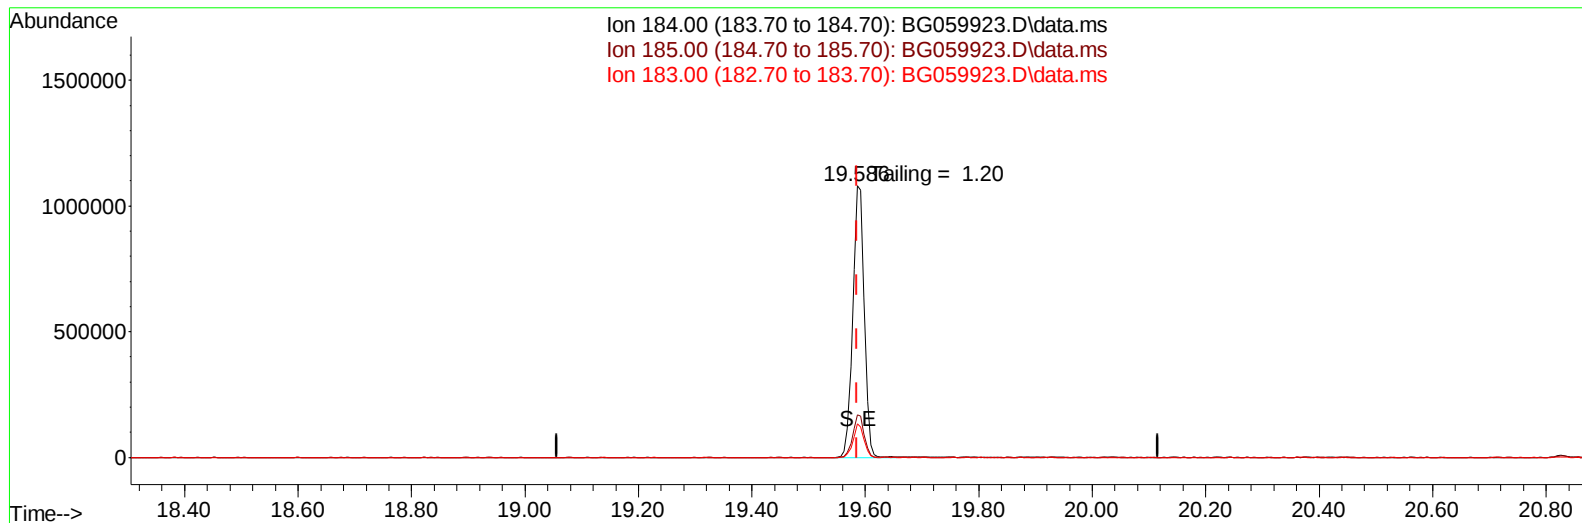

TIC: BG059923.D\data.ms

(77) Benzidine**19.586min (+ 0.000) 1062886.20 ng****response 1526219**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.60	15.66
183.00	10.30	12.43#
0.00	0.00	0.00