


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120123\
Data File : BG059923.D
Acq On : 1 Dec 2023 18:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 02 03:28:09 2023

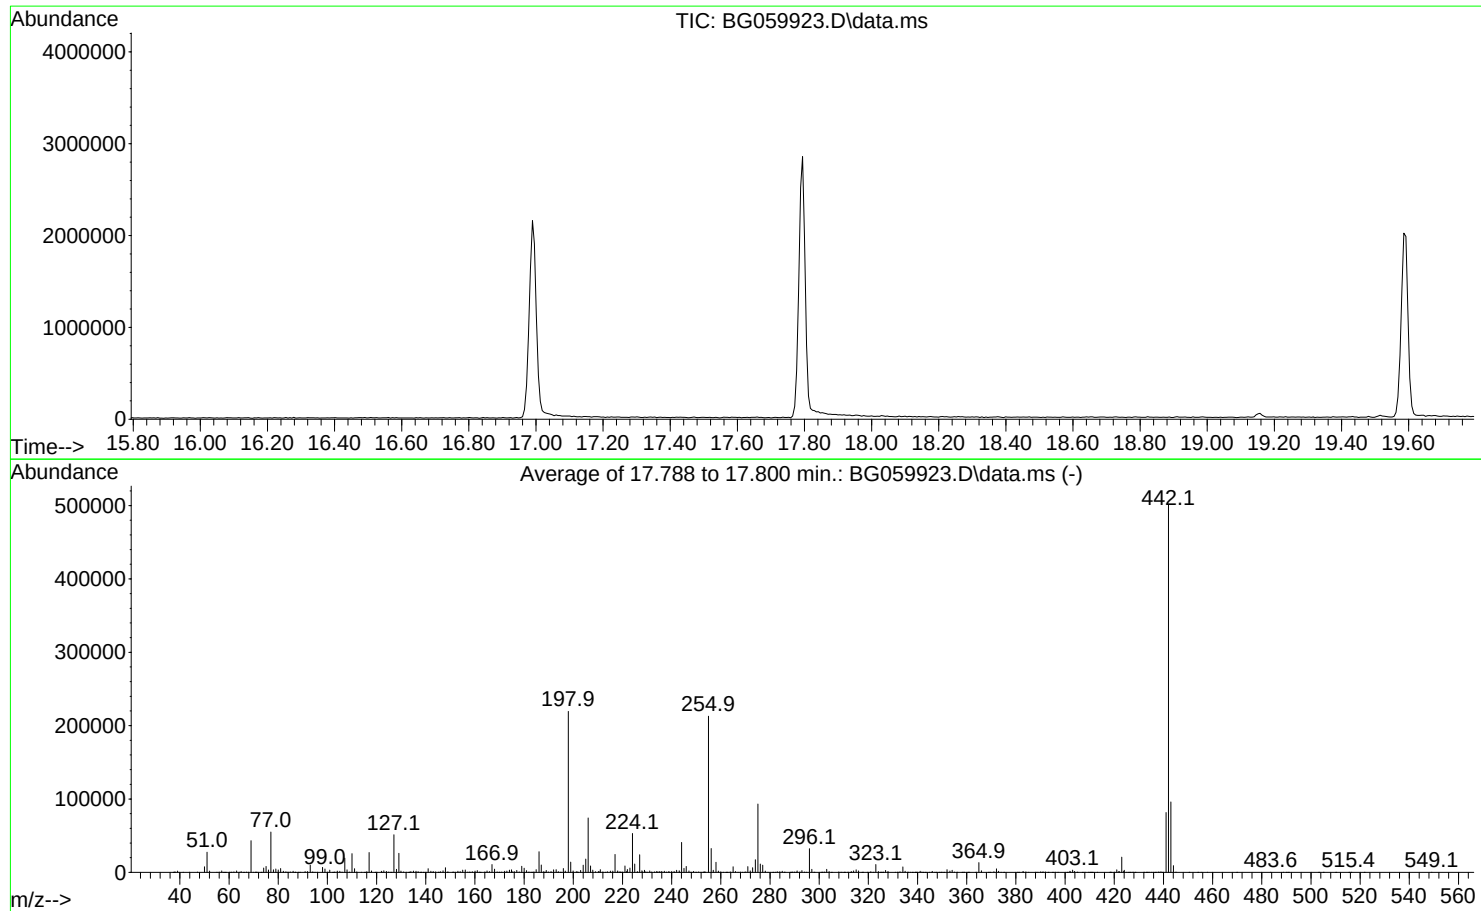




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	12.5	27499	PASS
68	69	0.00	2	0.4	184	PASS
69	198	0.00	100	19.7	43136	PASS
70	69	0.00	2	0.5	224	PASS
127	198	10	80	23.4	51352	PASS
197	198	0.00	2	0.9	1867	PASS
198	198	100	100	100.0	219520	PASS
199	198	5	9	6.4	14042	PASS
275	198	10	60	42.4	93155	PASS
365	198	1	100	6.0	13275	PASS
441	198	0.01	100	37.2	81597	PASS
442	442	50	100	100.0	501461	PASS
443	442	15	24	19.1	95960	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120123\
Data File : BG059923.D
Acq On : 1 Dec 2023 18:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 02 03:44:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 03:28:09 2023
Response via : Initial Calibration

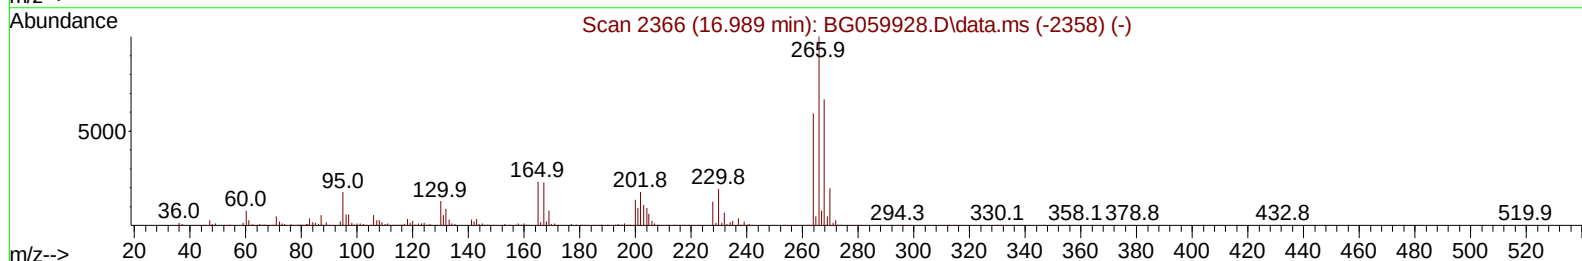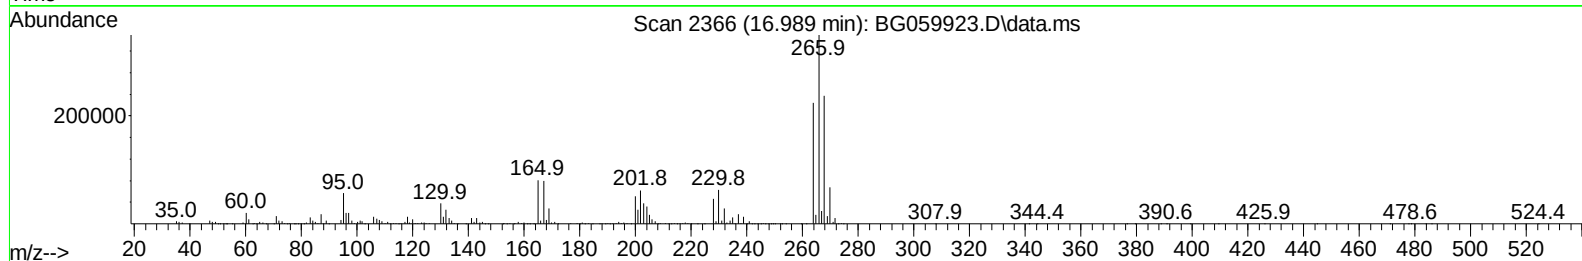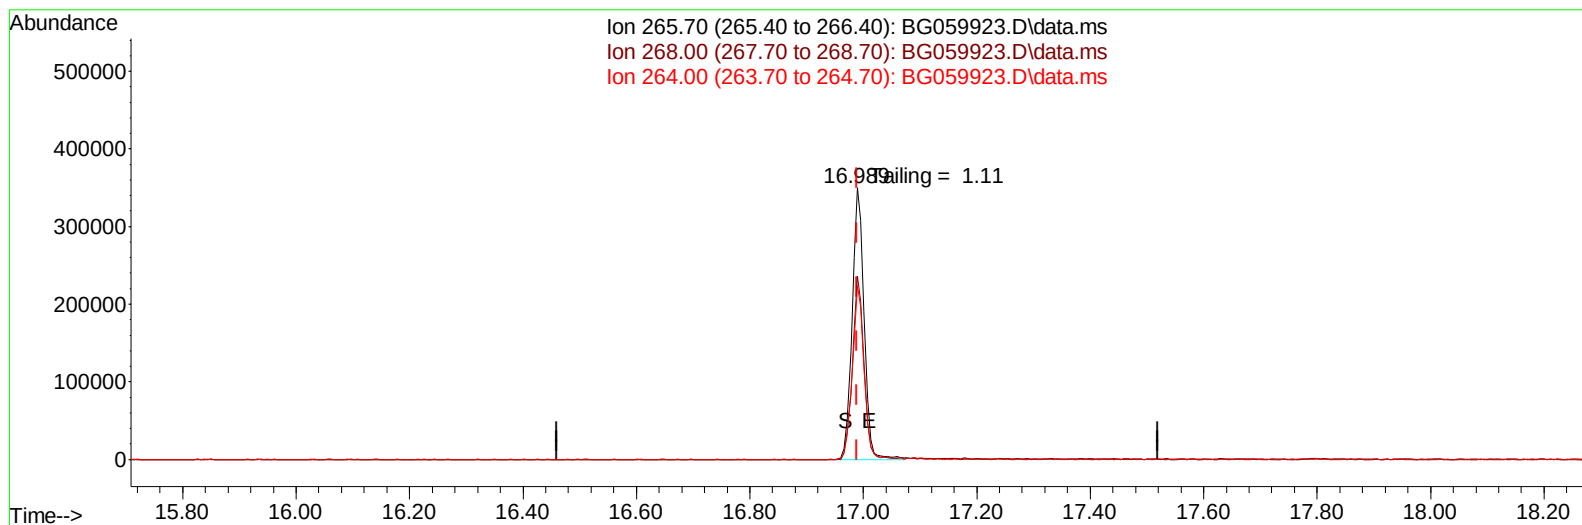

TIC: BG059923.D\data.ms

(70) Pentachlorophenol (C)

16.989min (+ 0.000) 310586.10 ng




response 514435

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.80	67.66
264.00	59.40	63.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120123\
Data File : BG059923.D
Acq On : 1 Dec 2023 18:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 02 03:44:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 03:28:09 2023
Response via : Initial Calibration

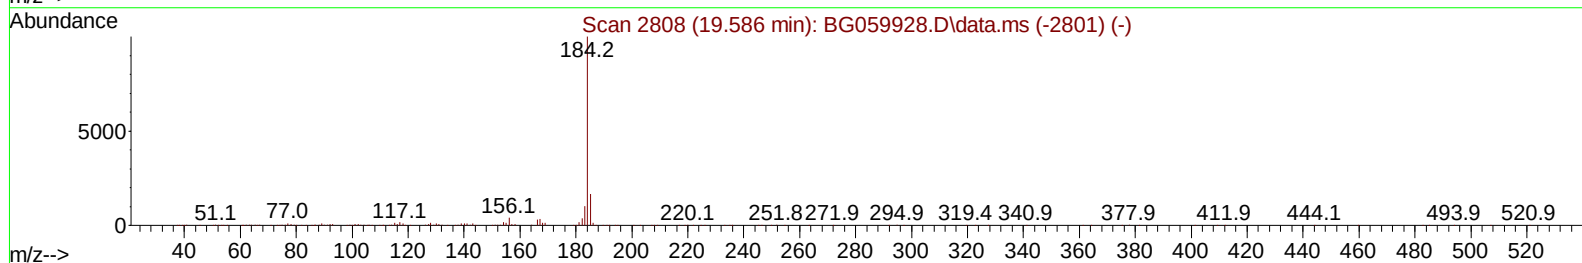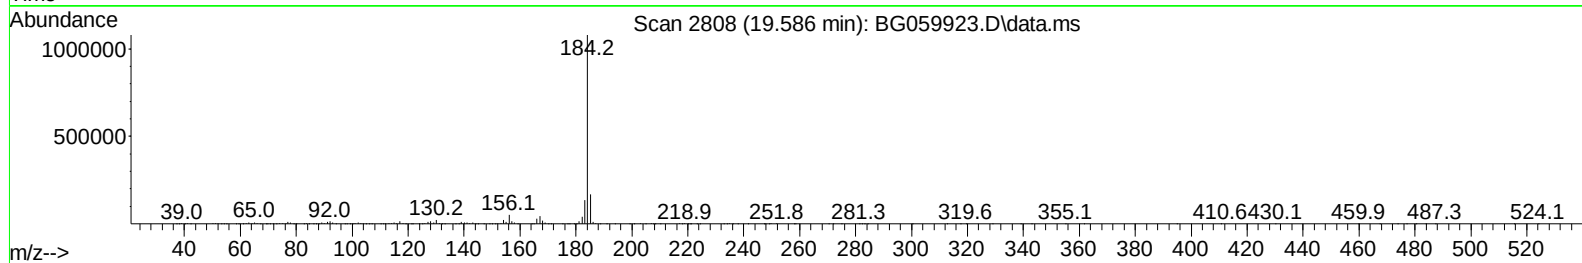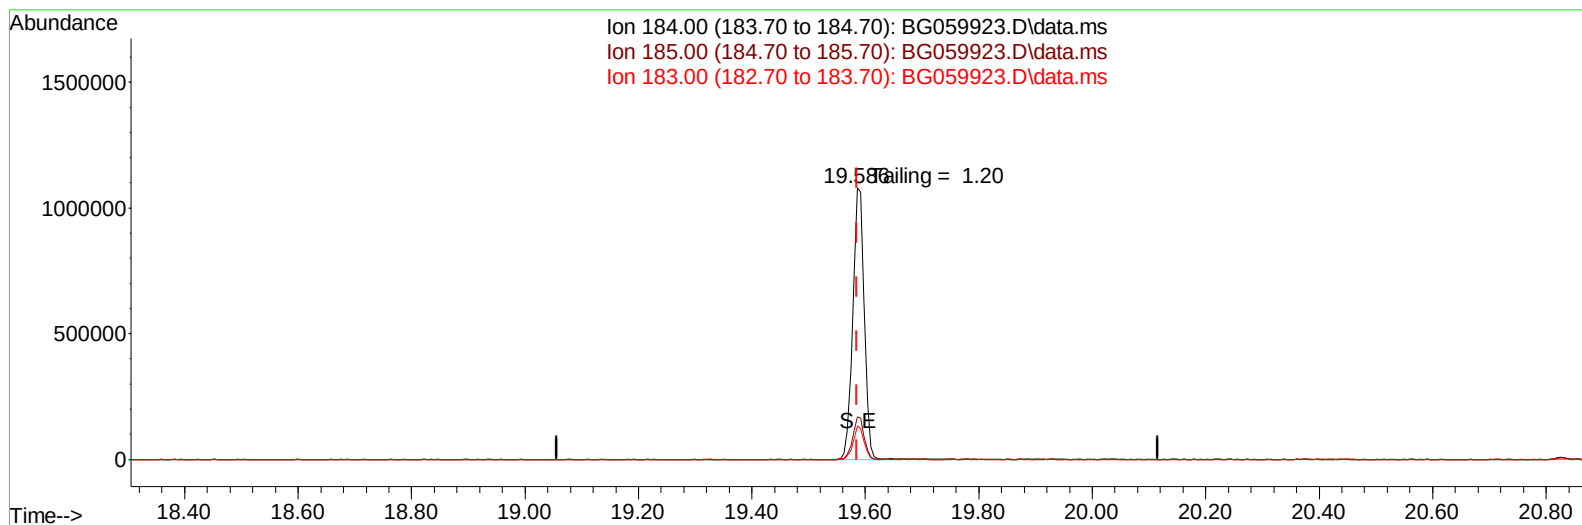

TIC: BG059923.D\data.ms

(77) Benzidine

19.586min (+ 0.000) 1062886.20 ng

response 1526219

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.60	15.66
183.00	10.30	12.43#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2023	BNA_G	<u>BG059923.D</u>
Compound Name	Response	Retention Time
DDT	1044287	20.825
DDD	54215	20.379
DDE	1787	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
56002	1100289	5.09

Instrument :
BNA_G
ClientSampleId :
DFTPP