

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
 Data File : BG051320.D
 Acq On : 3 Dec 2021 2:38
 Operator : CG/JU
 Sample : M4868-07DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKP2DL

Quant Time: Dec 03 03:19:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 24 06:04:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.194	152	33533	20.000	ng/u1	0.00
20) Naphthalene-d8	11.020	136	149340	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.828	164	100820	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.577	188	212521	20.000	ng/u1	0.00
79) Chrysene-d12	21.878	240	194716	20.000	ng/u1	0.00
88) Perylene-d12	25.274	264	198628	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.529	96	1935	2.005	ng/uL	-0.01
4) Pyridine-d5	3.970	84	25273	8.925	ng/u1	0.00
7) Phenol-d5	7.354	99	40491	12.217	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.507	67	26201	12.588	ng/u1	0.00
11) 2-Chlorophenol-d4	7.724	132	29872	12.517	ng/u1	0.00
15) 4-Methylphenol-d8	8.905	113	32561	12.175	ng/u1	0.00
21) Nitrobenzene-d5	9.369	128	15544	12.330	ng/u1	0.00
24) 2-Nitrophenol-d4	10.098	143	18198	12.797	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.650	165	29840	12.367	ng/u1	0.00
31) 4-Chloroaniline-d4	11.161	131	37456	10.610	ng/u1	0.00
46) Dimethylphthalate-d6	14.216	166	108173	13.944	ng/u1	0.00
49) Acenaphthylene-d8	14.522	160	133034	13.600	ng/u1	0.00
54) 4-Nitrophenol-d4	15.057	143	14737	11.736	ng/u1	0.00
60) Fluorene-d10	15.815	176	94569	13.538	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.950	200	10420	7.946	ng/u1	0.00
73) Anthracene-d10	17.671	188	165563	16.289	ng/u1	0.00
81) Pyrene-d10	19.957	212	188029	15.959	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.039	264	165374	15.589	ng/u1	0.00
Target Compounds						
					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.714	149	418282	49.395	ng/u1	99
89) Di-n-octyl phthalate	22.989	149	45504	3.162	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
Data File : BG051320.D
Acq On : 3 Dec 2021 2:38
Operator : CG/JU
Sample : M4868-07DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKP2DL

Quant Time: Dec 03 03:19:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 24 06:04:50 2021
Response via : Initial Calibration




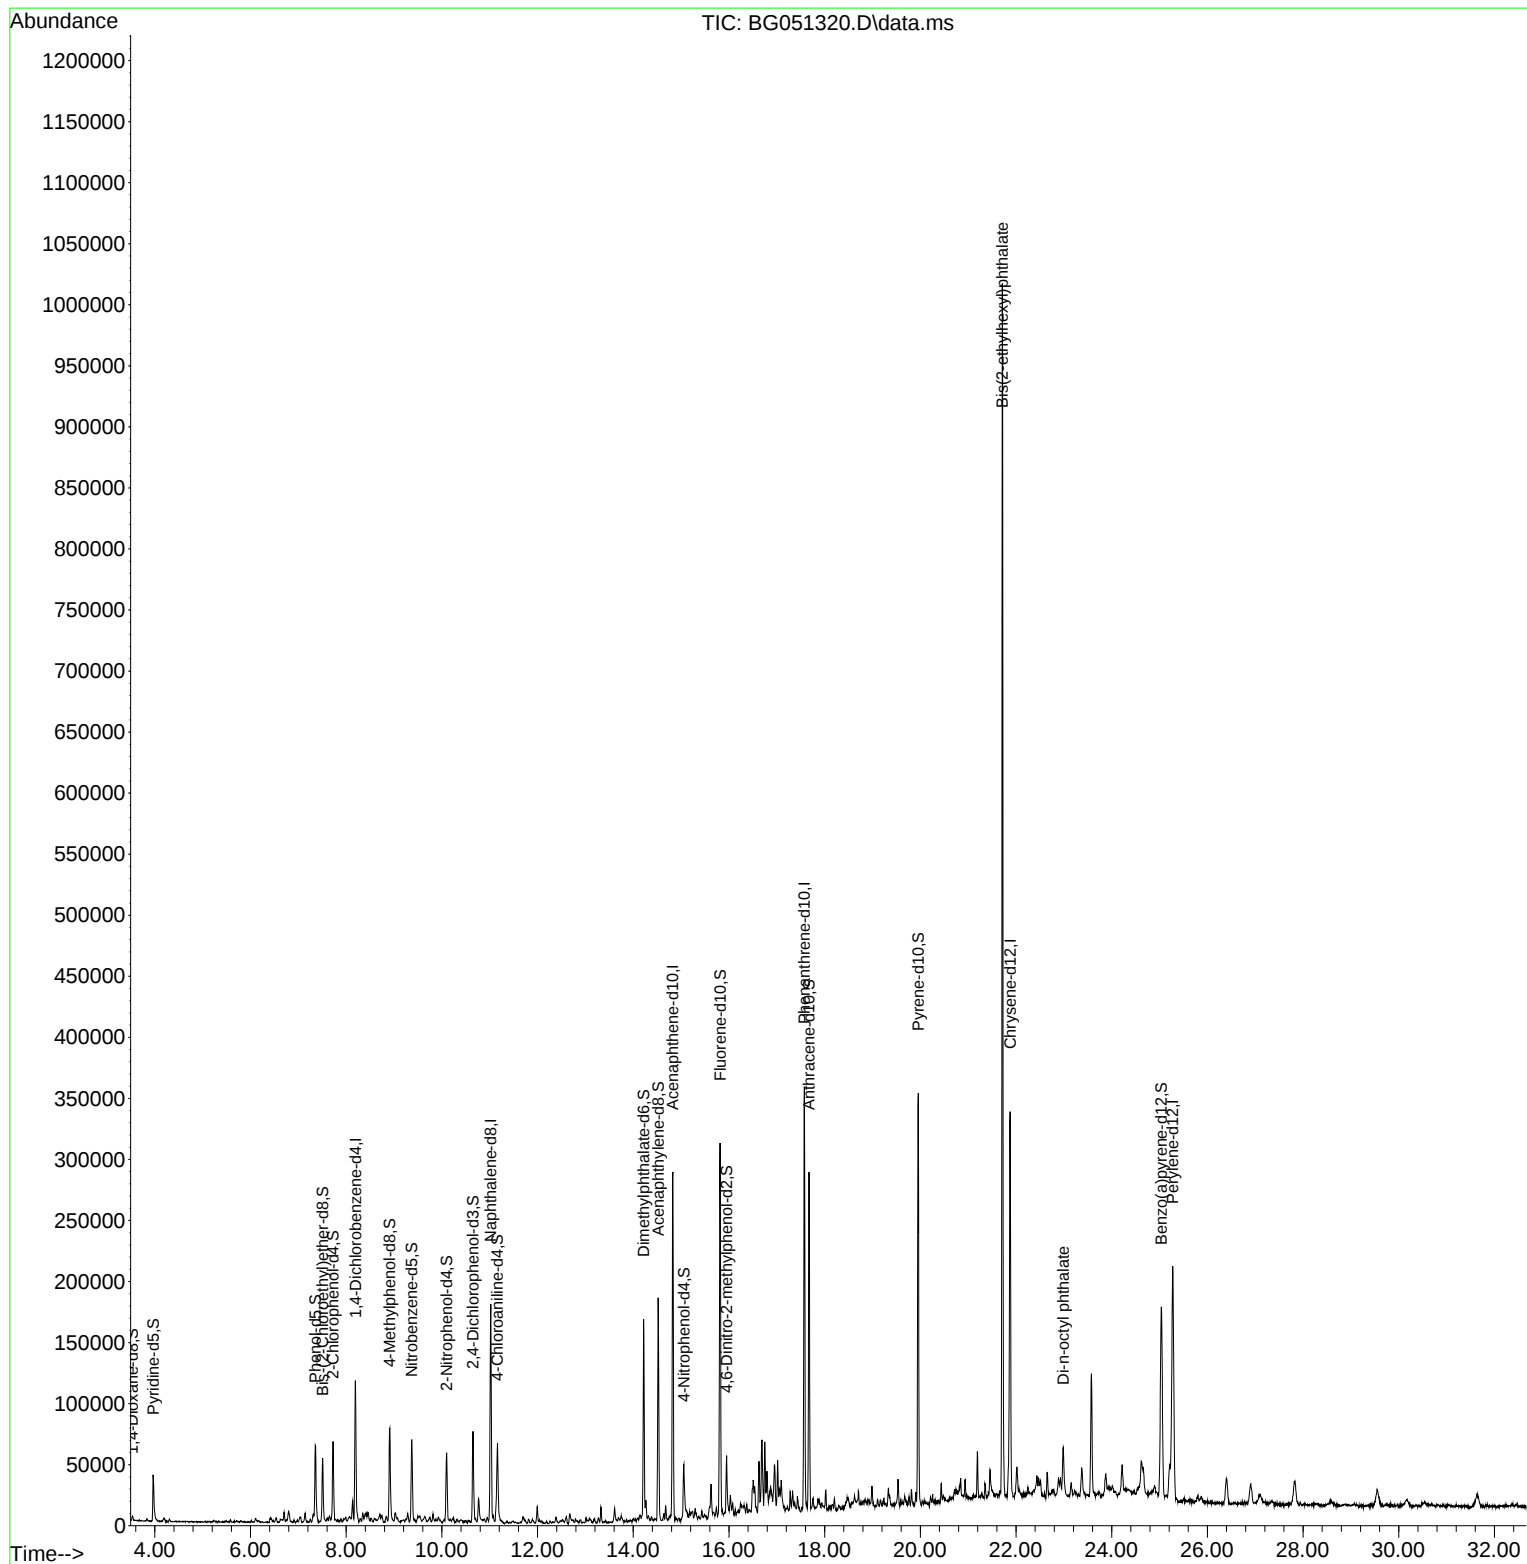


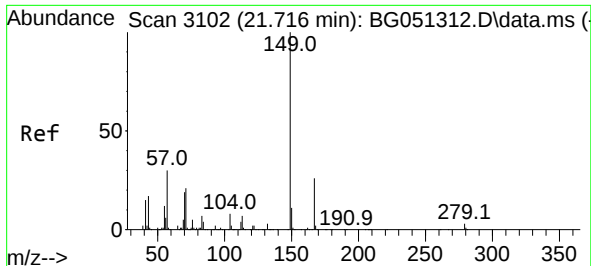

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 49.395 ng/ul
 RT: 21.714 min Scan# 3102
 Delta R.T. -0.009 min
 Lab File: BG051320.D
 Acq: 3 Dec 2021 2:38

Instrument :
 BNA_G
 ClientSampleId :
 BGKP2DL

Tgt Ion:149 Resp: 418282
 Ion Ratio Lower Upper
 149 100
 167 26.0 21.1 31.7
 279 3.6 2.7 4.1

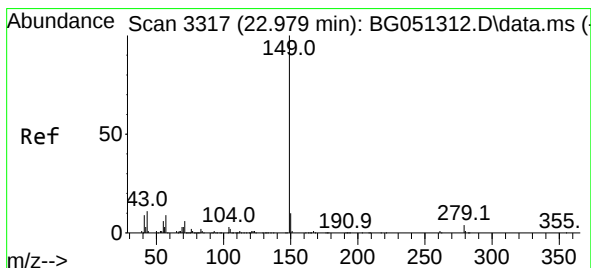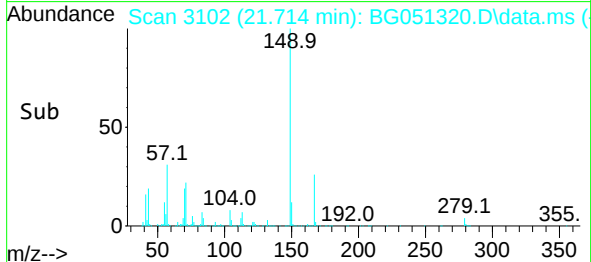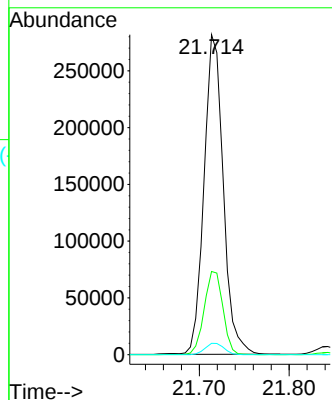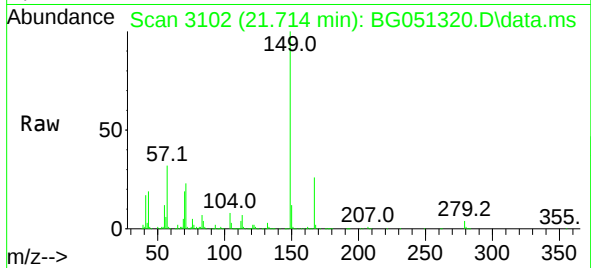

#89
 Di-n-octyl phthalate
 Concen: 3.162 ng/ul
 RT: 22.989 min Scan# 3319
 Delta R.T. 0.003 min
 Lab File: BG051320.D
 Acq: 3 Dec 2021 2:38

Tgt Ion:149 Resp: 45504

