

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
 Data File : BG051332.D
 Acq On : 3 Dec 2021 16:41
 Operator : CG/JU
 Sample : M4833-20
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESQN7

Quant Time: Dec 03 23:36:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 03 15:23:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.193	152	31823	20.000	ng/u1	0.00
20) Naphthalene-d8	11.019	136	138931	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.821	164	91693	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.570	188	175918	20.000	ng/u1	0.00
79) Chrysene-d12	21.877	240	146485	20.000	ng/u1	0.00
88) Perylene-d12	25.285	264	146290	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.528	96	3457	3.775	ng/uL	-0.02
4) Pyridine-d5	3.963	84	39139	14.565	ng/u1	-0.02
7) Phenol-d5	7.353	99	73904	23.498	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.506	67	48035	24.318	ng/u1	0.00
11) 2-Chlorophenol-d4	7.723	132	55732	24.608	ng/u1	0.00
15) 4-Methylphenol-d8	8.904	113	53365	21.026	ng/u1	0.00
21) Nitrobenzene-d5	9.368	128	29750	25.367	ng/u1	0.00
24) 2-Nitrophenol-d4	10.091	143	34097	25.774	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.649	165	55502	24.727	ng/u1	0.00
31) 4-Chloroaniline-d4	11.160	131	49885	15.189	ng/u1	0.00
46) Dimethylphthalate-d6	14.216	166	184308	26.124	ng/u1	0.00
49) Acenaphthylene-d8	14.521	160	238489	26.807	ng/u1	0.00
54) 4-Nitrophenol-d4	15.050	143	25855	22.640	ng/u1	0.00
60) Fluorene-d10	15.814	176	169963	26.752	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.943	200	21916	20.189	ng/u1	0.00
73) Anthracene-d10	17.670	188	243244	28.911	ng/u1	0.00
81) Pyrene-d10	19.956	212	266691	30.089	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.050	264	232589	29.770	ng/u1	0.00
Target Compounds						
83) Butylbenzylphthalate	20.843	149	7345	1.659	ng/u1#	Qvalue 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
Data File : BG051332.D
Acq On : 3 Dec 2021 16:41
Operator : CG/JU
Sample : M4833-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ESQN7

Quant Time: Dec 03 23:36:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 03 15:23:09 2021
Response via : Initial Calibration

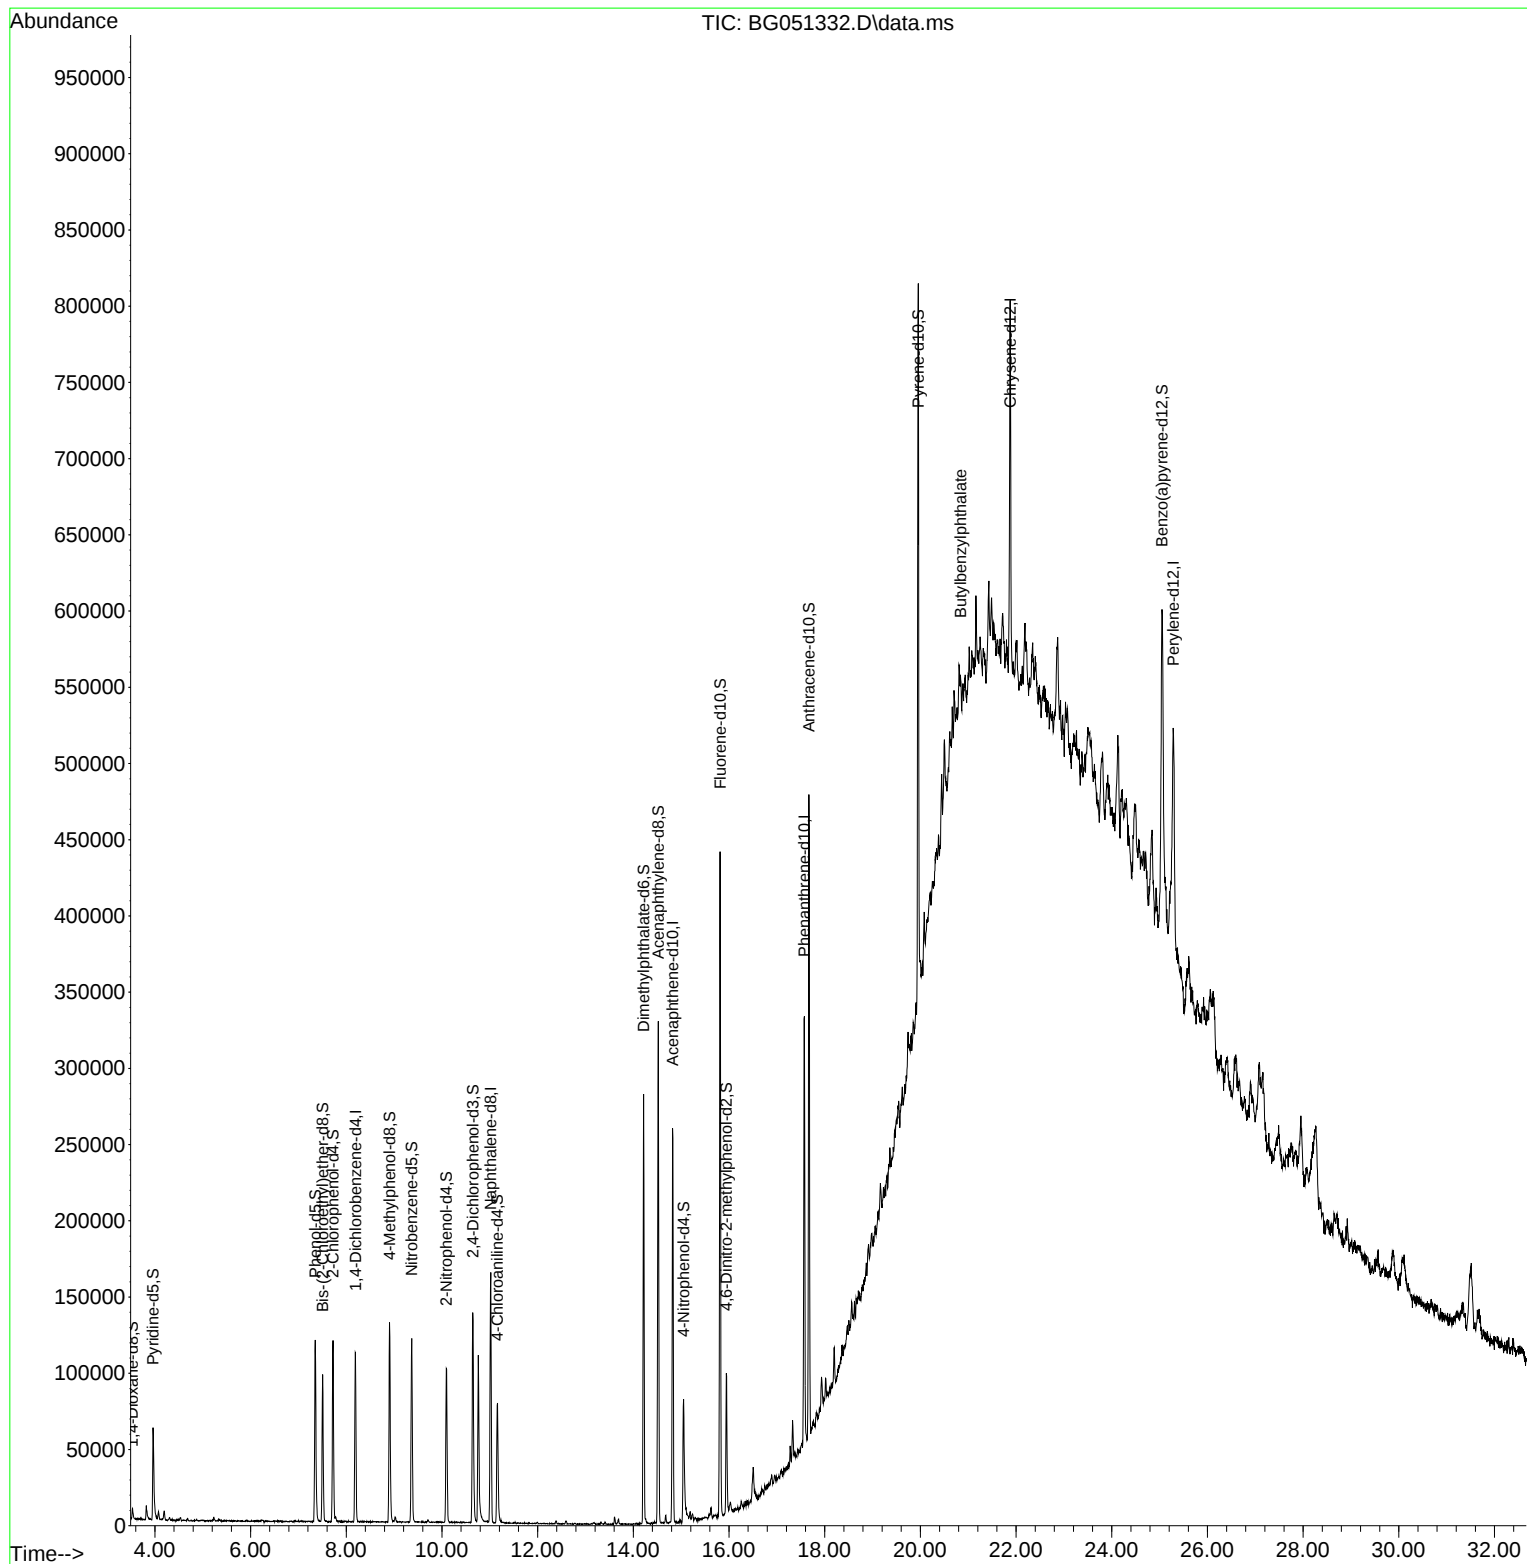

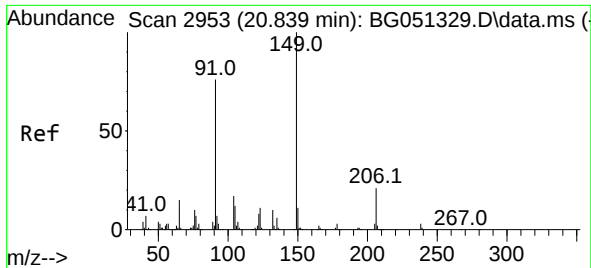

#83
 Butylbenzylphthalate
 Concen: 1.659 ng/ul
 RT: 20.843 min Scan# 2954
 Delta R.T. -0.004 min
 Lab File: BG051332.D
 Acq: 3 Dec 2021 16:41

Instrument :
 BNA_G
 ClientSampleId :
 ESQN7

Tgt Ion:149 Resp: 7345
 Ion Ratio Lower Upper
 149 100
 91 120.1 65.2 97.8#
 206 24.9 16.2 24.2#

