

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
 Data File : BG051337.D
 Acq On : 3 Dec 2021 20:07
 Operator : CG/JU
 Sample : M4833-13
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESQN0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/06/2021
 Supervised By :mohammad ahmed 12/07/2021

Quant Time: Dec 03 23:37:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 03 15:23:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.191	152	31186	20.000	ng/u1	-0.01
20) Naphthalene-d8	11.017	136	131871	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.825	164	86700	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.574	188	182261	20.000	ng/u1	0.00
79) Chrysene-d12	21.875	240	154256	20.000	ng/u1	0.00
88) Perylene-d12	25.277	264	153422	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.532	96	3395m	3.783	ng/uL	-0.01
4) Pyridine-d5	3.967	84	36609	13.902	ng/u1	-0.01
7) Phenol-d5	7.351	99	70307	22.810	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.504	67	46202	23.867	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.721	132	52836	23.805	ng/u1	-0.01
15) 4-Methylphenol-d8	8.908	113	50379	20.255	ng/u1	0.00
21) Nitrobenzene-d5	9.372	128	28210	25.342	ng/u1	0.00
24) 2-Nitrophenol-d4	10.095	143	32833	26.147	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.647	165	53216	24.978	ng/u1	0.00
31) 4-Chloroaniline-d4	11.158	131	50055	16.057	ng/u1	0.00
46) Dimethylphthalate-d6	14.214	166	173300	25.978	ng/u1	-0.01
49) Acenaphthylene-d8	14.519	160	223413	26.559	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.048	143	23897m	22.130	ng/u1	0.00
60) Fluorene-d10	15.812	176	157511	26.220	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.947	200	17087	15.193	ng/u1	0.00
73) Anthracene-d10	17.674	188	242146	27.779	ng/u1	0.00
81) Pyrene-d10	19.954	212	293347	31.429	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.042	264	246741	30.113	ng/u1	0.00
Target Compounds						
					Qvalue	
72) Phenanthrene	17.616	178	11420	1.135	ng/u1	97
80) Fluoranthene	19.619	202	28478	2.484	ng/u1	97
82) Pyrene	19.983	202	25316	2.258	ng/u1	98
85) Benzo(a)anthracene	21.858	228	12838	1.227	ng/u1	96
86) Bis(2-ethylhexyl)phtha...	21.711	149	9531	1.421	ng/u1	97
87) Chrysene	21.922	228	13419	1.335	ng/u1	93
90) Benzo(b)fluoranthene	24.190	252	16048	1.550	ng/u1#	89
93) Benzo(a)pyrene	25.107	252	11932	1.208	ng/u1#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
 Data File : BG051337.D
 Acq On : 3 Dec 2021 20:07
 Operator : CG/JU
 Sample : M4833-13
 Misc :
 ALS Vial : 42 Sample Multiplier: 1


Instrument :
 BNA_G
 ClientSampleId :
 ESQN0

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 12/06/2021
 Supervised By :mohammad ahmed 12/07/2021


Quant Time: Dec 03 23:37:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 03 15:23:09 2021
 Response via : Initial Calibration

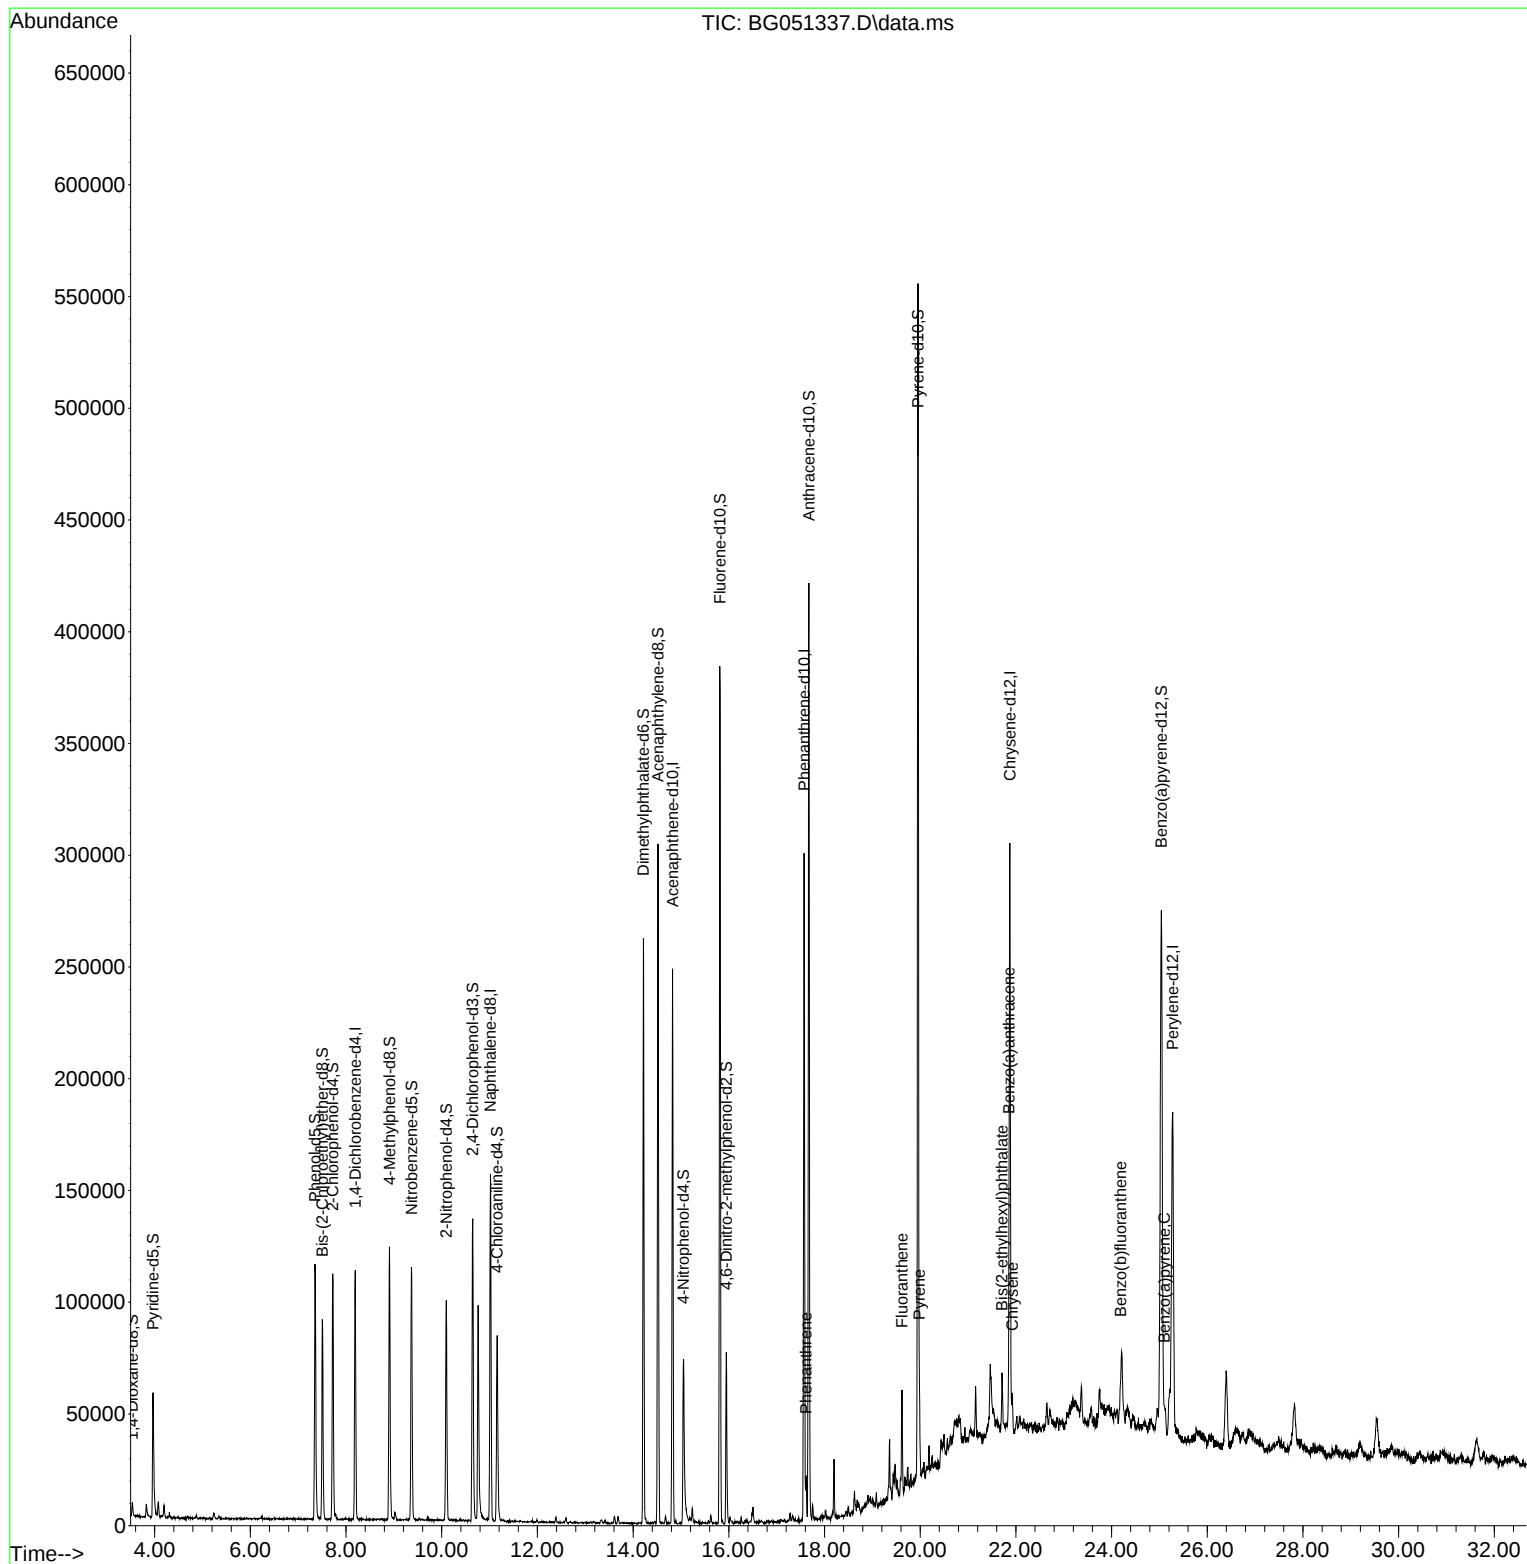

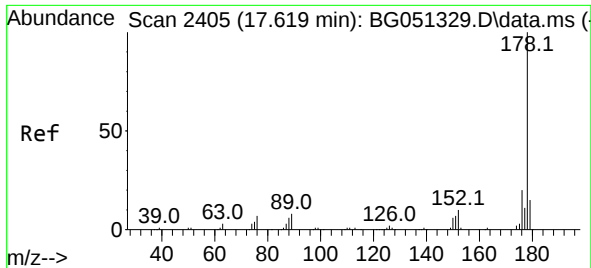

#72
Phenanthrene
Concen: 1.135 ng/ul
RT: 17.616 min Scan# 2404
Delta R.T. -0.006 min
Lab File: BG051337.D
Acq: 3 Dec 2021 20:07




Instrument :
BNA_G
ClientSampleId :
ESQN0

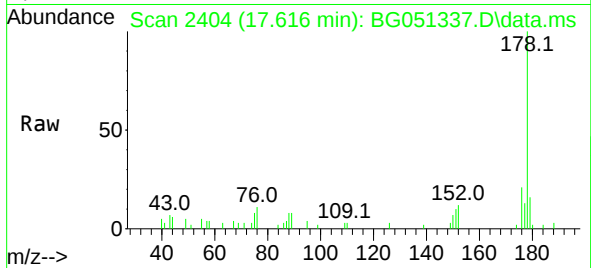


Tgt Ion:178 Resp: 11420
Ion Ratio Lower Upper
178 100
179 16.0 12.3 18.5
176 21.2 15.5 23.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/06/2021
Supervised By :mohammad ahmed 12/07/2021

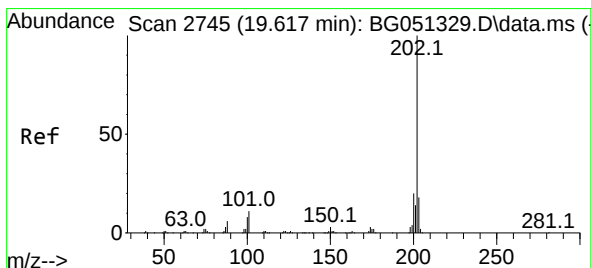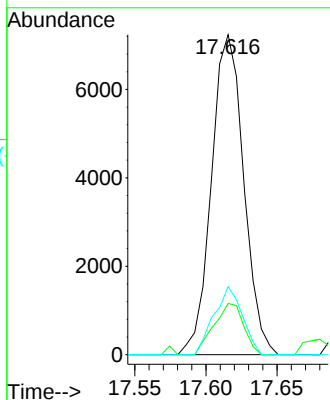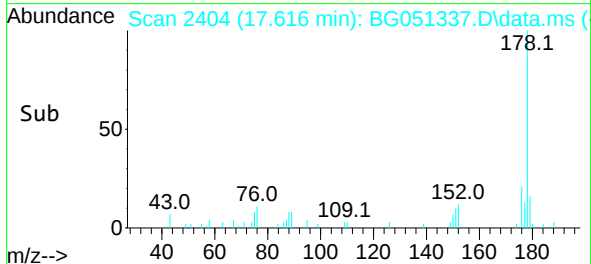


#80
Fluoranthene
Concen: 2.484 ng/ul
RT: 19.619 min Scan# 2745
Delta R.T. -0.006 min
Lab File: BG051337.D
Acq: 3 Dec 2021 20:07

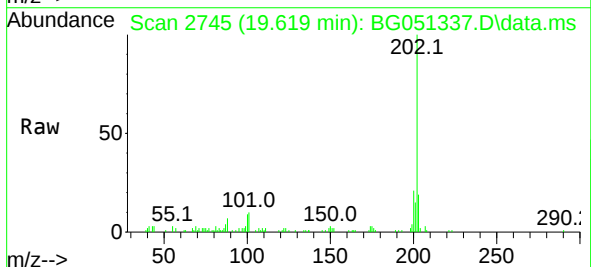


Tgt Ion:202 Resp: 28478
Ion Ratio Lower Upper
202 100
101 9.8 9.3 13.9
100 8.7 7.0 10.6

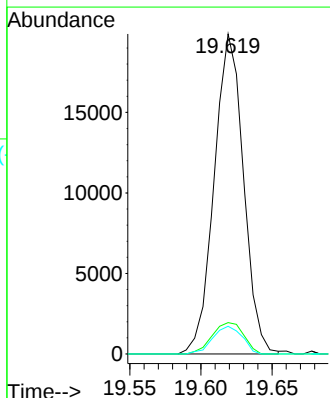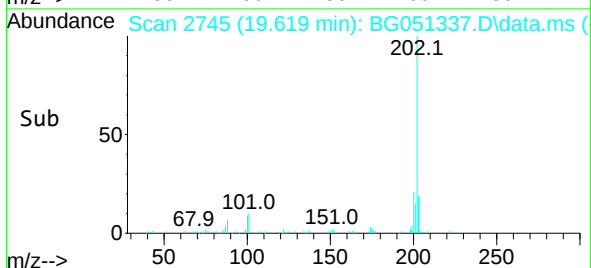

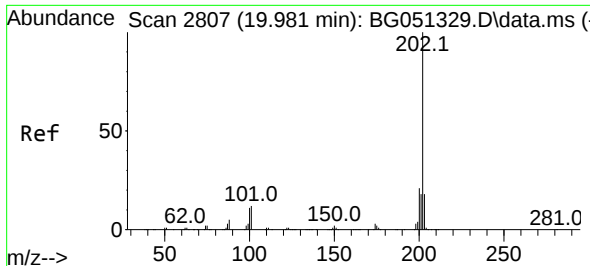

#82
Pyrene
Concen: 2.258 ng/ul
RT: 19.983 min Scan# 2807
Delta R.T. -0.006 min
Lab File: BG051337.D
Acq: 3 Dec 2021 20:07




Instrument :
BNA_G
ClientSampleId :
ESQN0

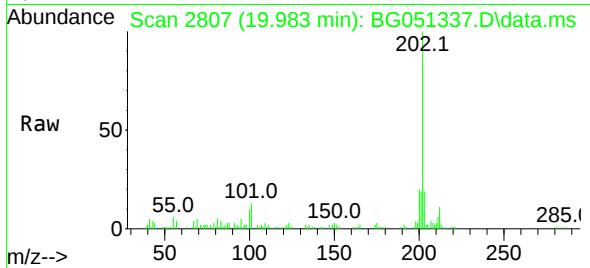

Tgt Ion:202 Resp: 25310
Ion Ratio Lower Upper
202 100
101 12.8 10.7 16.1
100 10.3 9.0 13.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/06/2021
Supervised By :mohammad ahmed 12/07/2021

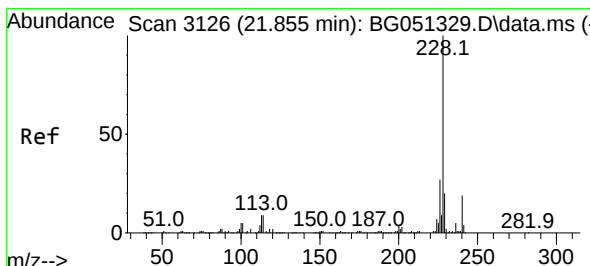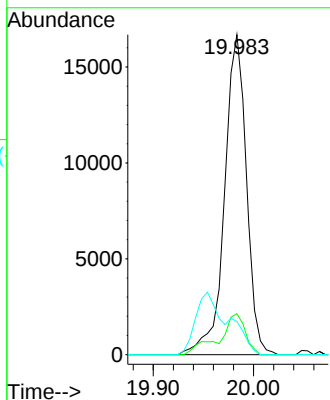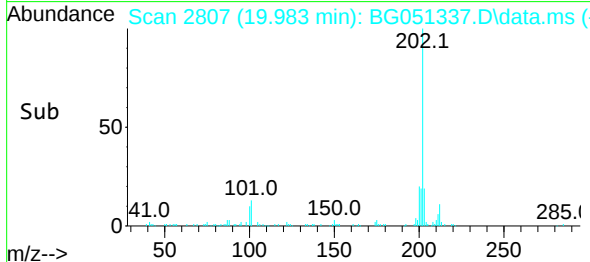

#85
Benzo(a)anthracene
Concen: 1.227 ng/ul
RT: 21.858 min Scan# 3126
Delta R.T. -0.006 min
Lab File: BG051337.D
Acq: 3 Dec 2021 20:07


Tgt Ion:228 Resp: 12838
Ion Ratio Lower Upper
228 100
229 20.6 15.7 23.5
226 24.8 22.3 33.5

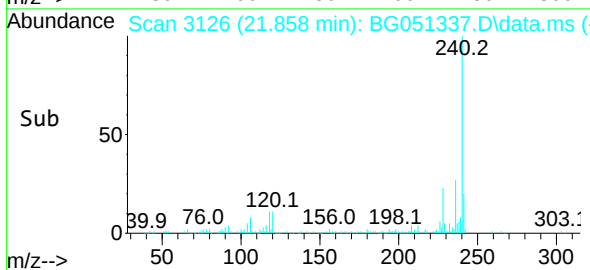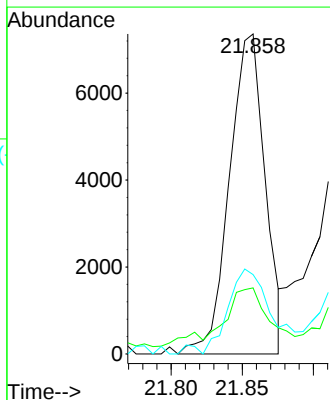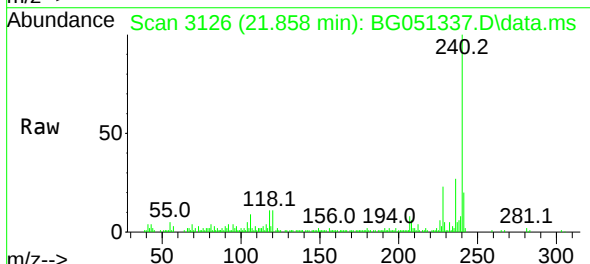

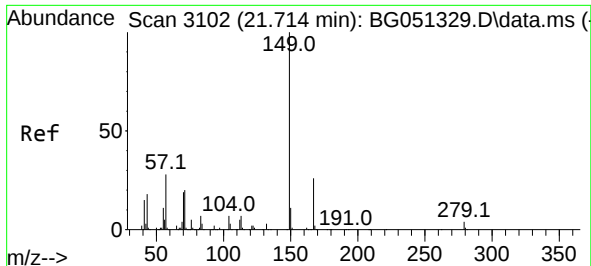

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.421 ng/ul
RT: 21.711 min Scan# 3102
Delta R.T. -0.012 min
Lab File: BG051337.D
Acq: 3 Dec 2021 20:07




Instrument :
BNA_G
ClientSampleId :
ESQN0

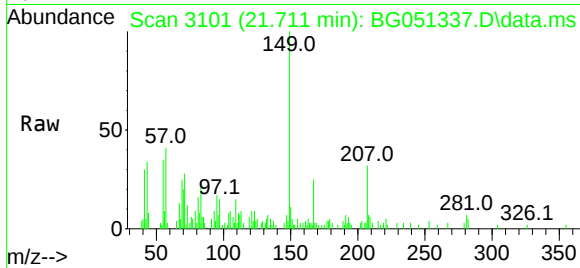

Tgt Ion:149 Resp: 953
Ion Ratio Lower Upper
149 100
167 24.7 21.1 31.7
279 3.5 2.7 4.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/06/2021
Supervised By :mohammad ahmed 12/07/2021

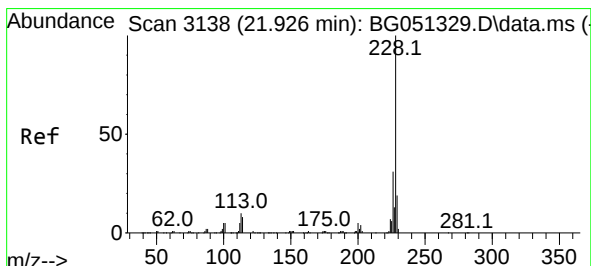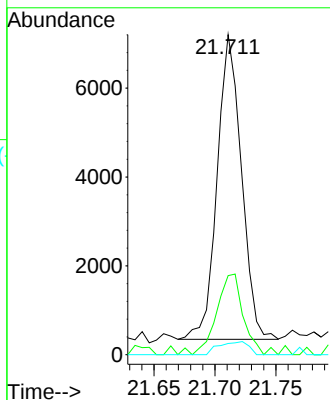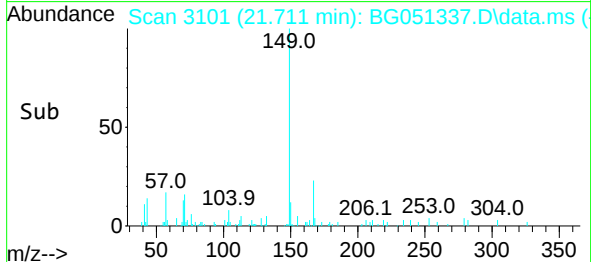

#87
Chrysene
Concen: 1.335 ng/ul
RT: 21.922 min Scan# 3137
Delta R.T. -0.012 min
Lab File: BG051337.D
Acq: 3 Dec 2021 20:07

Tgt Ion:228 Resp: 13419
Ion Ratio Lower Upper
228 100
226 27.1 24.8 37.2
229 22.9 15.8 23.6

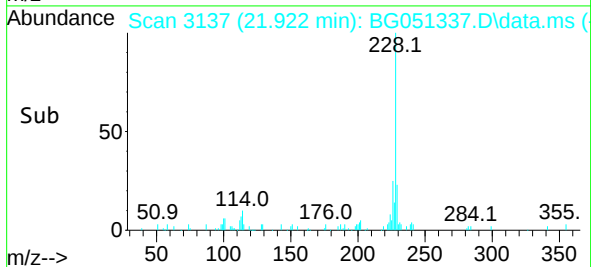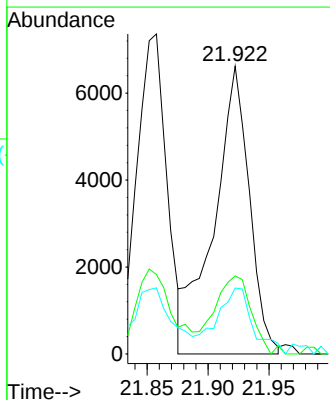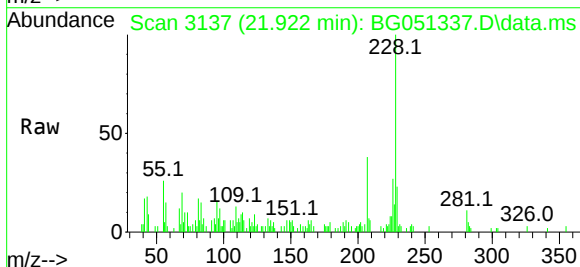

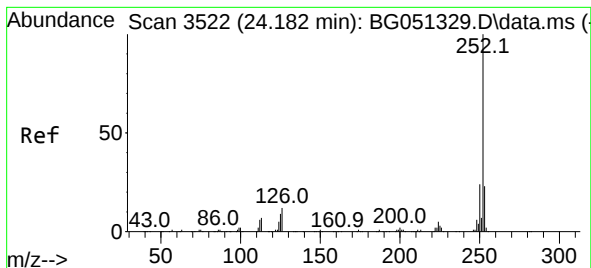

#90

Benzo(b)fluoranthene

Concen: 1.550 ng/ul

RT: 24.190 min Scan# 3523

Delta R.T. 0.000 min

Lab File: BG051337.D

Acq: 3 Dec 2021 20:07

Instrument :

BNL_G

ClientSampleId :

ESQ00





Tgt Ion:252 Resp: 1604

Ion	Ratio	Lower	Upper
252	100		
253	24.6	17.8	26.6
125	19.5	8.5	12.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/06/2021
Supervised By :mohammad ahmed 12/07/2021

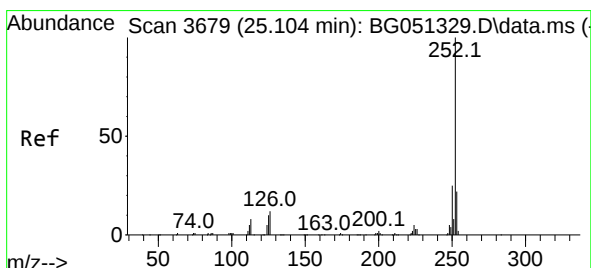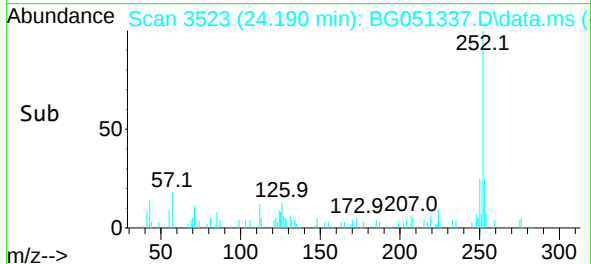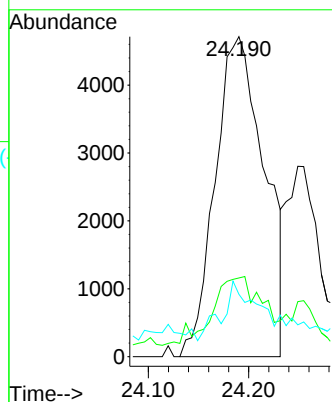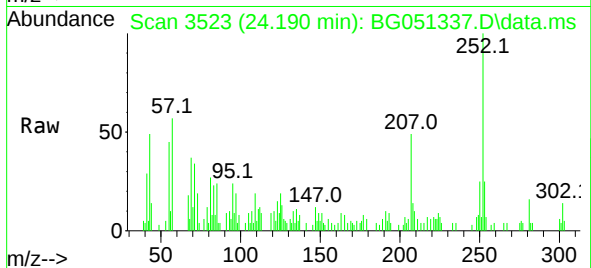

#93

Benzo(a)pyrene

Concen: 1.208 ng/ul

RT: 25.107 min Scan# 3679

Delta R.T. -0.018 min

Lab File: BG051337.D

Acq: 3 Dec 2021 20:07

Tgt Ion:252 Resp: 11932

Ion	Ratio	Lower	Upper
252	100		
253	21.9	17.4	26.2
125	15.2	9.1	13.7

