

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
 Data File : BG051313.D
 Acq On : 2 Dec 2021 21:50
 Operator : CG/JU
 Sample : PB141106BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.531	3	7	13	rVB2	9055	13346	1.35%	0.126%
2	3.965	76	81	95	rBV	114347	213309	21.58%	2.015%
3	4.312	137	140	144	rVB3	2173	2991	0.30%	0.028%
4	6.850	569	572	575	rBV	888	1181	0.12%	0.011%
5	6.997	596	597	602	rBV2	767	1007	0.10%	0.010%
6	7.232	632	637	639	rVV2	616	1034	0.10%	0.010%
7	7.356	651	658	674	rVB	150535	273667	27.69%	2.586%
8	7.508	676	684	695	rBV	119966	206421	20.89%	1.950%
9	7.726	714	721	731	rVB	148624	256073	25.91%	2.420%
10	7.990	764	766	770	rBV2	618	1086	0.11%	0.010%
11	8.196	793	801	811	rVB	117754	204809	20.72%	1.935%
12	8.907	915	922	937	rBV	183517	339978	34.40%	3.212%
13	9.371	993	1001	1012	rBV	150984	272102	27.53%	2.571%
14	10.099	1118	1125	1135	rVB	131012	235864	23.87%	2.229%
15	10.646	1212	1218	1233	rBV	166570	325994	32.99%	3.080%
16	11.022	1274	1282	1292	rVB	176950	326135	33.00%	3.082%
17	11.163	1298	1306	1323	rVB	177464	350855	35.50%	3.315%
18	12.608	1545	1552	1556	rBV3	2598	4838	0.49%	0.046%
19	14.218	1820	1826	1838	rVB	354209	533334	53.97%	5.039%
20	14.524	1871	1878	1890	rBV	416009	660263	66.81%	6.239%
21	14.823	1923	1929	1939	rBV	294742	473260	47.89%	4.472%
22	15.052	1962	1968	1983	rBV2	87675	201155	20.35%	1.901%
23	15.816	2091	2098	2108	rVB	520294	810506	82.01%	7.658%
24	15.951	2116	2121	2134	rBV	105614	170637	17.27%	1.612%
25	16.057	2134	2139	2144	rVB3	1714	2207	0.22%	0.021%
26	17.367	2357	2362	2366	rVB2	891	1551	0.16%	0.015%
27	17.579	2391	2398	2404	rBV	373199	583352	59.03%	5.512%
28	17.673	2407	2414	2425	rVV2	563677	888782	89.93%	8.398%
29	18.513	2553	2557	2559	rBV2	892	1086	0.11%	0.010%
30	18.642	2574	2579	2580	rBV3	878	1120	0.11%	0.011%
31	18.766	2596	2600	2602	rBV2	988	1288	0.13%	0.012%
32	19.007	2634	2641	2642	rVV3	843	1494	0.15%	0.014%
33	19.095	2651	2656	2659	rBV3	1033	1573	0.16%	0.015%
34	19.318	2691	2694	2696	rBV4	1254	1360	0.14%	0.013%
35	19.465	2717	2719	2723	rVB4	931	1240	0.13%	0.012%
36	19.524	2725	2729	2733	rBV5	8019	11873	1.20%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
 Data File : BG051313.D
 Acq On : 2 Dec 2021 21:50
 Operator : CG/JU
 Sample : PB141106BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	19.594	2736	2741	2745	rVV2	6979	10466	1.06%	0.099%
38	19.876	2787	2789	2792	rBV4	1155	1183	0.12%	0.011%
39	19.959	2796	2803	2811	rBV	664283	988267	100.00%	9.338%
40	20.211	2844	2846	2848	rVB3	1312	1012	0.10%	0.010%
41	20.246	2850	2852	2854	rBV3	1285	1437	0.15%	0.014%
42	20.264	2854	2855	2860	rVB5	1524	1749	0.18%	0.017%
43	20.305	2860	2862	2864	rBV3	1311	1508	0.15%	0.014%
44	20.376	2872	2874	2876	rBV2	1851	1833	0.19%	0.017%
45	20.493	2892	2894	2896	rBV3	1385	1291	0.13%	0.012%
46	20.669	2922	2924	2925	rBV2	2944	2056	0.21%	0.019%
47	20.740	2929	2936	2952	rVB6	14174	69306	7.01%	0.655%
48	21.880	3123	3130	3140	rBV	316213	561342	56.80%	5.304%
49	23.378	3380	3385	3387	rBV6	6362	10996	1.11%	0.104%
50	24.224	3524	3529	3533	rVB2	11998	21783	2.20%	0.206%
51	25.041	3657	3668	3681	rVB3	300588	881083	89.15%	8.325%
52	25.211	3693	3697	3698	rBV3	12172	15200	1.54%	0.144%
53	25.276	3699	3708	3720	rVB4	185444	562333	56.90%	5.313%
54	26.398	3895	3899	3908	rVB4	14957	37589	3.80%	0.355%
55	27.826	4135	4142	4144	rBV5	13748	33512	3.39%	0.317%
56	31.510	4767	4769	4772	rBV4	3433	2813	0.28%	0.027%




Sum of corrected areas: 10583530

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
Data File : BG051313.D
Acq On : 2 Dec 2021 21:50
Operator : CG/JU
Sample : PB141106BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK106

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

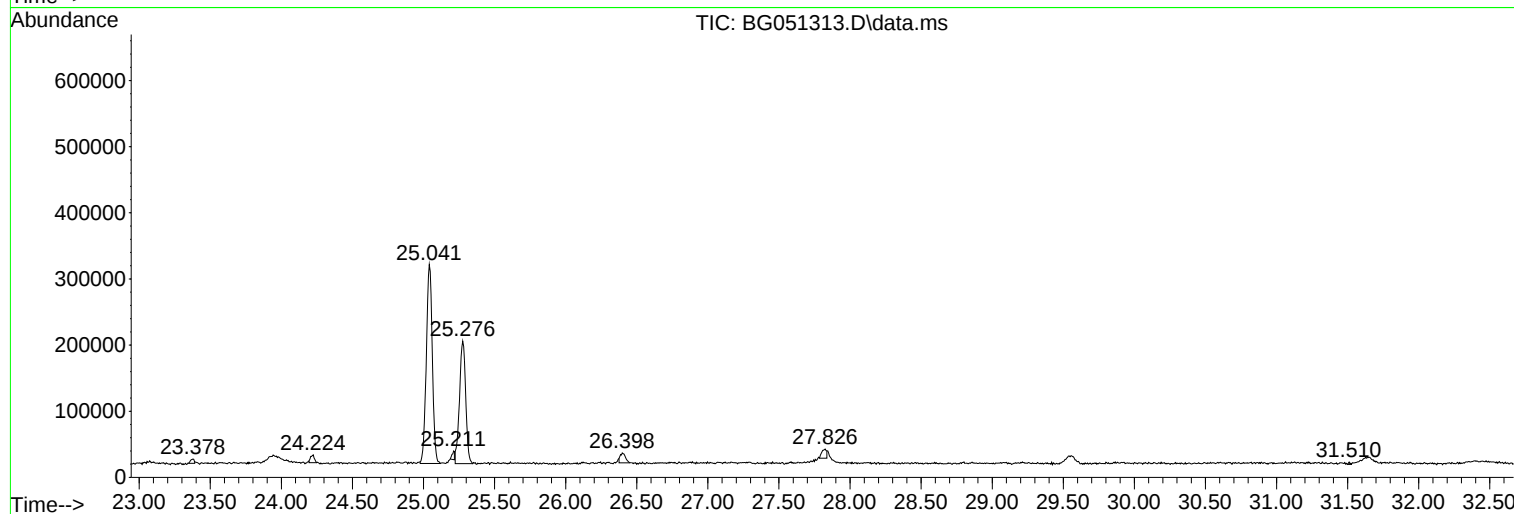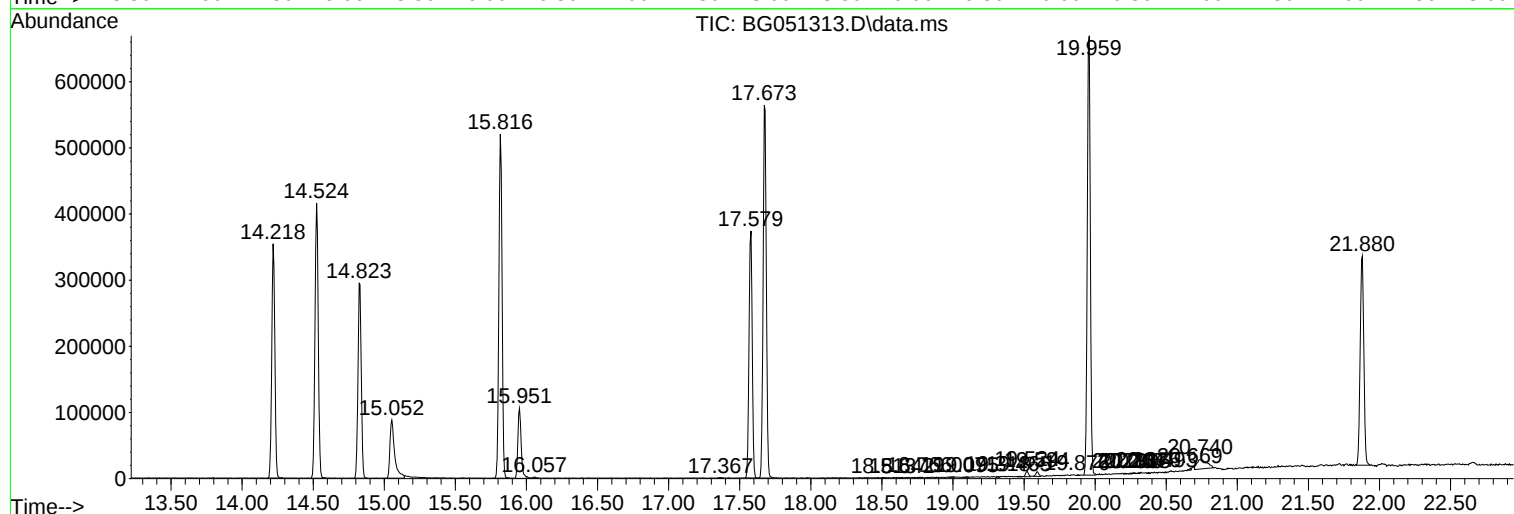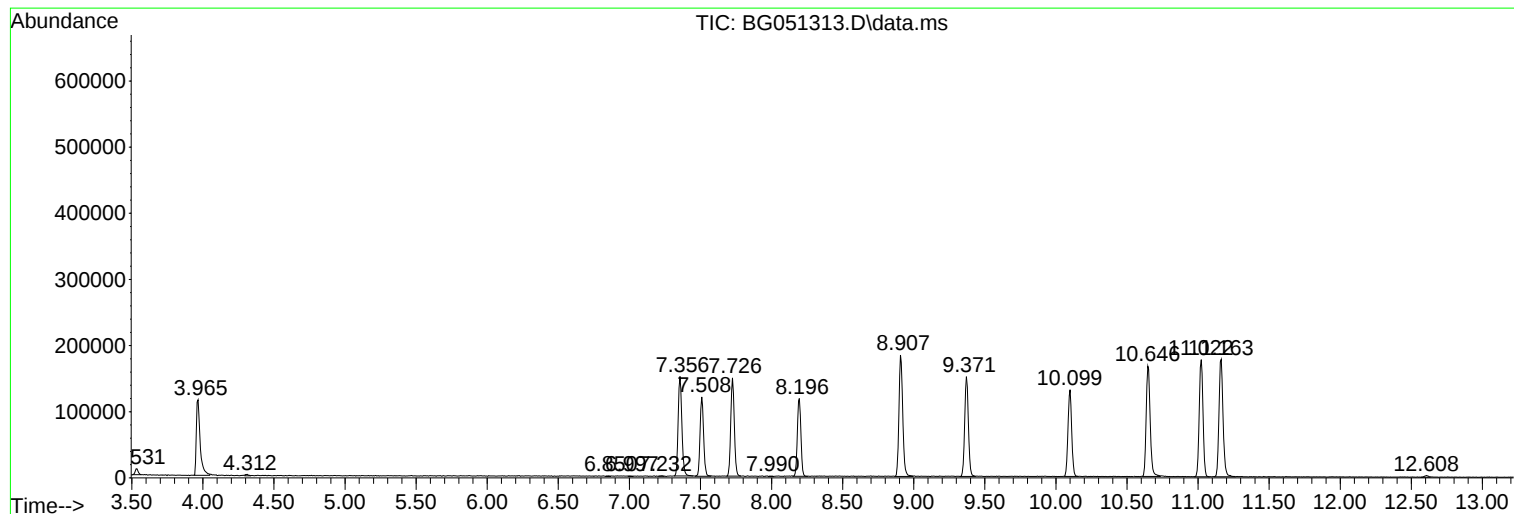

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
Data File : BG051313.D
Acq On : 2 Dec 2021 21:50
Operator : CG/JU
Sample : PB141106BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK106










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.740	2.47 ng/ul	69306	Chrysene-d12	21.880

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Tetratetracontane	619	C44H90	007098-22-8	59
2		Hexadecane, 2,6,10,14-tetramethyl-	282	C20H42	000638-36-8	53
3		2-Bromotetradecane	276	C14H29Br	074036-95-6	50
4		Tridecanol, 2-ethyl-2-methyl-	242	C16H34O	1010115-66-1	50
5		Tetracosane	338	C24H50	000646-31-1	50

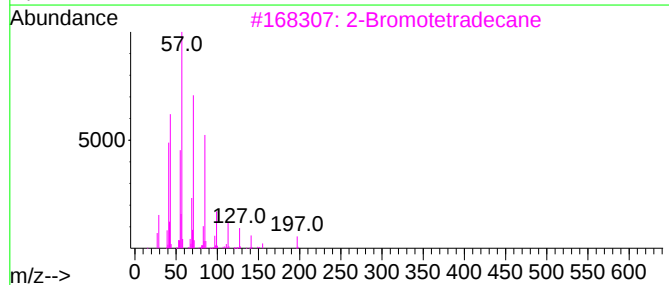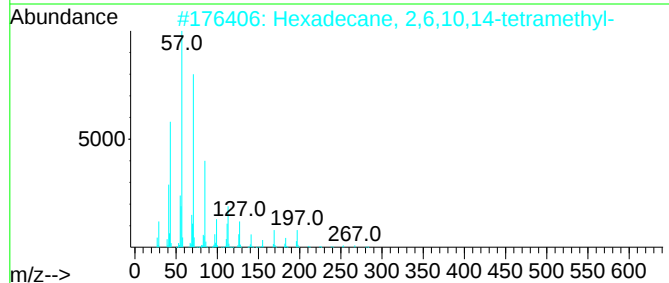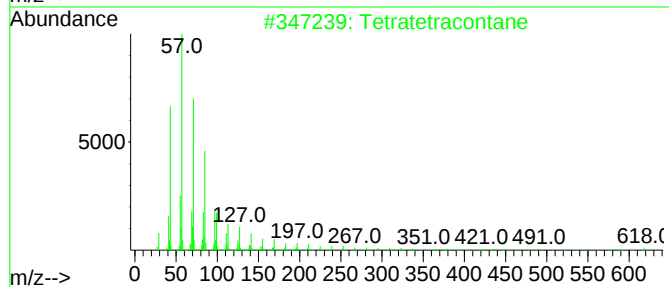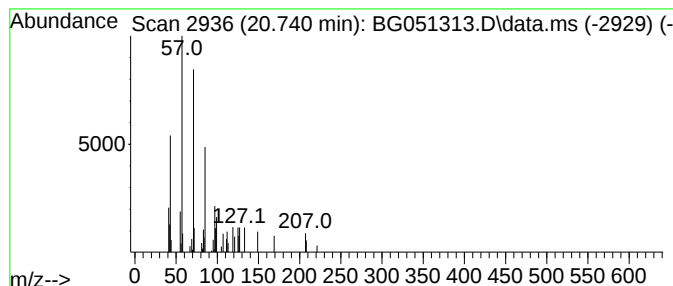

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
Data File : BG051313.D
Acq On : 2 Dec 2021 21:50
Operator : CG/JU
Sample : PB141106BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK106

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.740	2.5	ng/u1	69306	5	21.880	561342	20.0