

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
 Data File : BG051315.D
 Acq On : 2 Dec 2021 23:12
 Operator : CG/JU
 Sample : PB141136BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.534	4	8	15	rVB	9166	14094	1.45%	0.142%
2	3.963	76	81	96	rBV	113631	210321	21.64%	2.126%
3	4.304	134	139	144	rBV4	2432	4267	0.44%	0.043%
4	7.354	651	658	673	rBV	142631	265040	27.27%	2.680%
5	7.506	677	684	697	rVV	114400	200374	20.61%	2.026%
6	7.724	714	721	731	rVB	139039	245643	25.27%	2.484%
7	7.847	741	742	746	rBV2	805	1003	0.10%	0.010%
8	8.194	794	801	810	rVB	103725	177975	18.31%	1.799%
9	8.911	916	923	938	rVB	172442	322193	33.14%	3.257%
10	9.369	994	1001	1014	rVB	143908	260690	26.82%	2.636%
11	10.097	1118	1125	1135	rVB	122824	228035	23.46%	2.306%
12	10.650	1212	1219	1228	rBV	156910	309742	31.86%	3.132%
13	11.020	1274	1282	1291	rVB	158049	285919	29.41%	2.891%
14	11.161	1298	1306	1317	rBV	175549	343338	35.32%	3.471%
15	12.606	1547	1552	1559	rVB2	2136	4065	0.42%	0.041%
16	14.216	1820	1826	1836	rBV	334250	506380	52.09%	5.120%
17	14.522	1871	1878	1889	rBV	391090	626881	64.49%	6.338%
18	14.827	1923	1930	1939	rVB	265848	418104	43.01%	4.227%
19	15.050	1963	1968	1991	rBV	83658	199464	20.52%	2.017%
20	15.814	2092	2098	2110	rVB	477654	770164	79.23%	7.787%
21	15.949	2116	2121	2133	rBV	100382	161713	16.64%	1.635%
22	16.055	2137	2139	2148	rVB4	1989	2610	0.27%	0.026%
23	17.577	2391	2398	2405	rBV	333892	507927	52.25%	5.135%
24	17.677	2408	2415	2426	rBV	555357	863630	88.84%	8.732%
25	18.170	2497	2499	2504	rBV2	599	1142	0.12%	0.012%
26	18.593	2568	2571	2573	rBV3	806	1020	0.10%	0.010%
27	18.963	2632	2634	2637	rBV3	1046	983	0.10%	0.010%
28	19.169	2667	2669	2673	rVB3	1052	1089	0.11%	0.011%
29	19.410	2708	2710	2713	rBV3	1065	1120	0.12%	0.011%
30	19.516	2723	2728	2734	rBV3	7508	10657	1.10%	0.108%
31	19.592	2736	2741	2745	rBV2	7252	10924	1.12%	0.110%
32	19.763	2769	2770	2772	rBV	1283	1023	0.11%	0.010%
33	19.845	2779	2784	2785	rBV5	1948	3080	0.32%	0.031%
34	19.956	2796	2803	2812	rBV	662986	972080	100.00%	9.828%
35	20.221	2847	2848	2850	rBV	1074	1047	0.11%	0.011%
36	20.268	2854	2856	2857	rBV2	1765	1183	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
 Data File : BG051315.D
 Acq On : 2 Dec 2021 23:12
 Operator : CG/JU
 Sample : PB141136BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK136

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	20.432	2882	2884	2885	rVB2	1876	1046	0.11%	0.011%
38	20.468	2885	2890	2894	rBV7	2218	4941	0.51%	0.050%
39	20.526	2898	2900	2901	rBV2	1761	1001	0.10%	0.010%
40	20.609	2912	2914	2916	rBV3	1768	1660	0.17%	0.017%
41	20.685	2922	2927	2928	rBV5	3522	5202	0.54%	0.053%
42	20.738	2931	2936	2944	rVV8	8164	24565	2.53%	0.248%
43	20.849	2953	2955	2957	rVB3	3067	2000	0.21%	0.020%
44	21.584	3078	3080	3083	rBV4	2776	2539	0.26%	0.026%
45	21.878	3123	3130	3137	rBV	284094	494280	50.85%	4.997%
46	22.095	3165	3167	3170	rVB4	3473	2287	0.24%	0.023%
47	23.006	3320	3322	3323	rVB2	3138	1417	0.15%	0.014%
48	23.200	3353	3355	3357	rBV3	2781	1809	0.19%	0.018%
49	23.370	3380	3384	3390	rVB9	7246	13879	1.43%	0.140%
50	25.039	3658	3668	3679	rBV2	295522	849659	87.41%	8.590%
51	25.274	3692	3708	3720	rVB2	158828	511000	52.57%	5.166%
52	26.402	3890	3900	3907	rBV6	11264	36111	3.71%	0.365%
53	30.785	4644	4646	4647	rBV	3881	2569	0.26%	0.026%



Sum of corrected areas: 9890885

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
Data File : BG051315.D
Acq On : 2 Dec 2021 23:12
Operator : CG/JU
Sample : PB141136BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

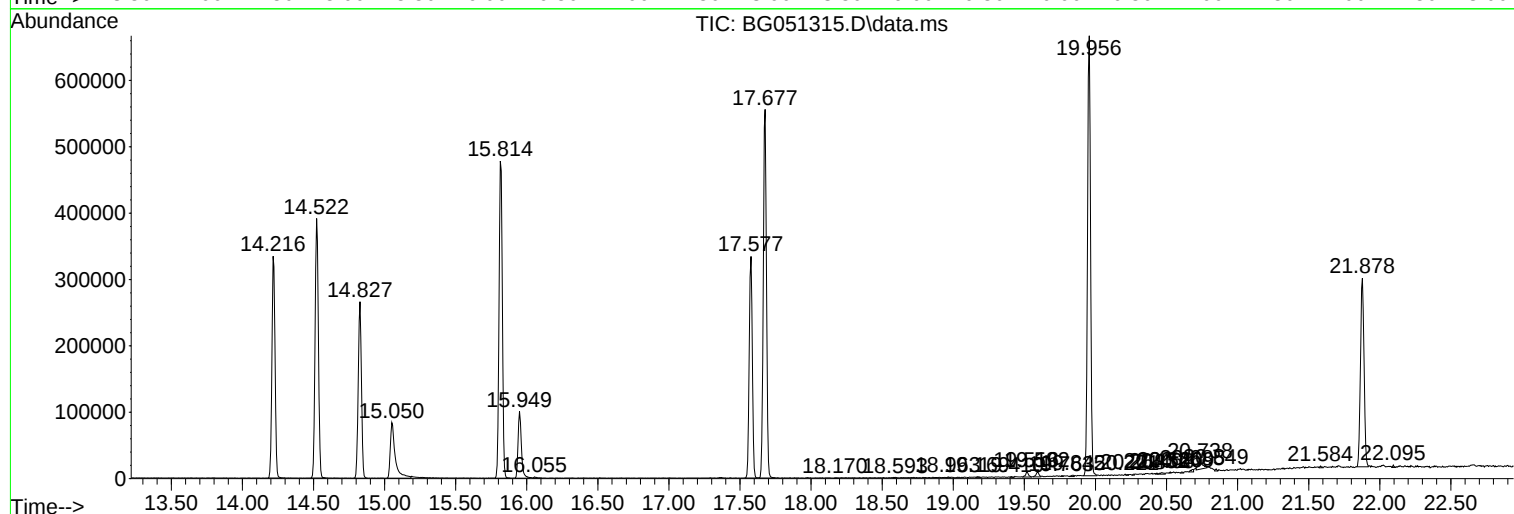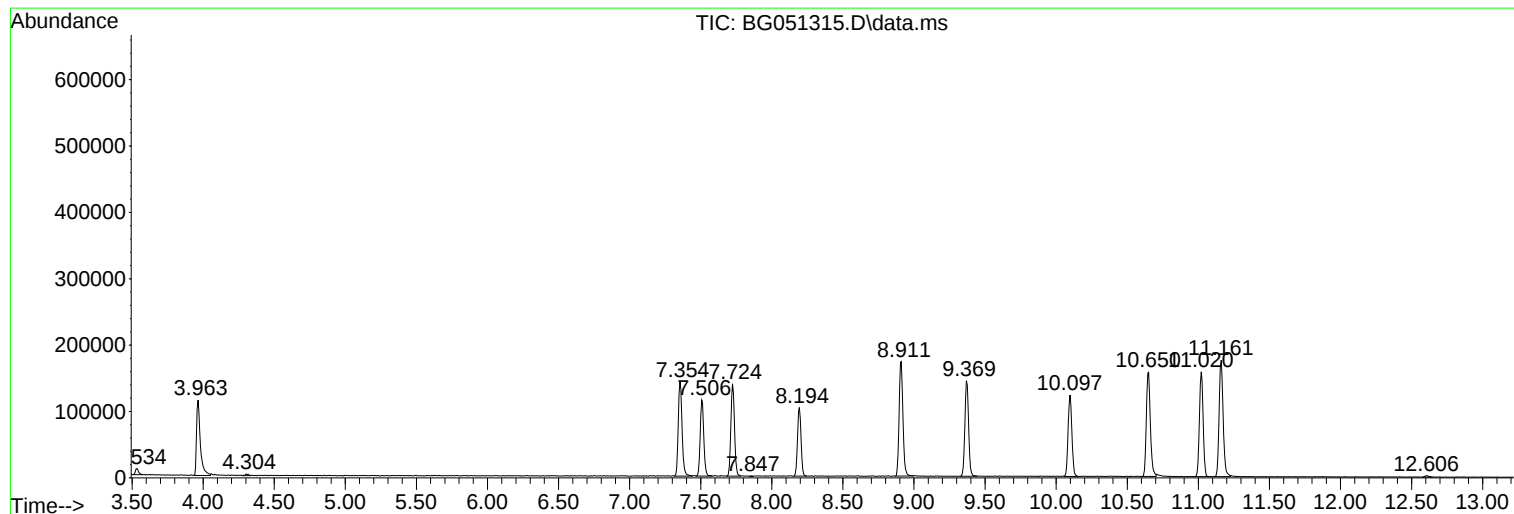

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
Data File : BG051315.D
Acq On : 2 Dec 2021 23:12
Operator : CG/JU
Sample : PB141136BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120221\
Data File : BG051315.D
Acq On : 2 Dec 2021 23:12
Operator : CG/JU
Sample : PB141136BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc