
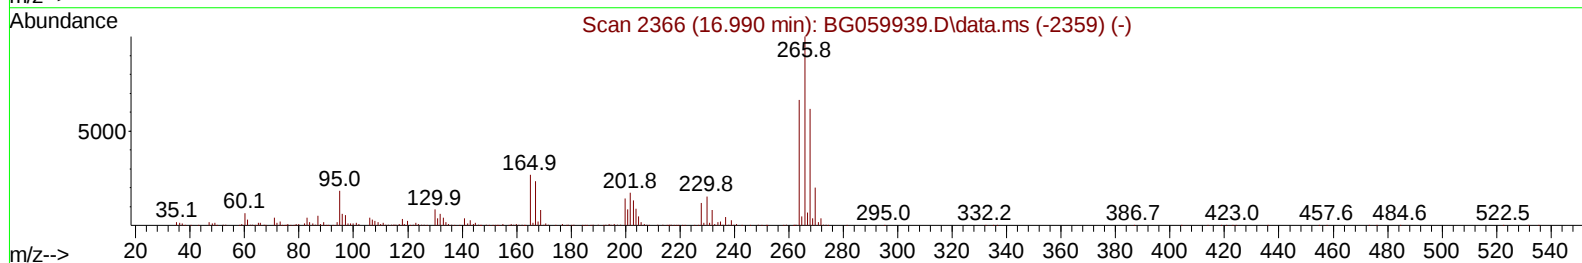
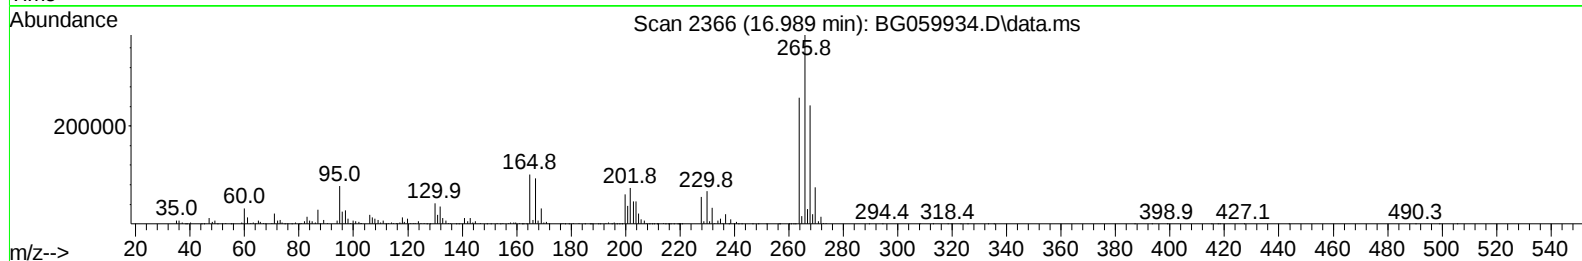


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120423\
Data File : BG059934.D
Acq On : 4 Dec 2023 16:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 03:02:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 02:26:15 2023
Response via : Initial Calibration

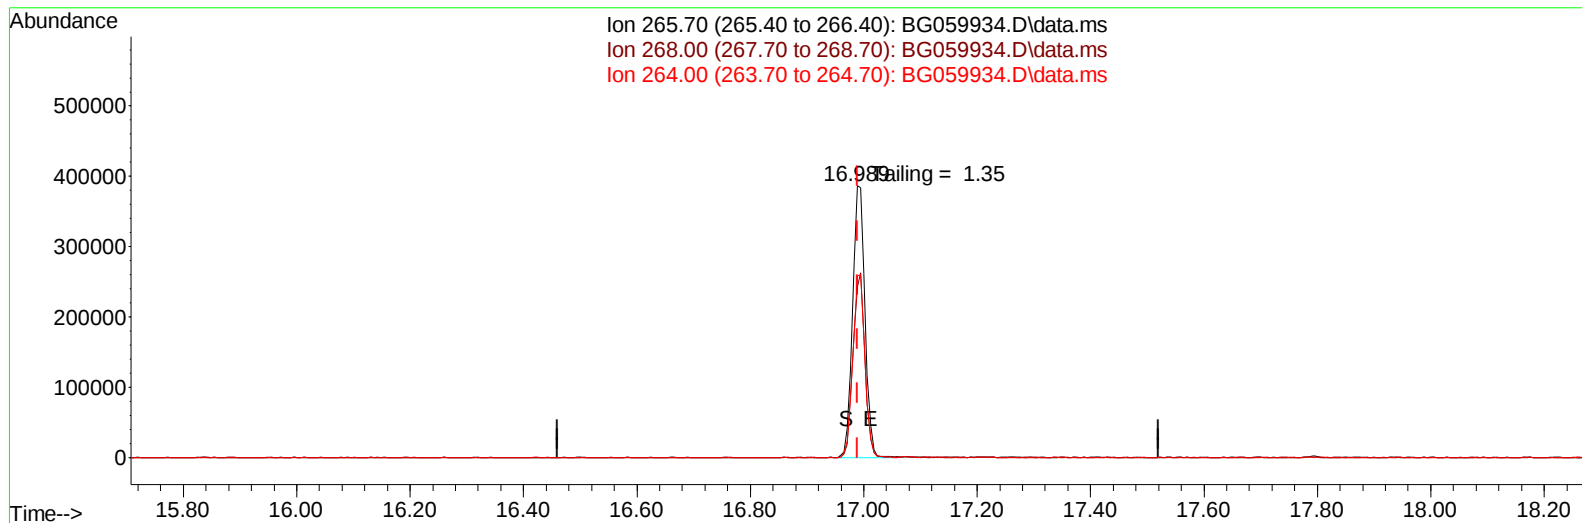

TIC: BG059934.D\data.ms

(70) Pentachlorophenol (C)




16.989min (-0.001) 473344.15 ng

response 587651

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	62.79
264.00	66.50	66.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120423\
Data File : BG059934.D
Acq On : 4 Dec 2023 16:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 03:02:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 02:26:15 2023
Response via : Initial Calibration

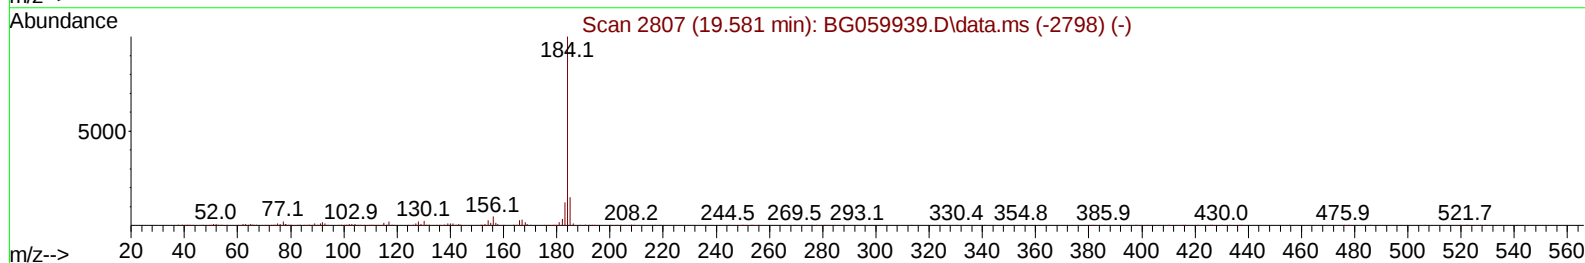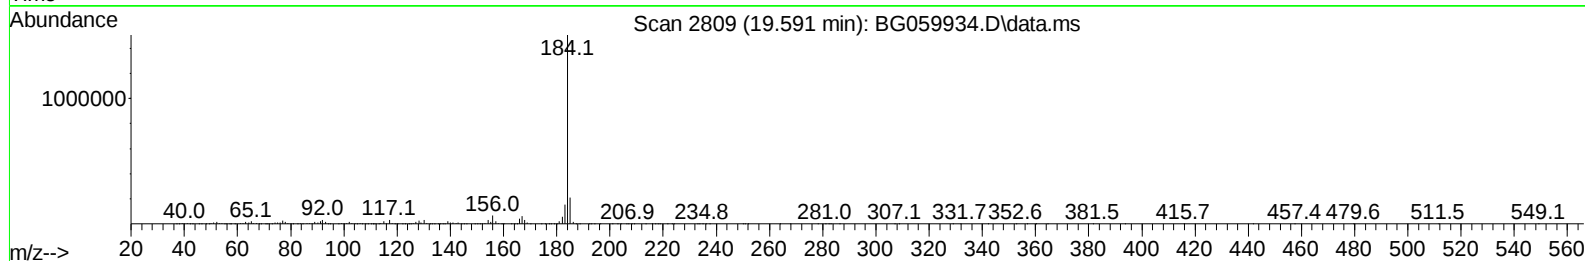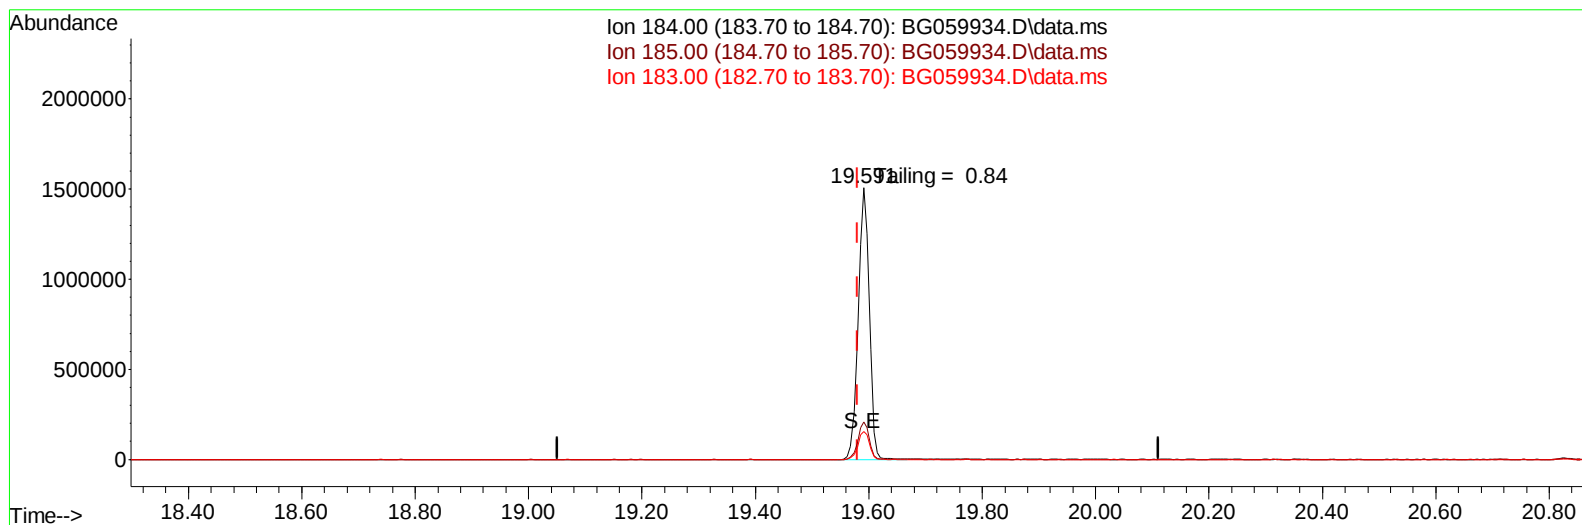

TIC: BG059934.D\data.ms

(77) Benzidine**19.591min (+ 0.010) 2382272.94 ng****response 2047974**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.85
183.00	12.10	10.35
0.00	0.00	0.00