


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120423\
 Data File : BG059934.D
 Acq On : 4 Dec 2023 16:34
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 05 02:26:15 2023

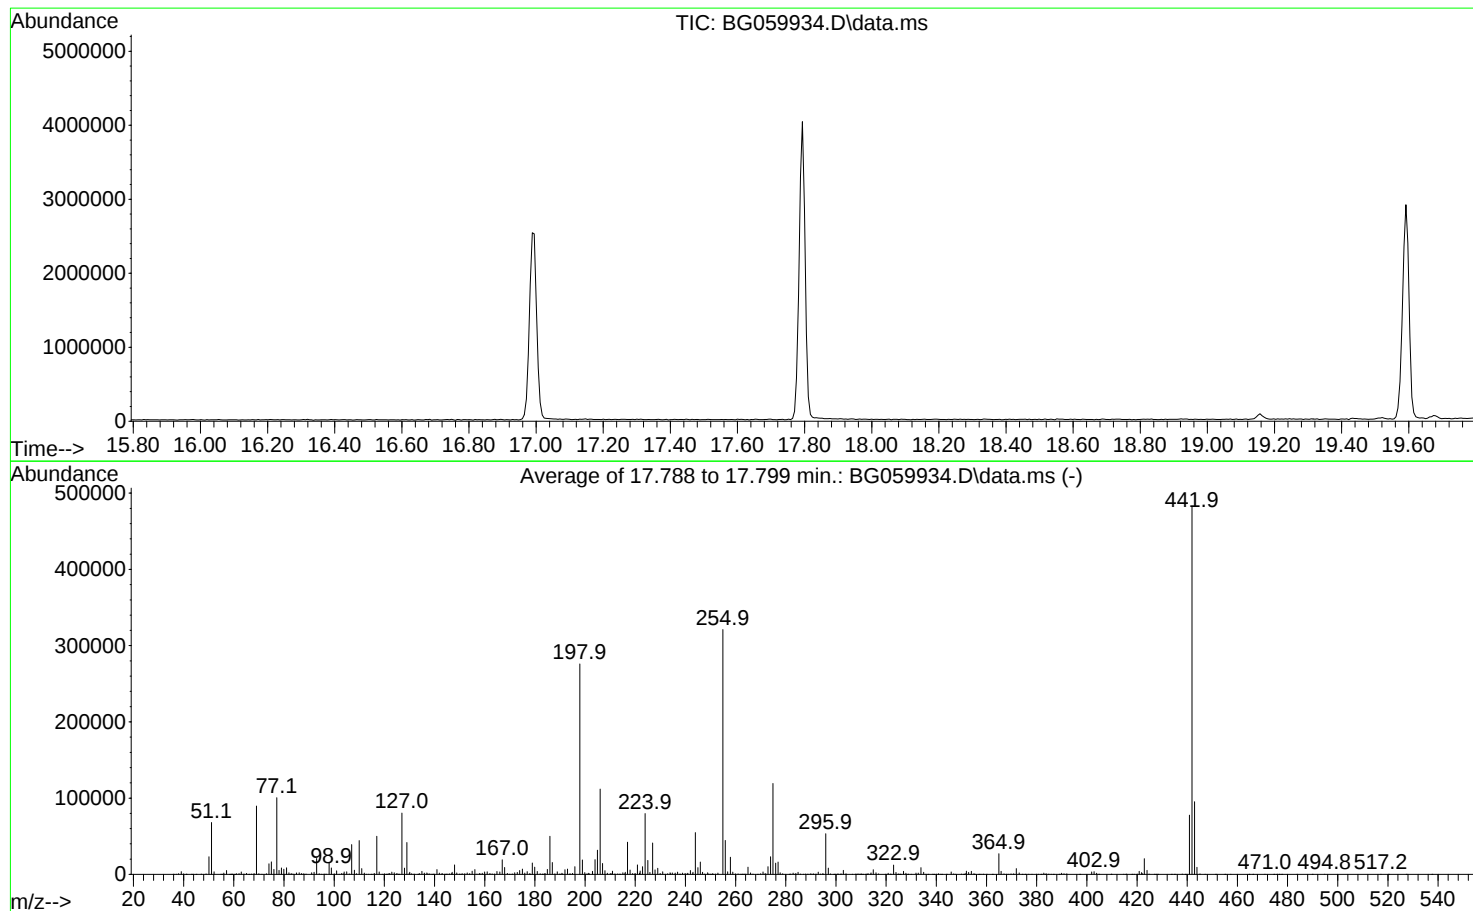




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	67923	PASS
68	69	0.00	2	1.3	1151	PASS
69	198	0.00	100	32.5	89707	PASS
70	69	0.00	2	1.0	880	PASS
127	198	10	80	29.1	80429	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	276011	PASS
199	198	5	9	6.8	18889	PASS
275	198	10	60	43.2	119200	PASS
365	198	1	100	9.8	27040	PASS
441	198	0.01	100	28.1	77696	PASS
442	442	50	100	100.0	482475	PASS
443	442	15	24	19.8	95325	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120423\
Data File : BG059934.D
Acq On : 4 Dec 2023 16:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 05 03:02:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 02:26:15 2023
Response via : Initial Calibration

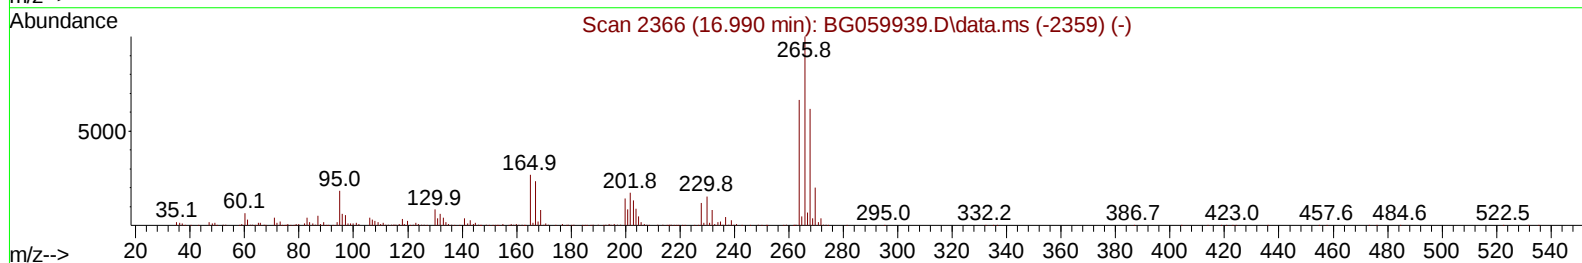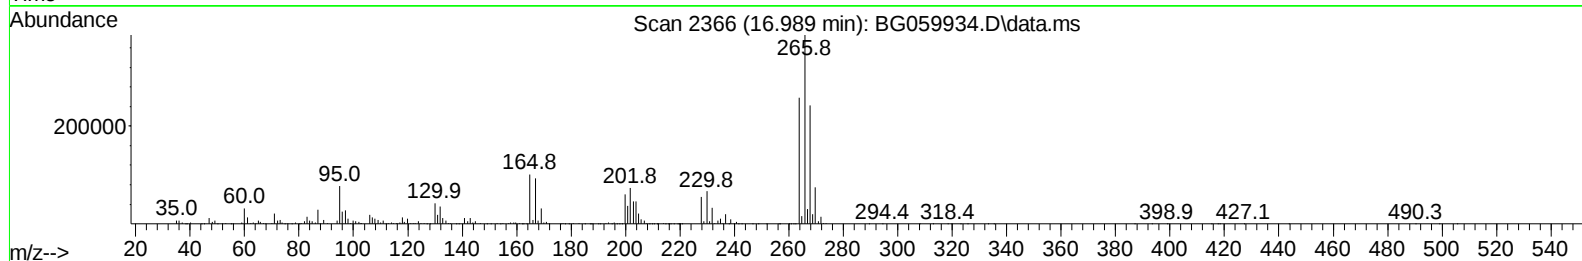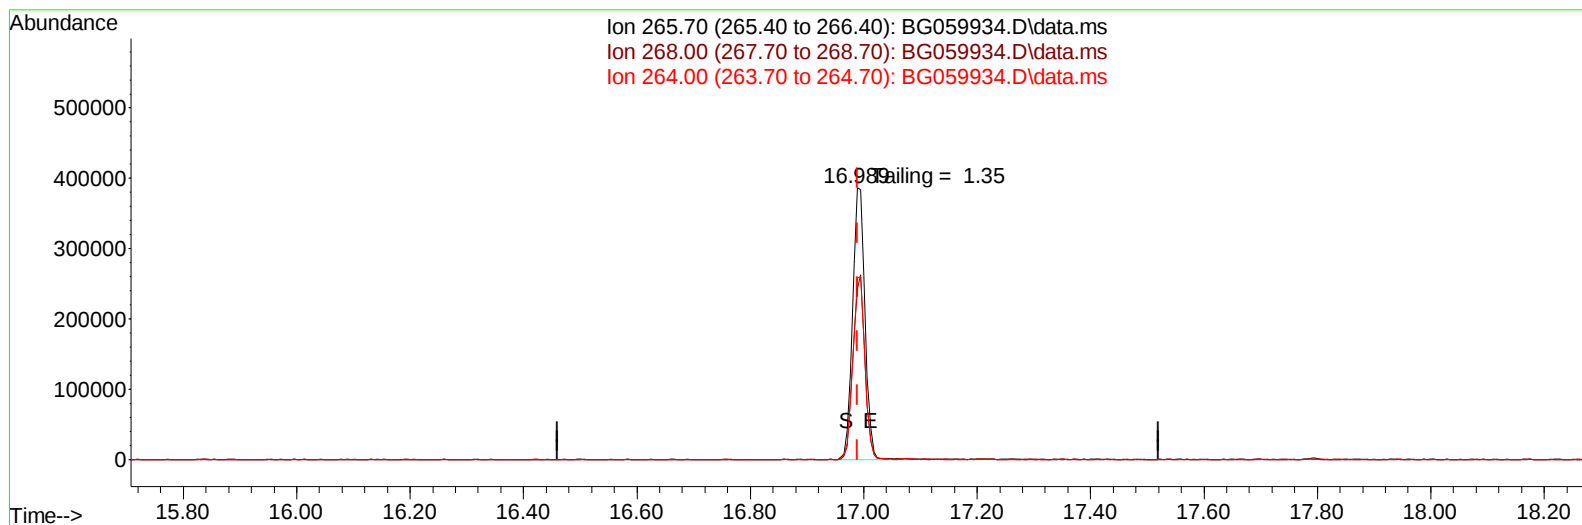

TIC: BG059934.D\data.ms

(70) Pentachlorophenol (C)

16.989min (-0.001) 473344.15 ng




response 587651

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	62.79
264.00	66.50	66.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120423\
Data File : BG059934.D
Acq On : 4 Dec 2023 16:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 05 03:02:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 02:26:15 2023
Response via : Initial Calibration

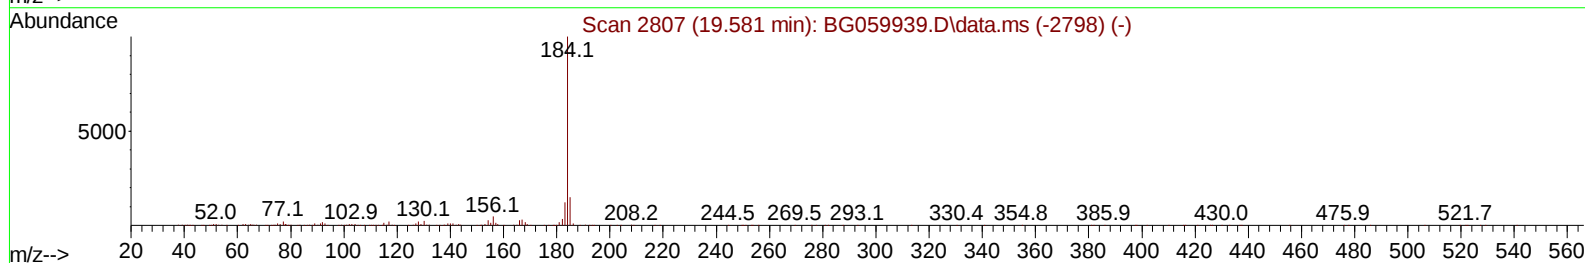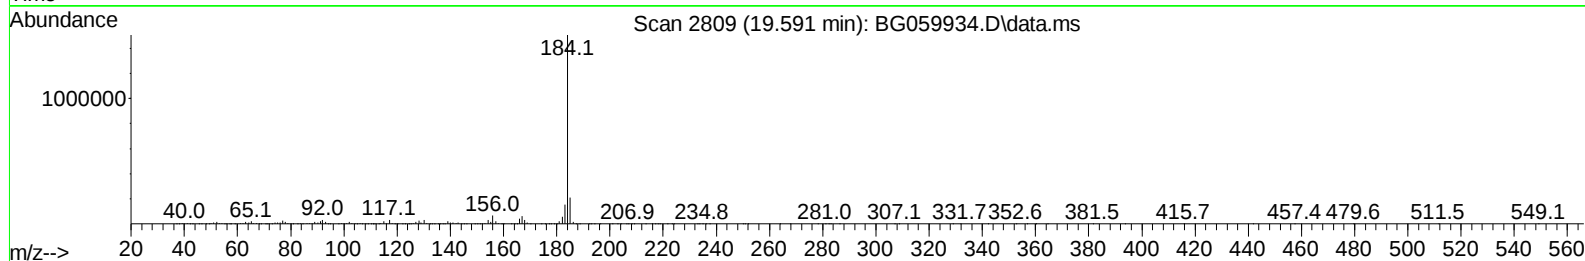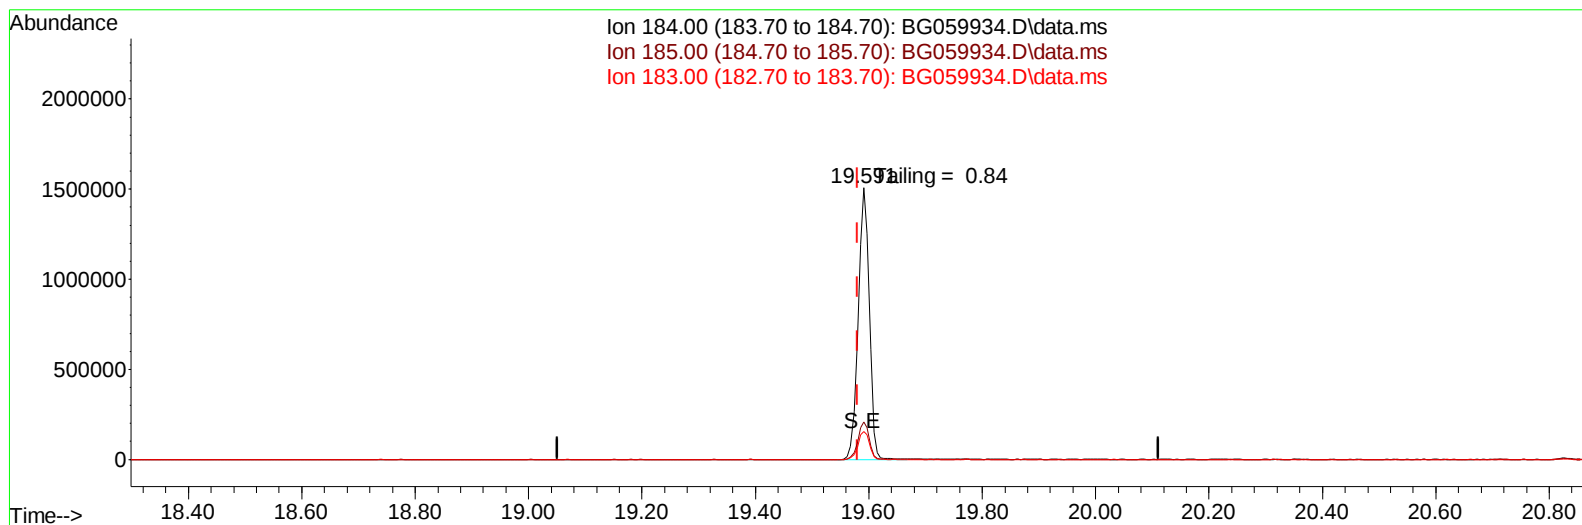

TIC: BG059934.D\data.ms

(77) Benzidine

19.591min (+ 0.010) 2382272.94 ng

response 2047974

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.85
183.00	12.10	10.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/4/2023	BNA_G	<u>BG059934.D</u>
Compound Name	Response	Retention Time
DDT	1437127	20.831
DDD	19190	20.443
DDE	0	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19190	1456317	1.32

Instrument :
BNA_G
ClientSampleId :
DFTPP