

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120523\
 Data File : BG059950.D
 Acq On : 5 Dec 2023 15:25
 Operator : MA/JU
 Sample : 05560-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RT4746

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG059950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.141	5	9	15	rVB	280963	392741	3.80%	1.138%
2	5.526	409	415	422	rVB	1095231	1673956	16.18%	4.852%
3	7.112	678	685	692	rVB	1196014	1972127	19.06%	5.716%
4	7.953	822	828	837	rVB	317826	558525	5.40%	1.619%
5	9.116	1016	1026	1033	rBV	665786	1148551	11.10%	3.329%
6	10.767	1297	1307	1314	rBV	369129	670270	6.48%	1.943%
7	13.223	1718	1725	1731	rBV	2688360	4055996	39.19%	11.755%
8	14.592	1952	1958	1965	rVB	752861	1215627	11.75%	3.523%
9	16.084	2203	2212	2223	rVB	2287351	3456991	33.41%	10.019%
10	17.342	2420	2426	2433	rBV	1273266	1943310	18.78%	5.632%
11	18.241	2574	2579	2584	rBV4	110392	161698	1.56%	0.469%
12	19.968	2867	2873	2879	rBV	7922975	10348511	100.00%	29.993%
13	21.272	3091	3095	3102	rBV6	82215	144576	1.40%	0.419%
14	21.619	3147	3154	3162	rBV	1964837	3213342	31.05%	9.313%
15	24.809	3685	3697	3710	rBV2	1150259	3547147	34.28%	10.281%




Sum of corrected areas: 34503368

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120523\
Data File : BG059950.D
Acq On : 5 Dec 2023 15:25
Operator : MA/JU
Sample : 05560-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RT4746

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

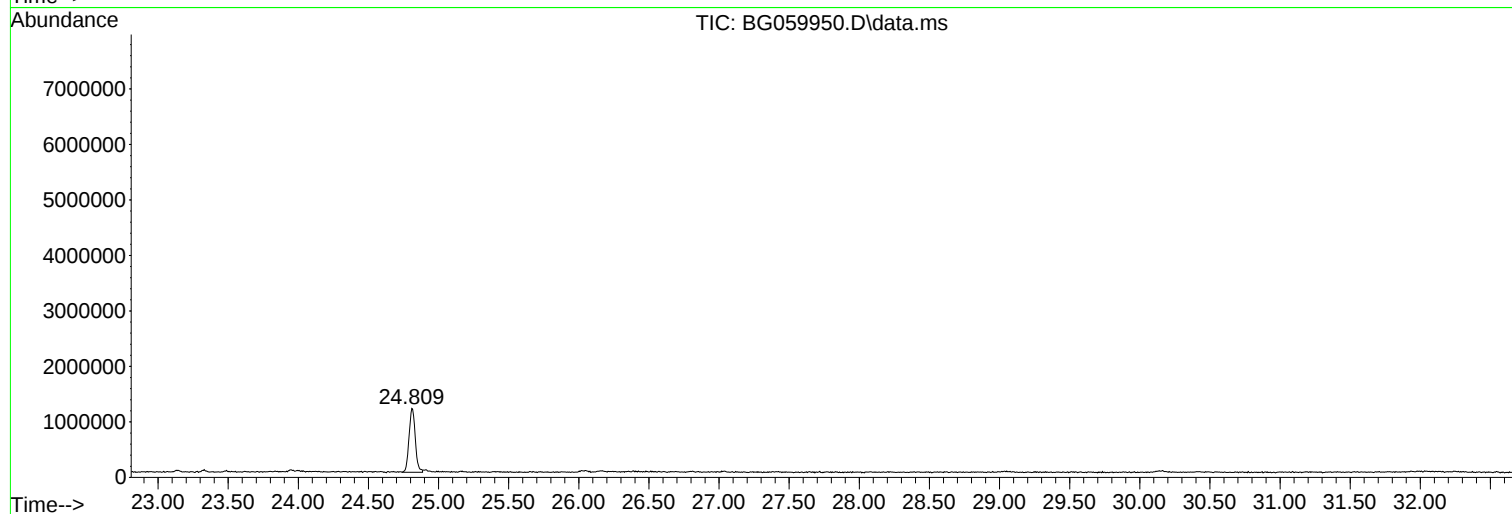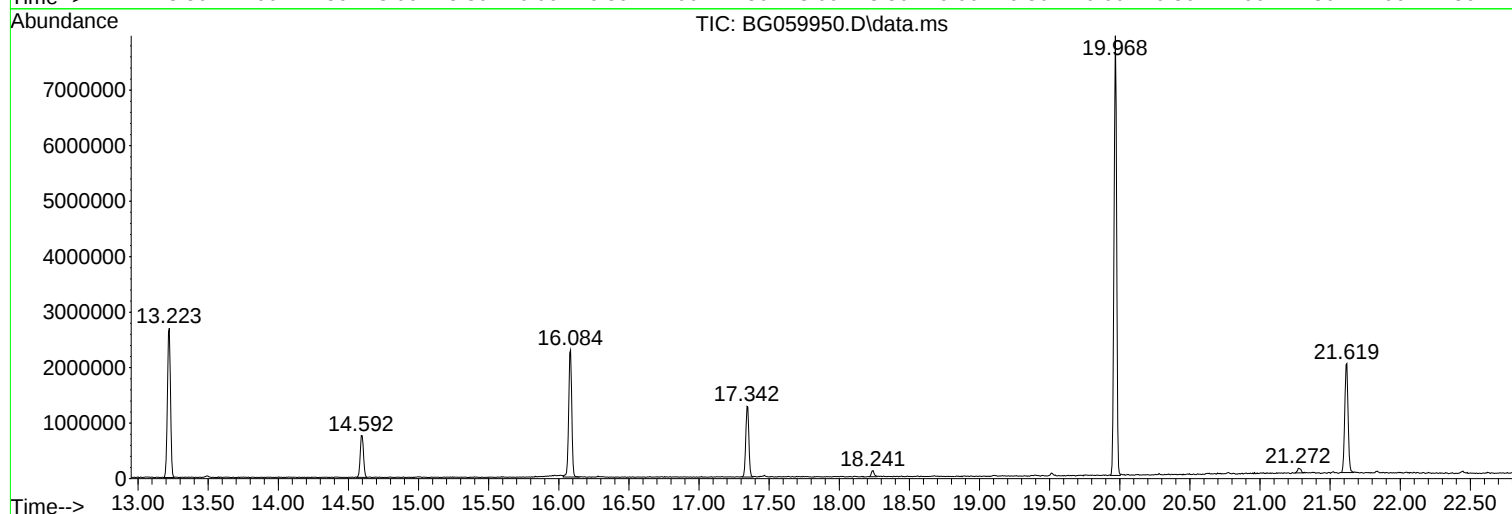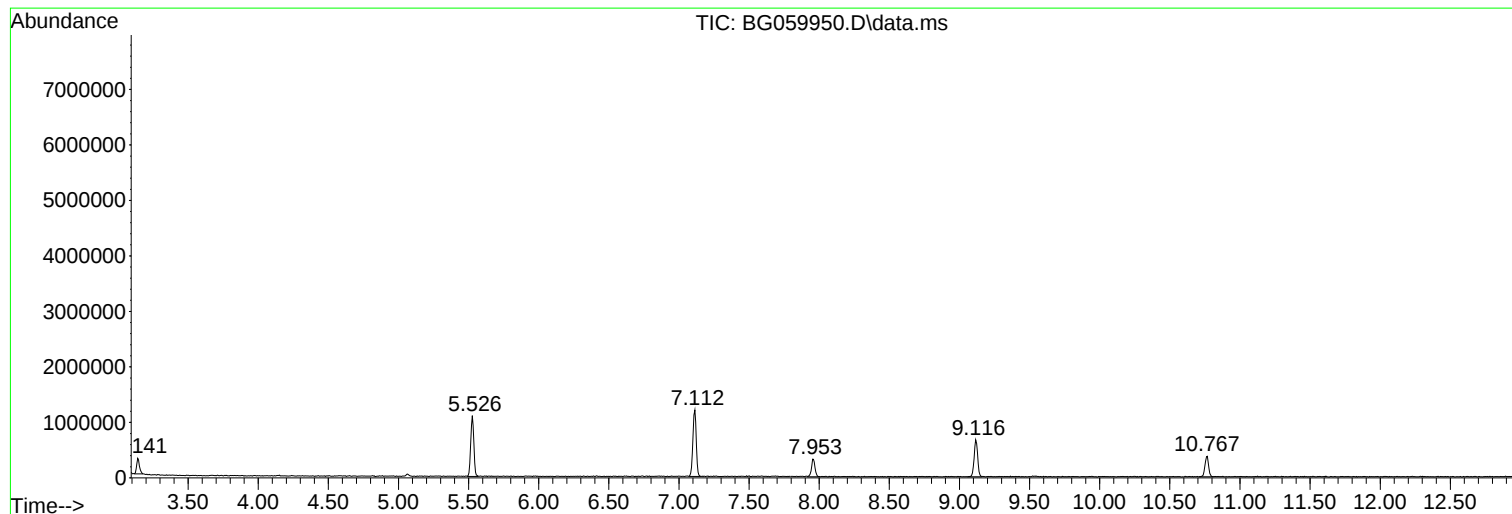

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120523\
Data File : BG059950.D
Acq On : 5 Dec 2023 15:25
Operator : MA/JU
Sample : 05560-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RT4746










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.141 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.141	14.06 ng	392741	1,4-Dichlorobenzene-d4	7.959

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	40		
2	N-Ethylformamide	73	C3H7NO	000627-45-2	9		
3	3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	9		
4	1,3-Dioxolane, 2-pentadecyl-	284	C18H36O2	004360-57-0	9		
5	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	9		

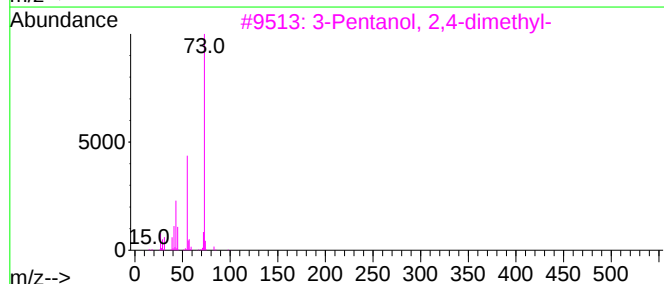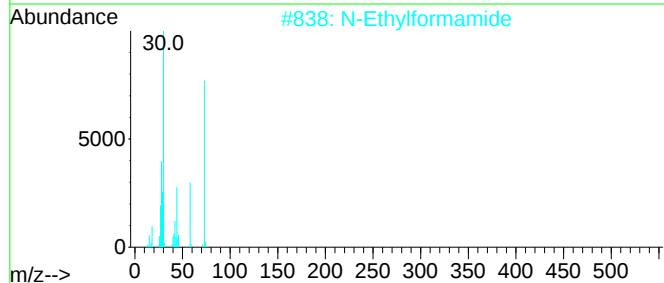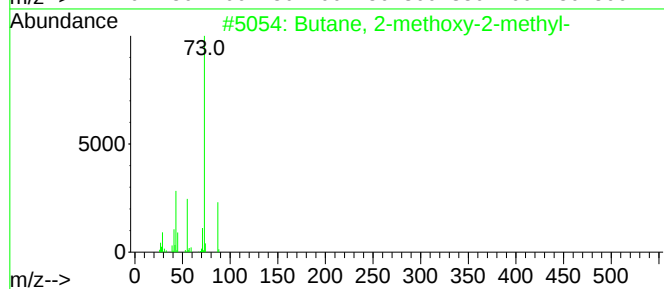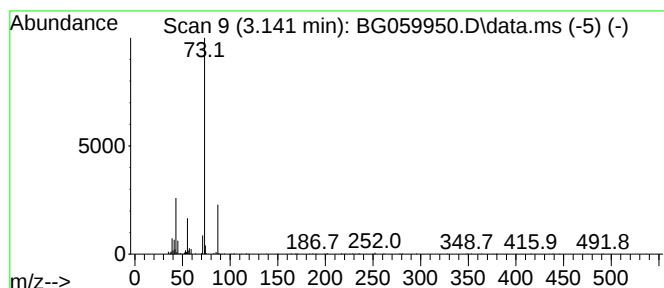

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120523\
Data File : BG059950.D
Acq On : 5 Dec 2023 15:25
Operator : MA/JU
Sample : 05560-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RT4746

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.141	3.141	14.1	ng	392741	1	7.959	558525	20.0