
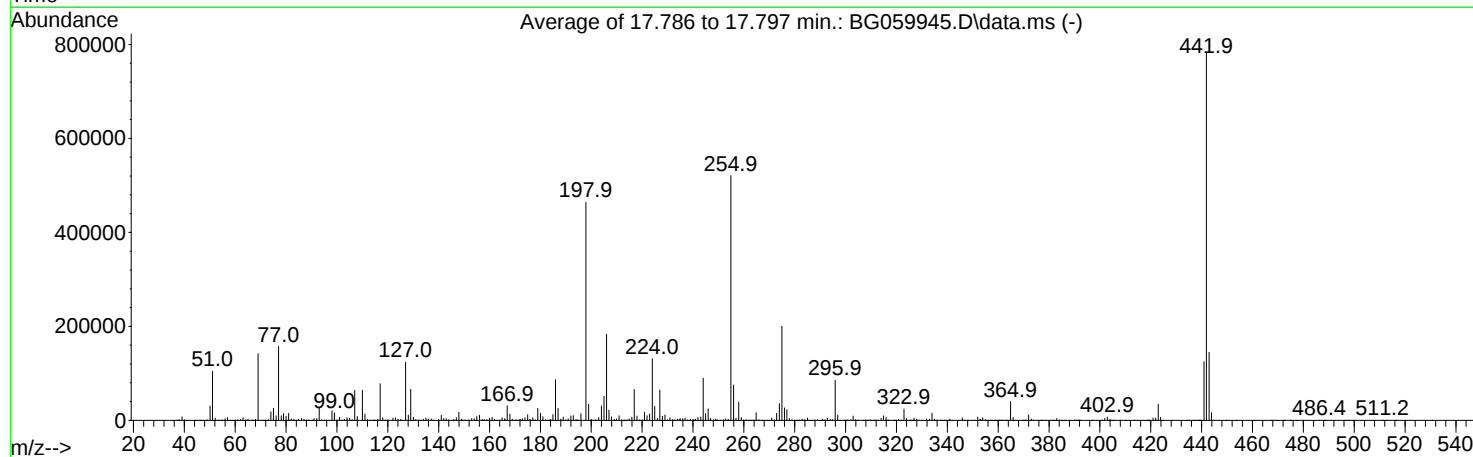


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120523\
 Data File : BG059945.D
 Acq On : 5 Dec 2023 11:58
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 05 02:26:15 2023

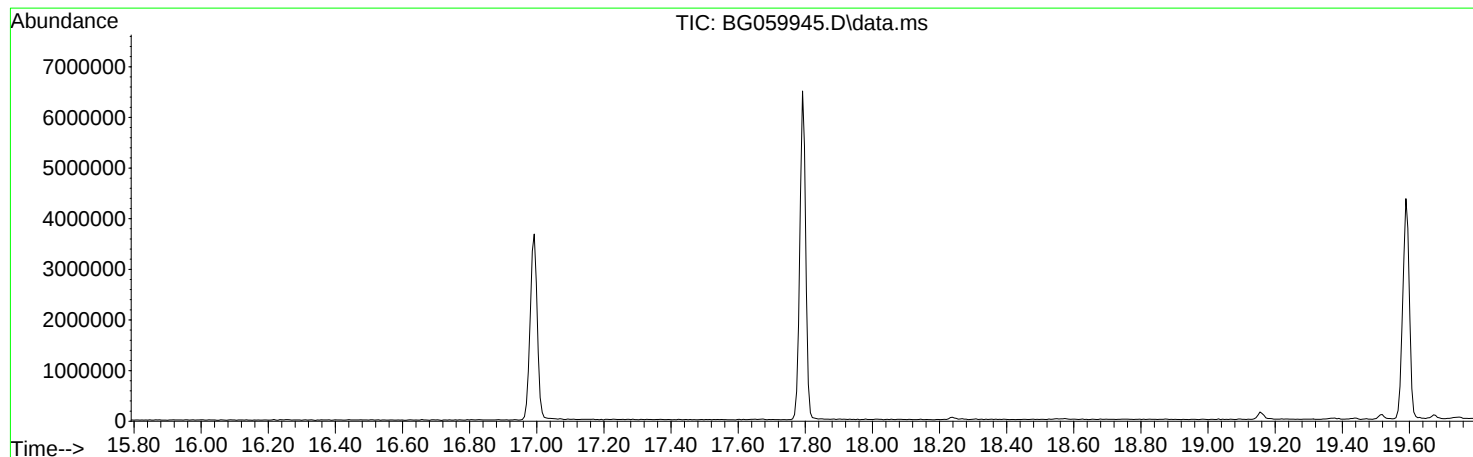




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	104716	PASS
68	69	0.00	2	1.7	2428	PASS
69	198	0.00	100	30.6	142168	PASS
70	69	0.00	2	0.5	764	PASS
127	198	10	80	26.7	123731	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	463851	PASS
199	198	5	9	7.3	33997	PASS
275	198	10	60	43.2	200213	PASS
365	198	1	100	8.6	39998	PASS
441	198	0.01	100	27.0	125139	PASS
442	442	50	100	100.0	782869	PASS
443	442	15	24	18.5	144872	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120523\
Data File : BG059945.D
Acq On : 5 Dec 2023 11:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 05 18:22:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 02:26:15 2023
Response via : Initial Calibration

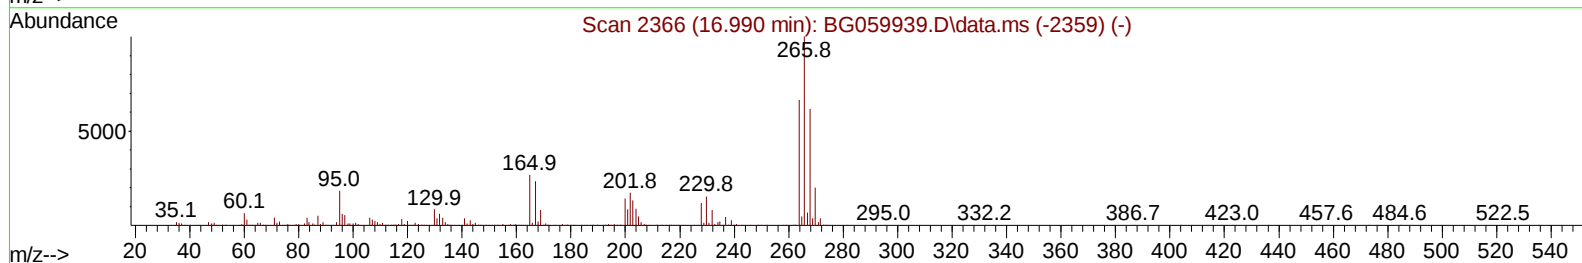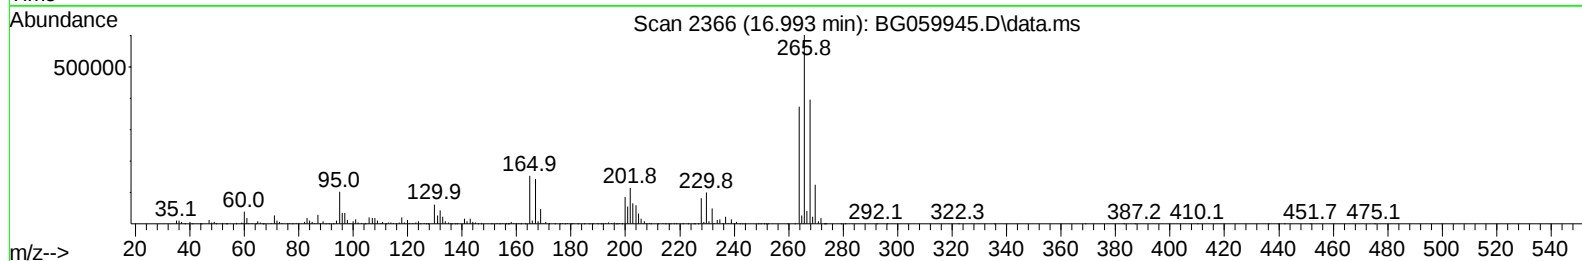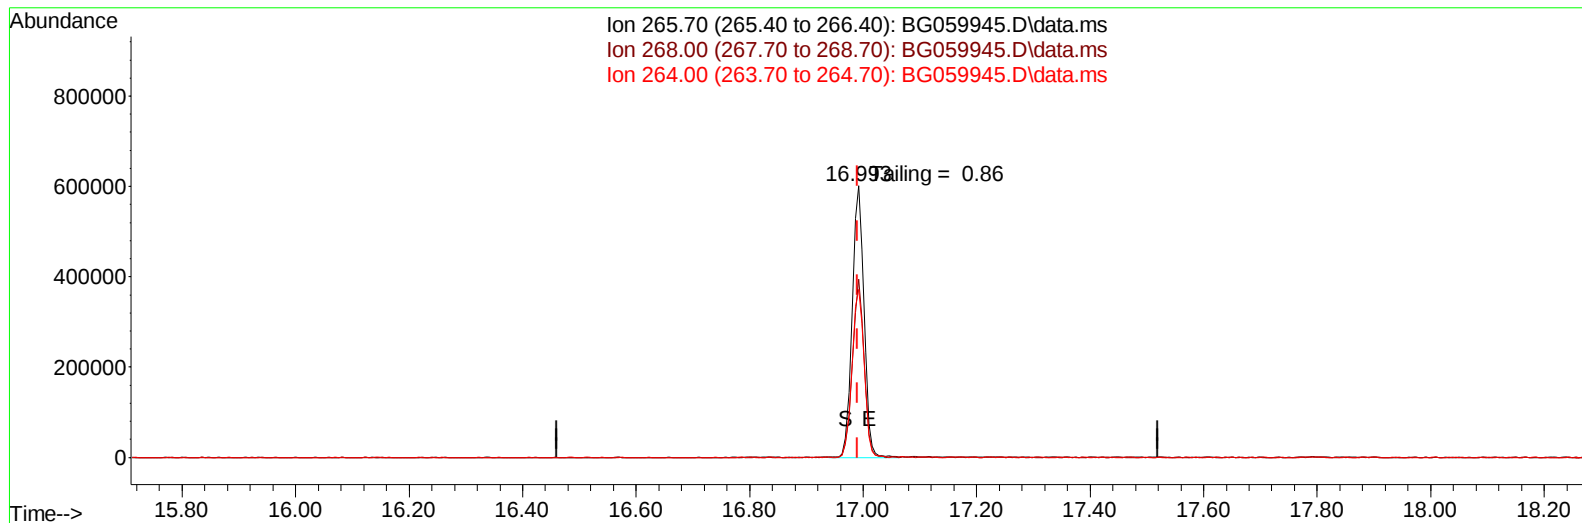

TIC: BG059945.D\data.ms

(70) Pentachlorophenol (C)

16.993min (+ 0.003) 151618.85 ng




response 876329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	65.62
264.00	66.50	61.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120523\
Data File : BG059945.D
Acq On : 5 Dec 2023 11:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 05 18:22:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 02:26:15 2023
Response via : Initial Calibration

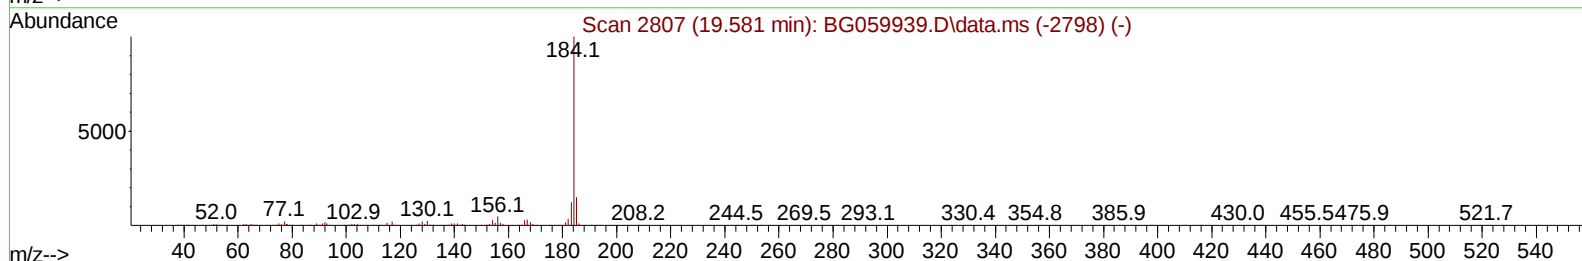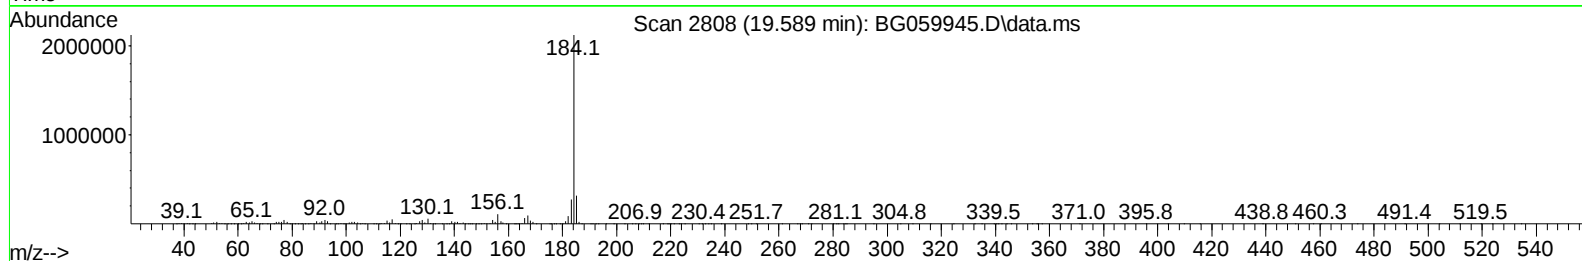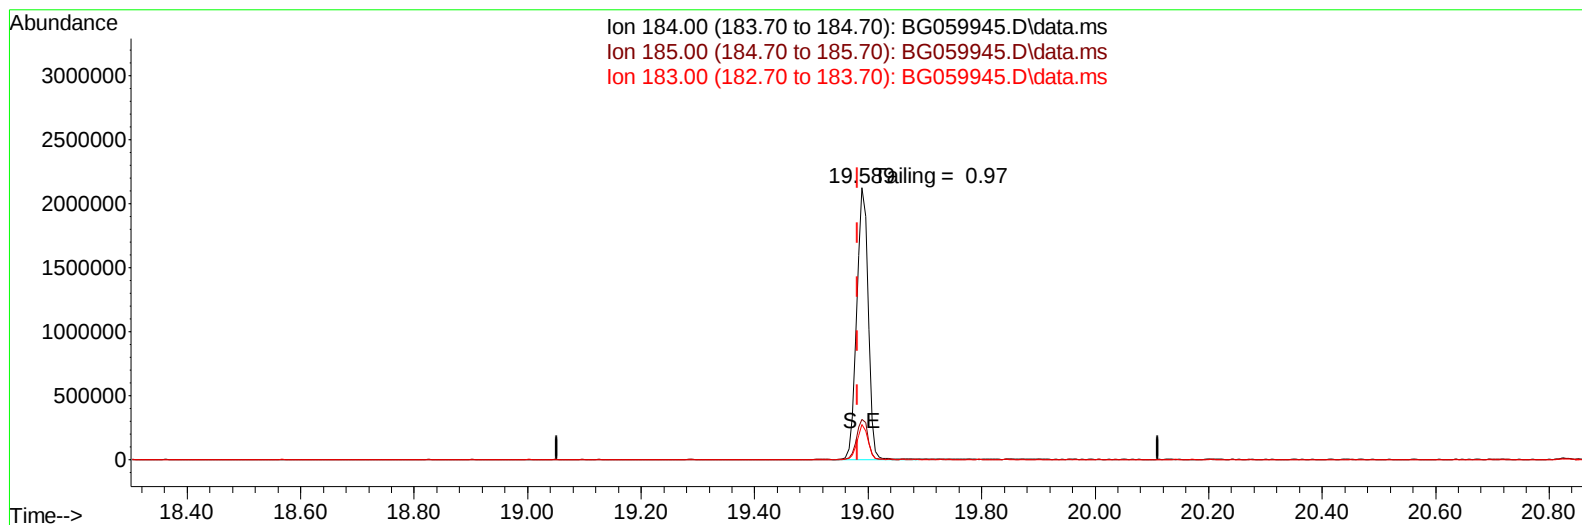

TIC: BG059945.D\data.ms

(77) Benzidine**19.589min (+ 0.008) 42680.66 ng****response 2966966**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.84
183.00	12.10	12.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/5/2023	BNA_G	<u>BG059945.D</u>
Compound Name	Response	Retention Time
DDT	2052689	20.829
DDD	43316	20.383
DDE	474	19.877
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43790	2096479	2.09

Instrument :
BNA_G
ClientSampleId :
DFTPP