
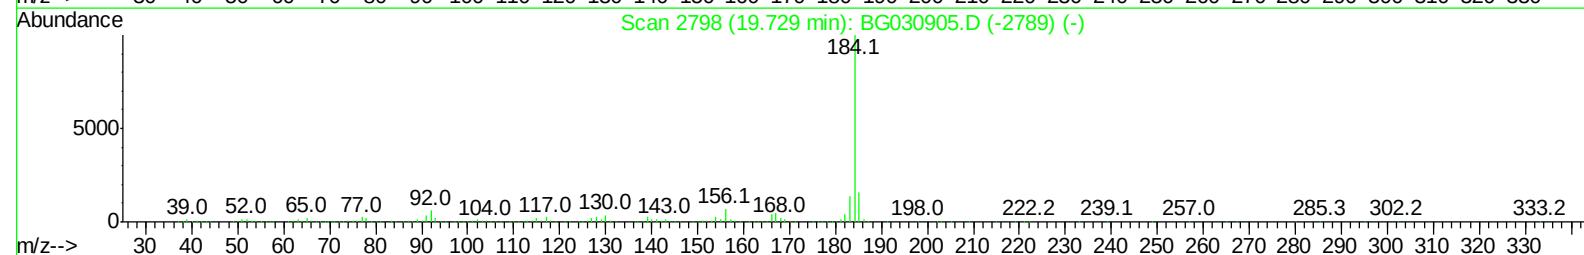
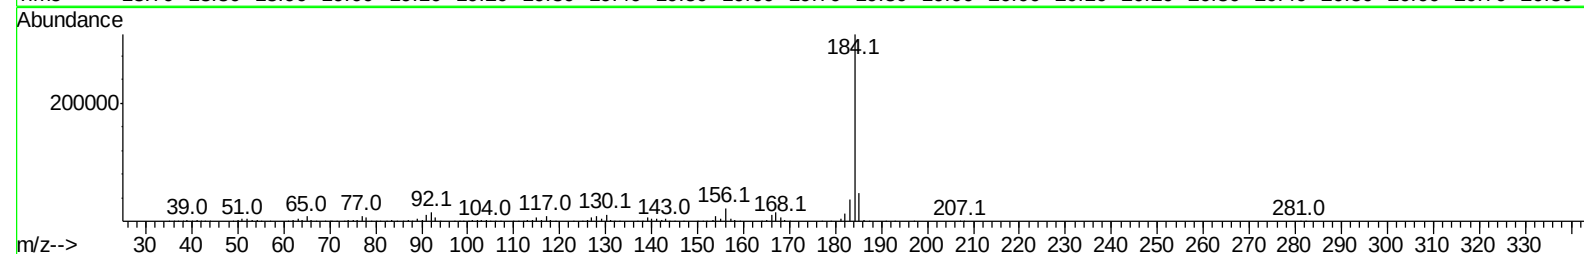


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG120617\
Data File : BG031369.D
Acq On : 6 Dec 2017 13:56
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 07:28:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 17:58:37 2017
Response via : Initial Calibration

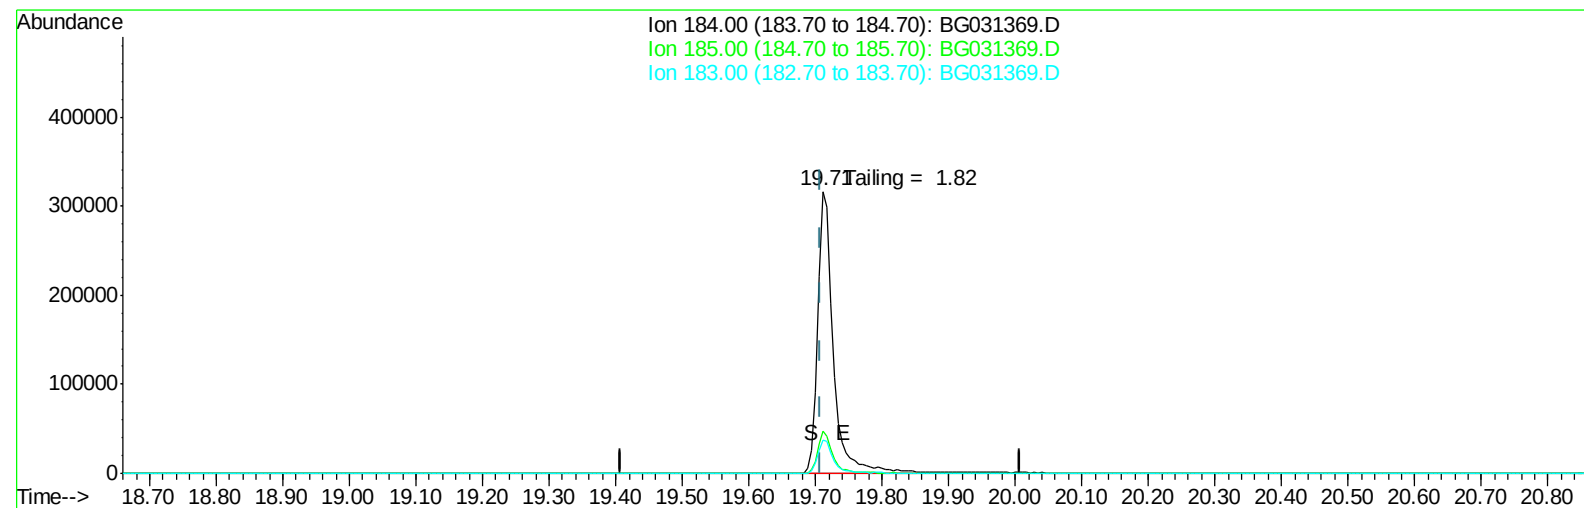

TIC: BG031369.D

(76) Benzidine




19.711min (+0.002) 136475.51ng

response 526065

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.01
183.00	13.30	12.00
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG120617\
Data File : BG031369.D
Acq On : 6 Dec 2017 13:56
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 07:28:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 17:58:37 2017
Response via : Initial Calibration

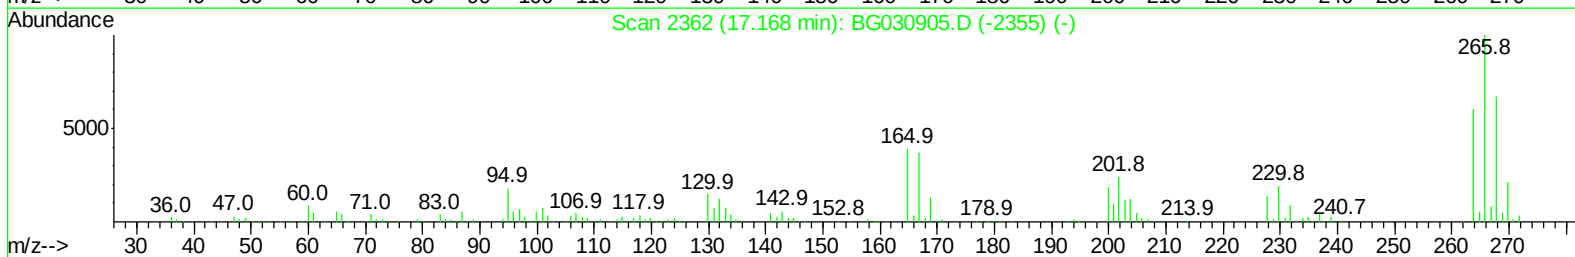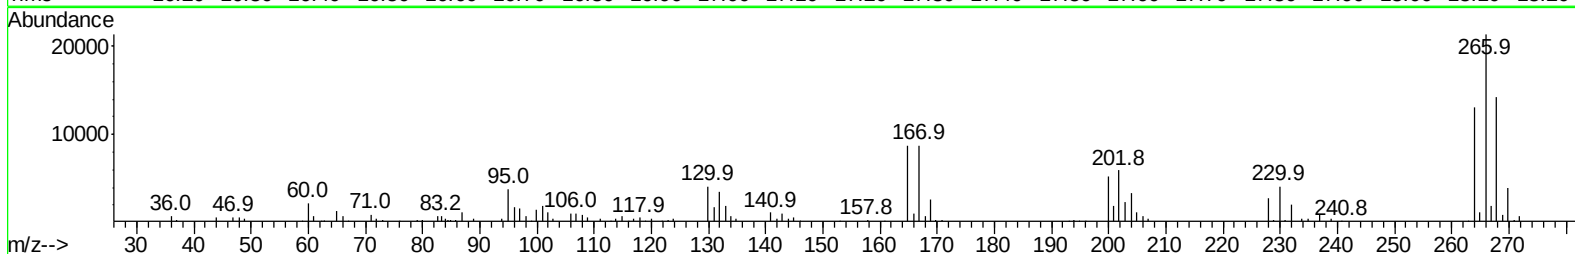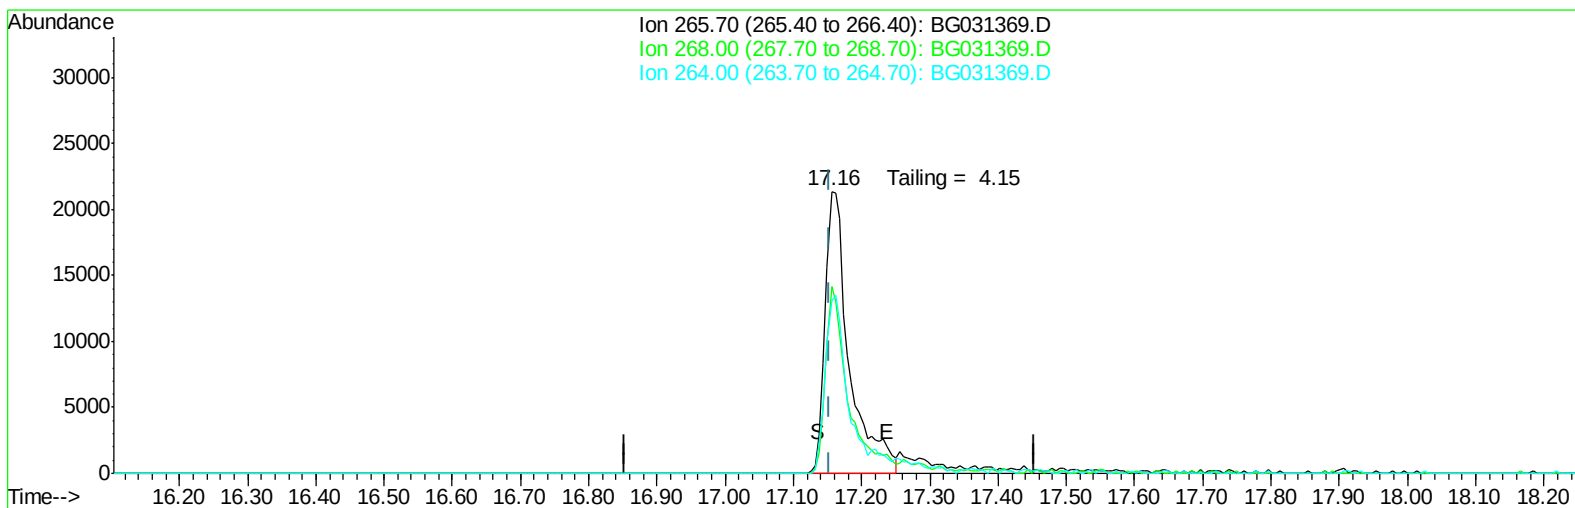

TIC: BG031369.D

(69) Pentachlorophenol (C)

17.156min (+0.002) 28146.68ng

response 52346

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.47
264.00	62.00	61.37
0.00	0.00	0.00