


Data Path : Z:\HPCHEM1\BNA G\Data\BG120617\
 Data File : BG031369.D
 Acq On : 6 Dec 2017 13:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 06 17:58:37 2017

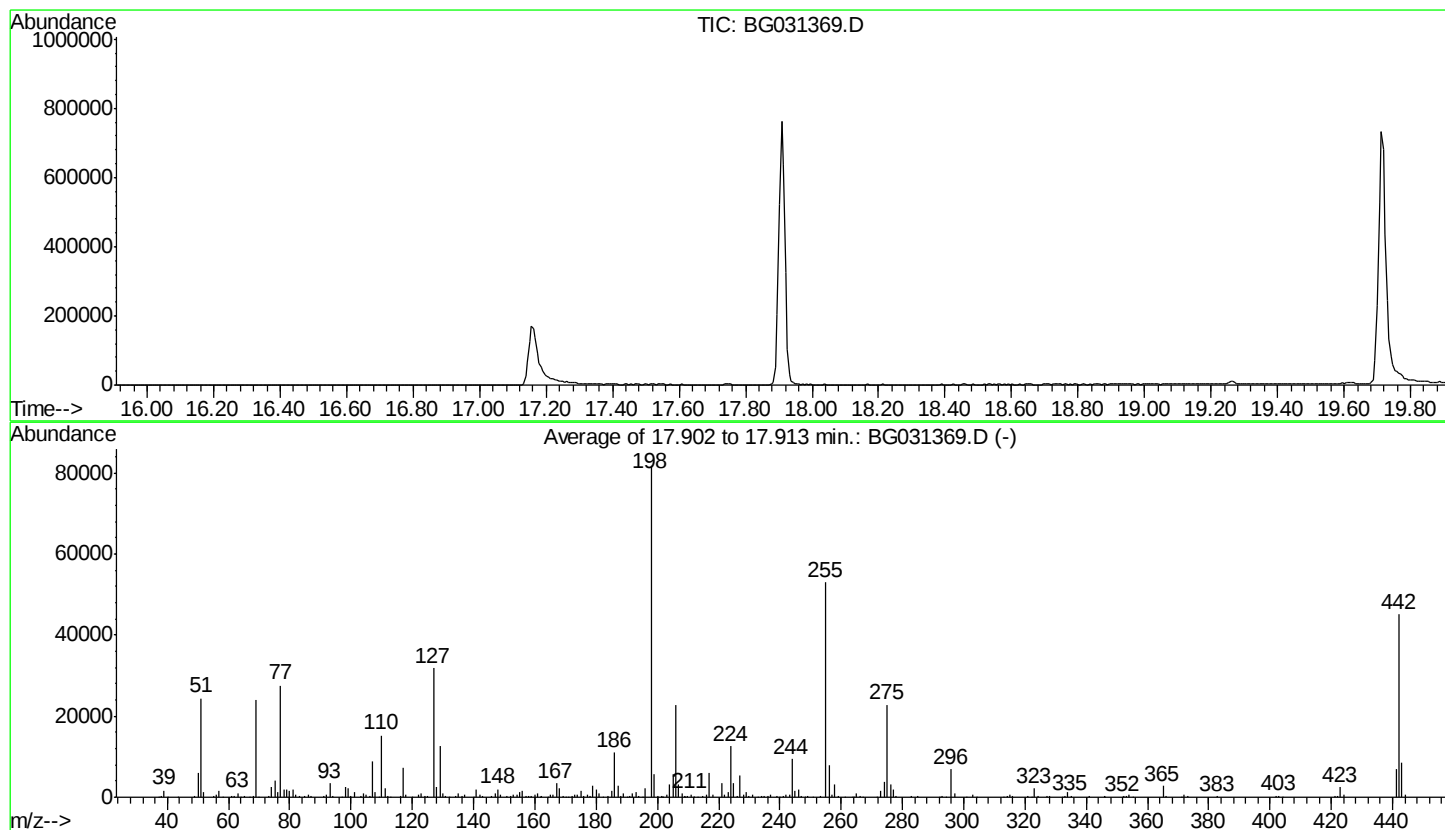

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	24453	PASS
68	69	0.00	2	0.8	194	PASS
69	198	0.00	100	29.4	24032	PASS
70	69	0.00	2	0.3	63	PASS
127	198	10	80	39.0	31877	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81826	PASS
199	198	5	9	6.8	5546	PASS
275	198	10	60	27.9	22819	PASS
365	198	1	100	3.4	2757	PASS
441	442	0.01	24	15.2	6854	PASS
442	198	50	100	55.1	45085	PASS
443	442	15	24	19.1	8630	PASS