


Data Path : Z:\HPCHEM1\BNA G\Data\BG120617\
 Data File : BG031388.D
 Acq On : 7 Dec 2017 1:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 06 17:58:37 2017

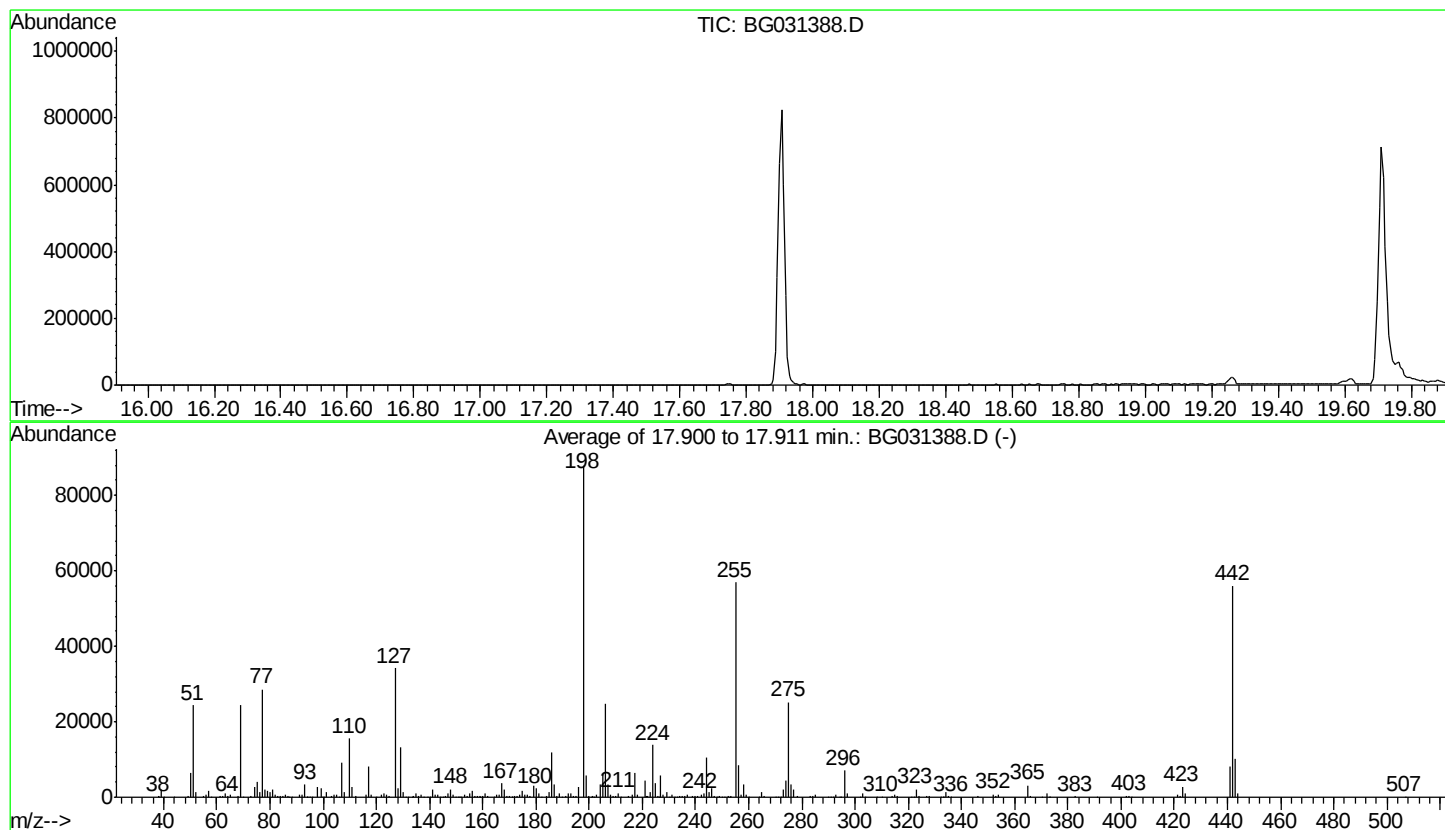

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	24384	PASS
68	69	0.00	2	1.3	308	PASS
69	198	0.00	100	27.9	24496	PASS
70	69	0.00	2	0.2	61	PASS
127	198	10	80	38.9	34173	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87890	PASS
199	198	5	9	6.6	5844	PASS
275	198	10	60	28.8	25282	PASS
365	198	1	100	3.5	3108	PASS
441	442	0.01	24	14.7	8271	PASS
442	198	50	100	63.8	56077	PASS
443	442	15	24	18.2	10224	PASS