
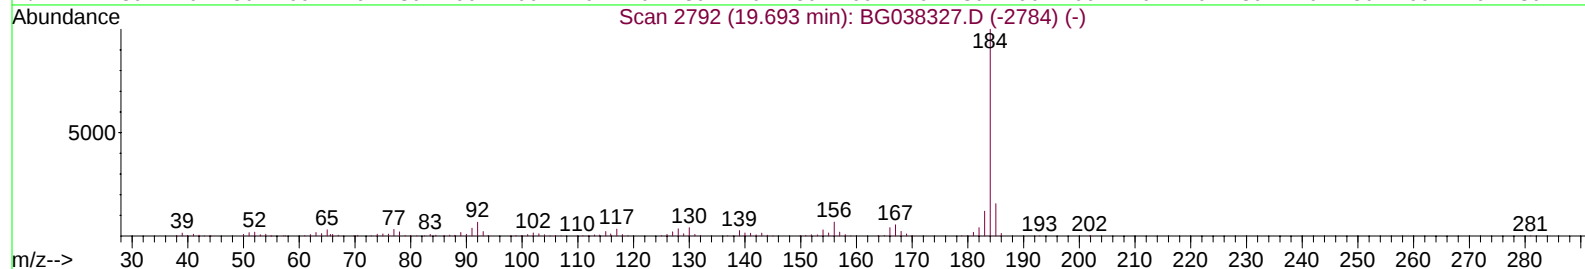
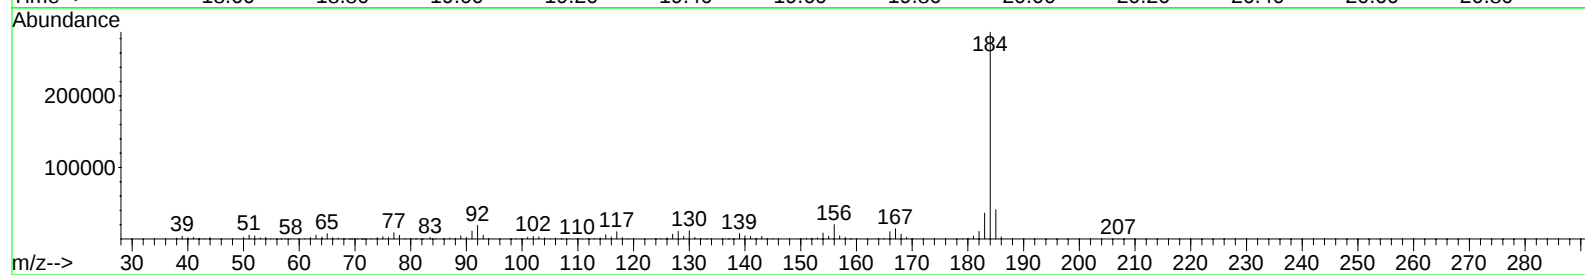


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120618\  
Data File  : BG038375.D  
Acq On     : 6 Dec 2018      8:56  
Operator   : JU/SJ  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1      Sample Multiplier: 1
```

Quant Time: Dec 06 10:00:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

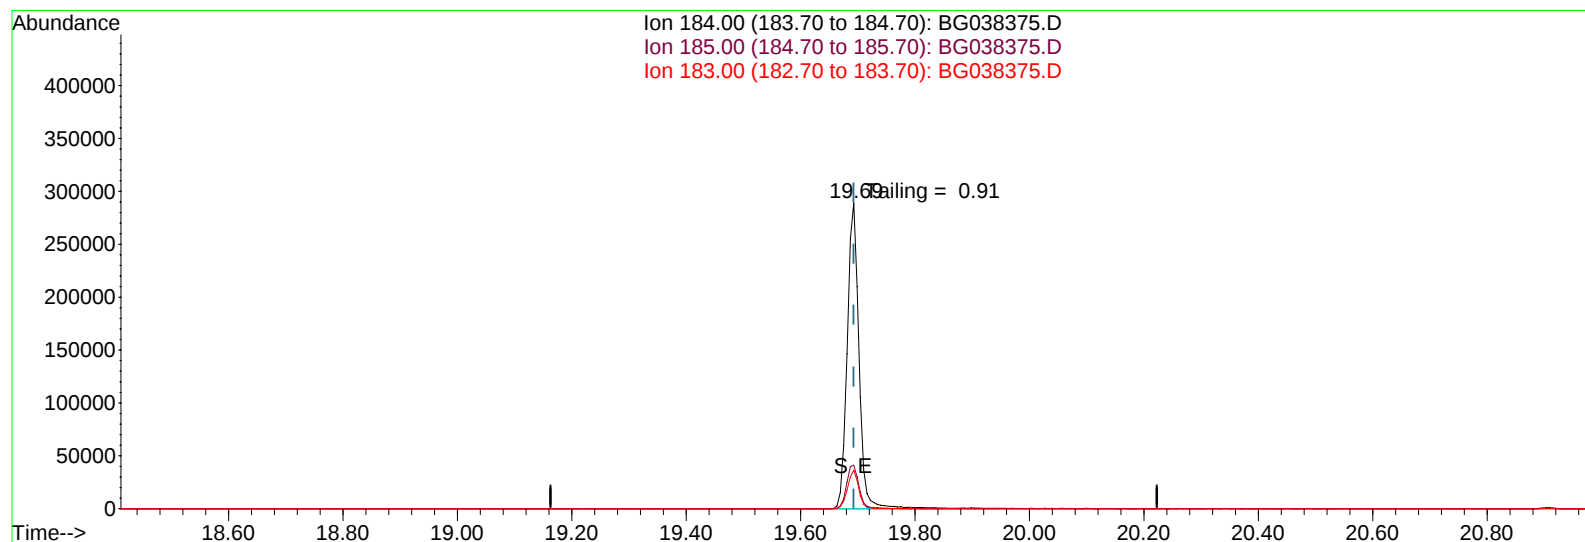

TIC: BG038375.D

(77) Benzidine




19.693min (-0.000) 62206.00ng

response 417725

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.24
183.00	12.70	12.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120618\
Data File : BG038375.D
Acq On : 6 Dec 2018 8:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 10:00:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

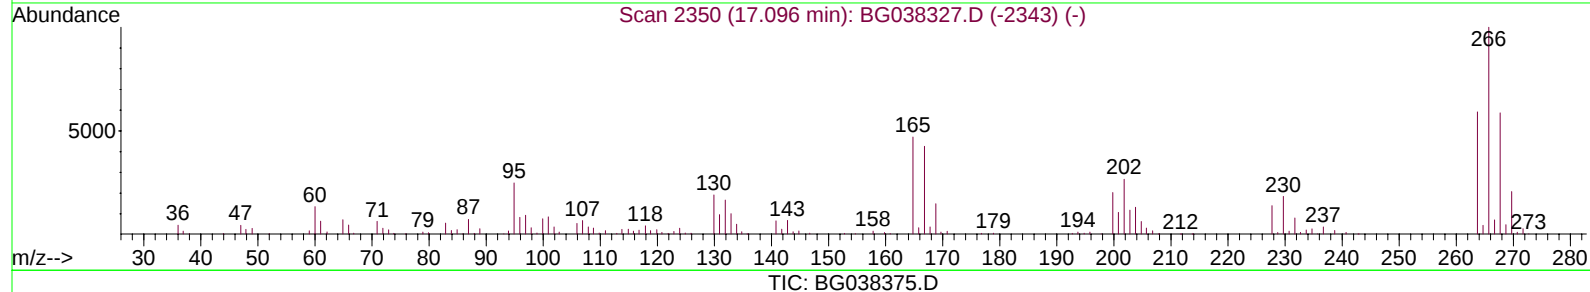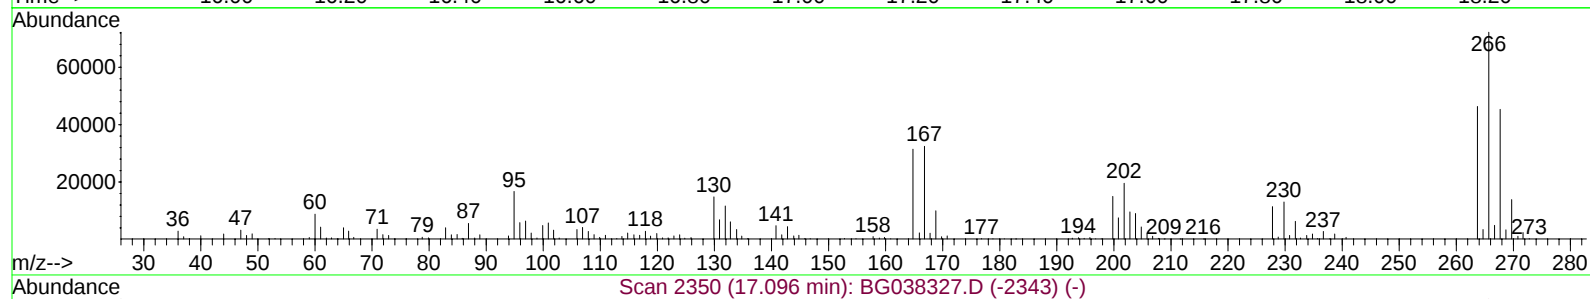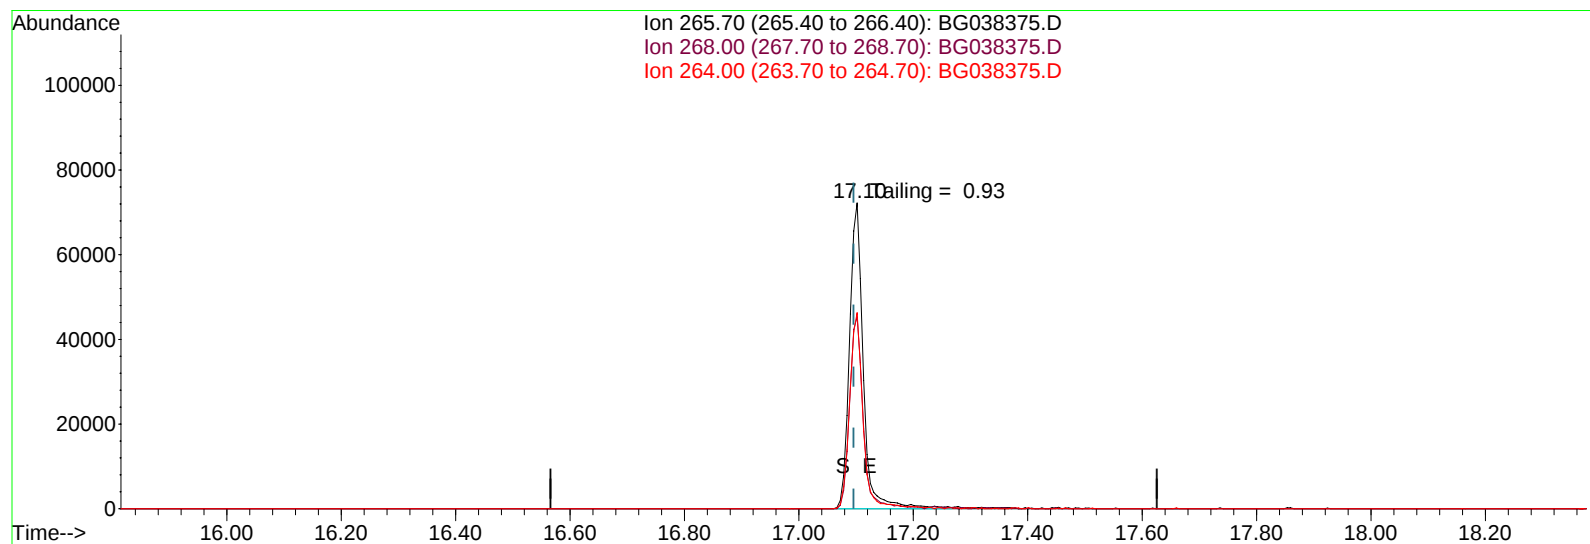

(70) Pentachlorophenol (C)

17.102min (+0.006) 76532.10ng

response 119697

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.38
264.00	73.60	68.87
0.00	0.00	0.00