


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120618\
 Data File : BG038375.D
 Acq On : 6 Dec 2018 8:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 04 17:15:40 2018

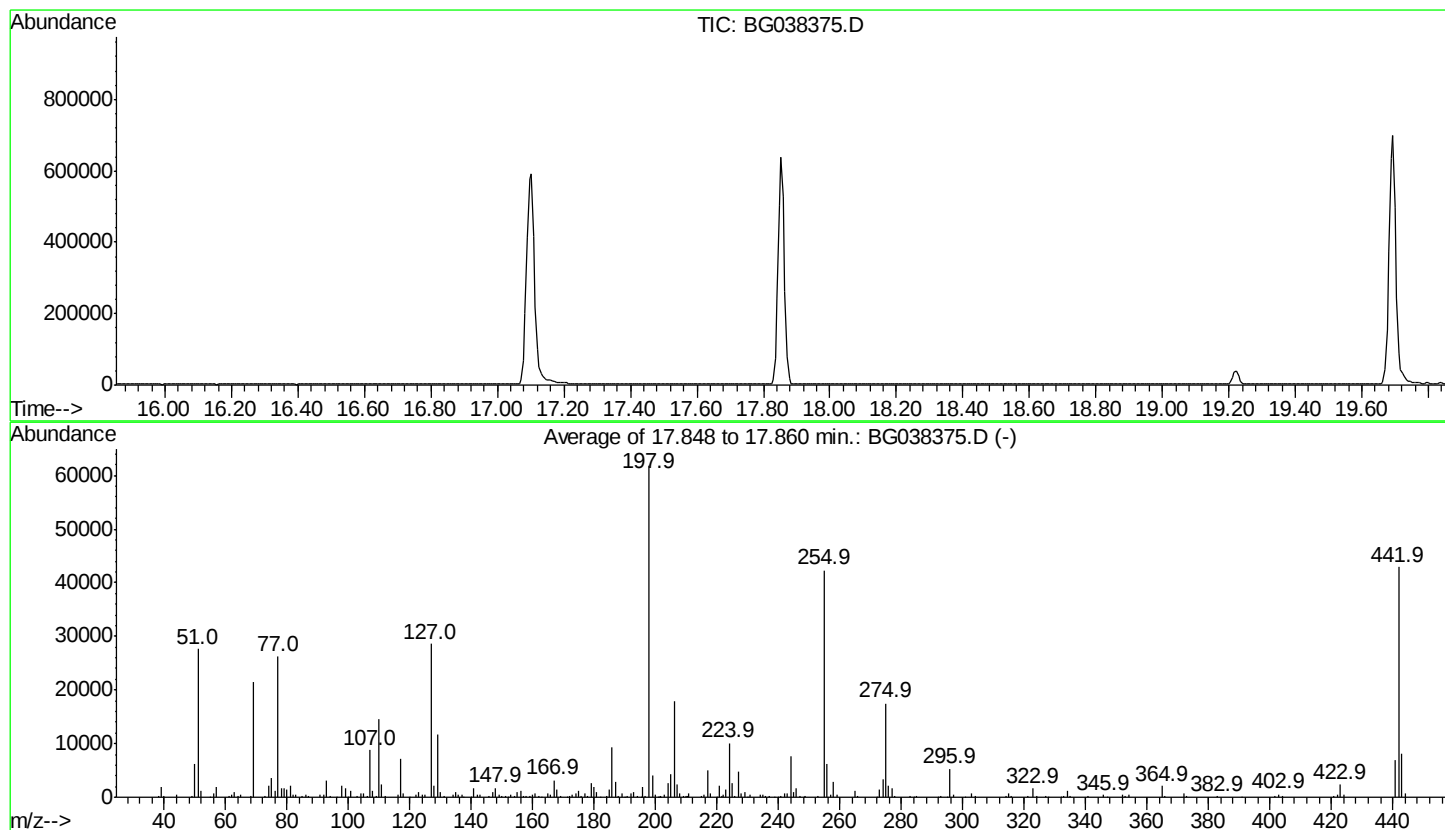

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	27600	PASS
68	69	0.00	2	0.6	128	PASS
69	198	0.00	100	34.6	21421	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.3	28602	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61840	PASS
199	198	5	9	6.6	4112	PASS
275	198	10	60	28.2	17445	PASS
365	198	1	100	3.4	2093	PASS
441	198	0.01	100	11.1	6856	PASS
442	198	50	100	69.3	42882	PASS
443	442	15	24	18.7	8015	PASS