


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120618\
 Data File : BG038391.D
 Acq On : 6 Dec 2018 21:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 04 17:15:40 2018

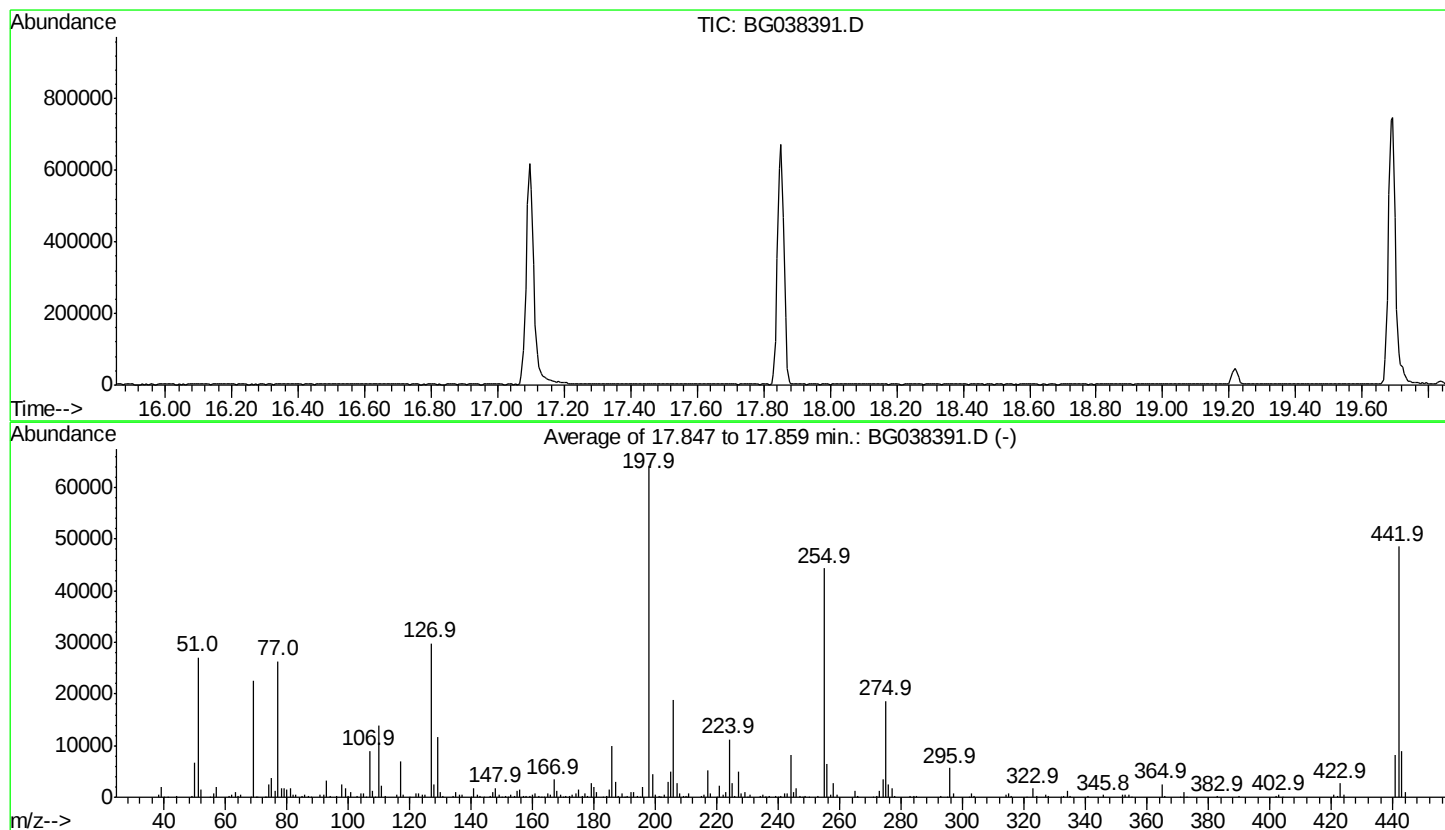

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	27133	PASS
68	69	0.00	2	0.3	73	PASS
69	198	0.00	100	35.2	22590	PASS
70	69	0.00	2	0.6	128	PASS
127	198	10	80	46.5	29869	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64234	PASS
199	198	5	9	6.9	4449	PASS
275	198	10	60	29.2	18727	PASS
365	198	1	100	4.0	2579	PASS
441	198	0.01	100	12.6	8111	PASS
442	198	50	100	75.6	48581	PASS
443	442	15	24	18.3	8899	PASS