
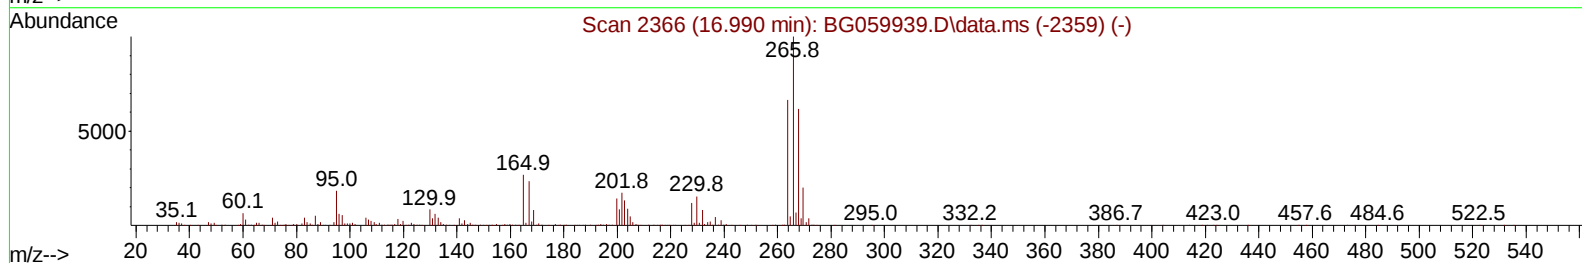
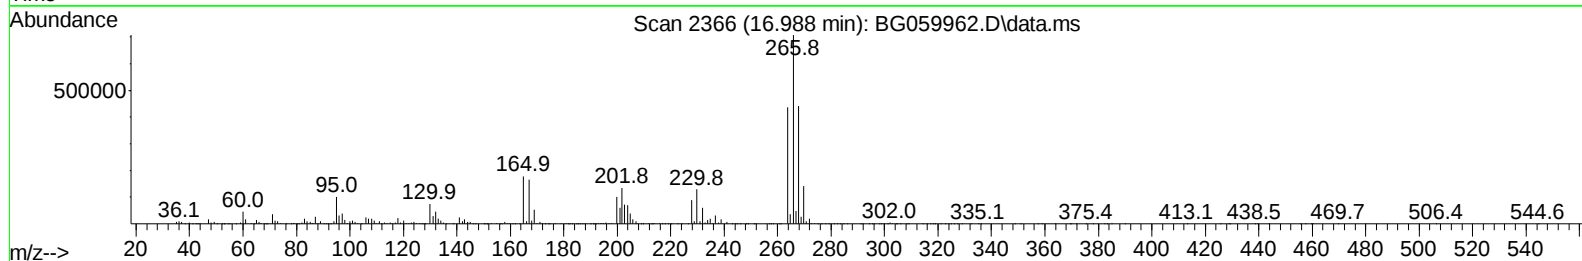


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG120623\  
Data File : BG059962.D  
Acq On : 6 Dec 2023 9:49  
Operator : MA/JU  
Sample : DFTTP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 01:38:04 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG120423.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 05 02:26:15 2023  
Response via : Initial Calibration

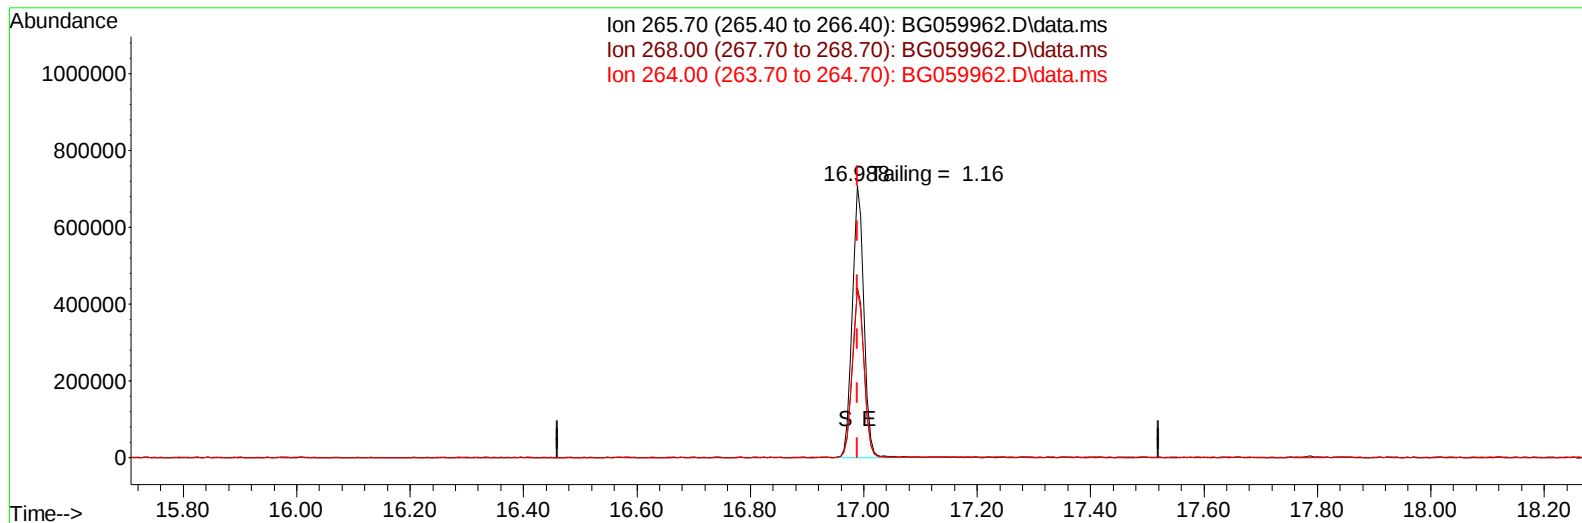

TIC: BG059962.D\data.ms

**(70) Pentachlorophenol (C)**




**16.988min (-0.001) 366050.95 ng**

**response 1009884**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.60  | 62.43  |
| 264.00 | 66.50  | 61.86  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG120623\  
Data File : BG059962.D  
Acq On : 6 Dec 2023 9:49  
Operator : MA/JU  
Sample : DFTTP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 01:38:04 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG120423.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 05 02:26:15 2023  
Response via : Initial Calibration

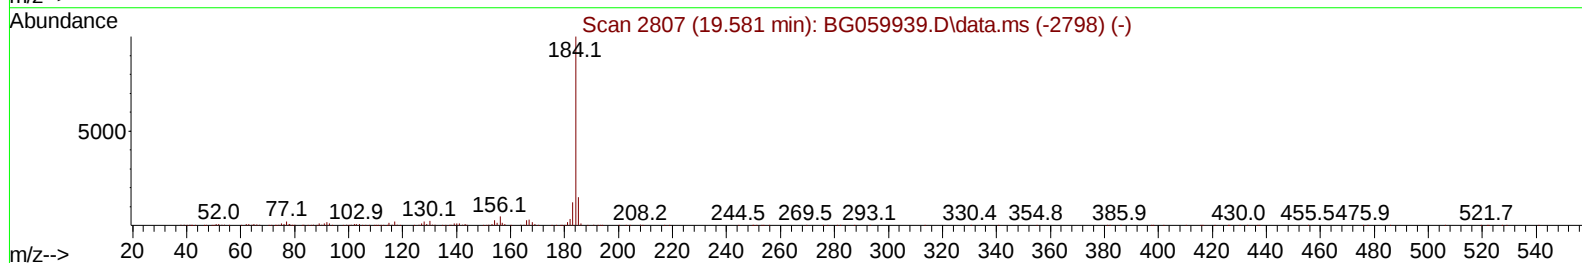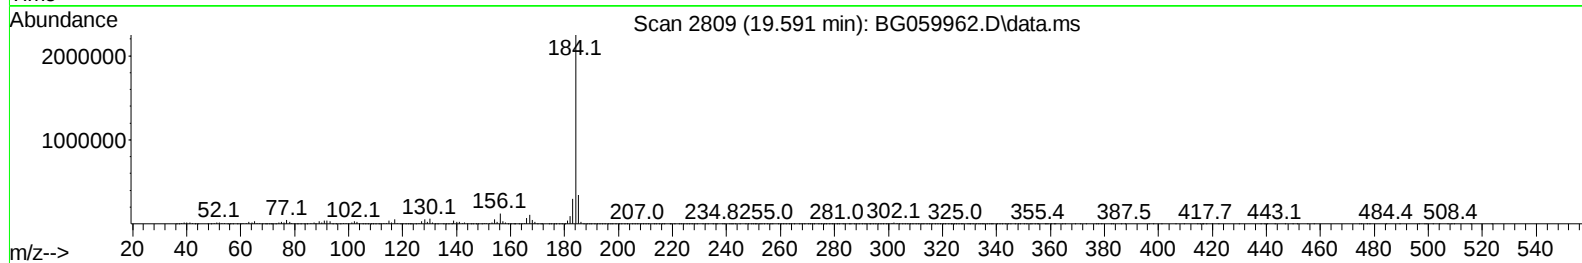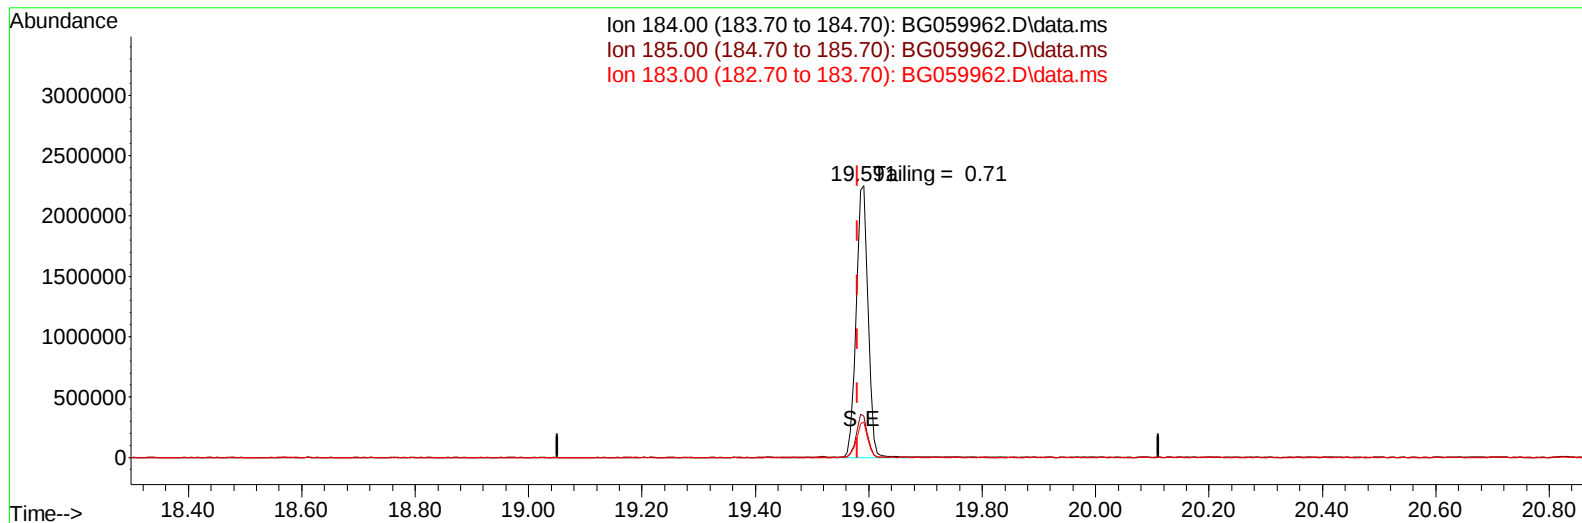

TIC: BG059962.D\data.ms

**(77) Benzidine****19.591min (+ 0.010) 357485.10 ng****response 3296158**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 15.15  |
| 183.00 | 12.10  | 13.11  |
| 0.00   | 0.00   | 0.00   |