
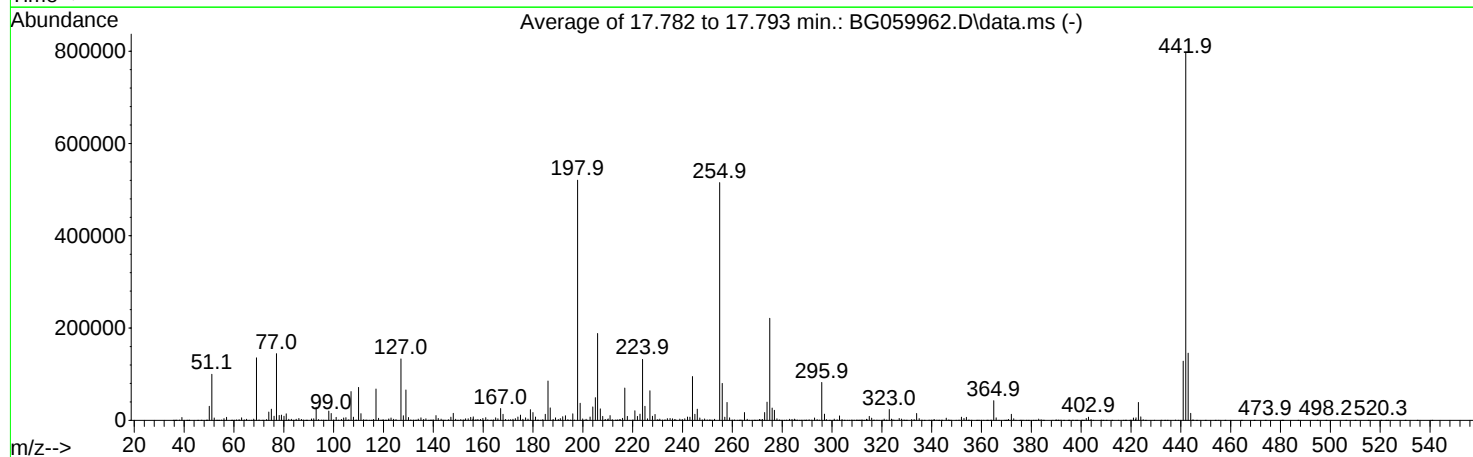


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120623\
Data File : BG059962.D
Acq On : 6 Dec 2023 9:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 05 02:26:15 2023

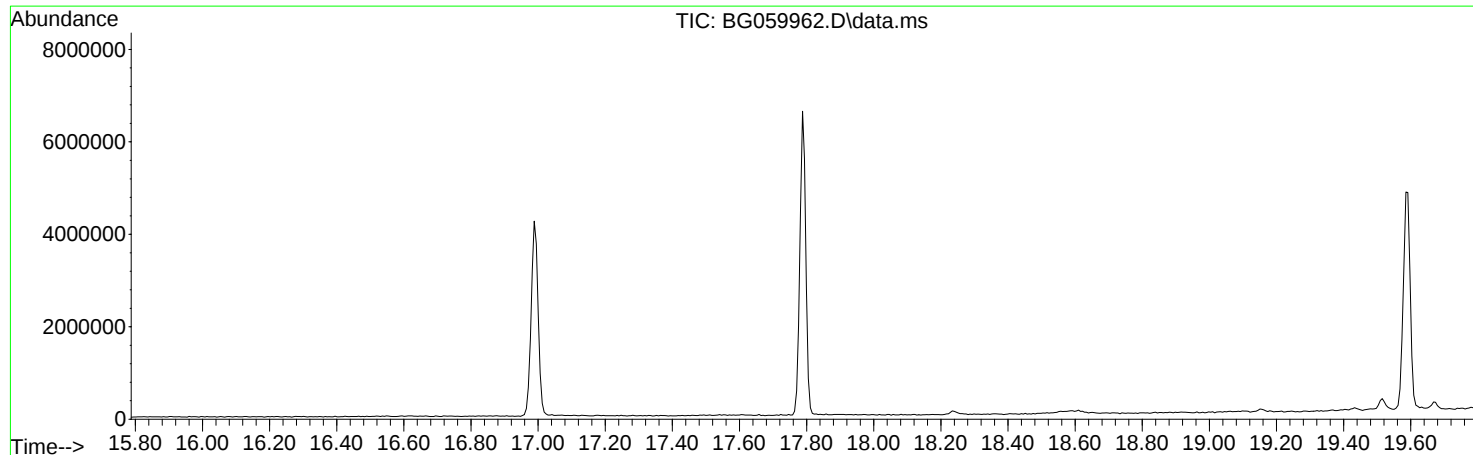




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.2	99739	PASS
68	69	0.00	2	2.0	2706	PASS
69	198	0.00	100	26.1	135682	PASS
70	69	0.00	2	0.7	1006	PASS
127	198	10	80	25.6	133179	PASS
197	198	0.00	2	0.2	866	PASS
198	198	100	100	100.0	520512	PASS
199	198	5	9	7.1	37112	PASS
275	198	10	60	42.5	221227	PASS
365	198	1	100	8.2	42643	PASS
441	198	0.01	100	24.6	128240	PASS
442	442	50	100	100.0	797141	PASS
443	442	15	24	18.3	145664	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120623\
 Data File : BG059962.D
 Acq On : 6 Dec 2023 9:49
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Dec 07 01:38:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 05 02:26:15 2023
 Response via : Initial Calibration

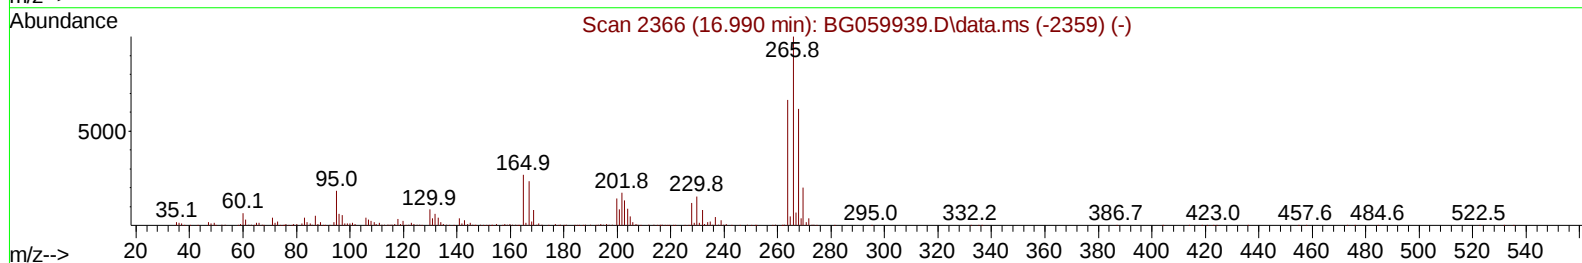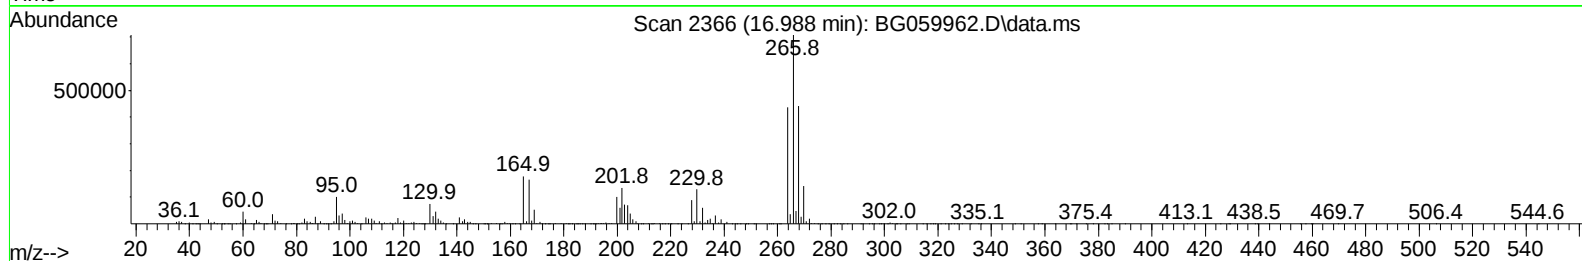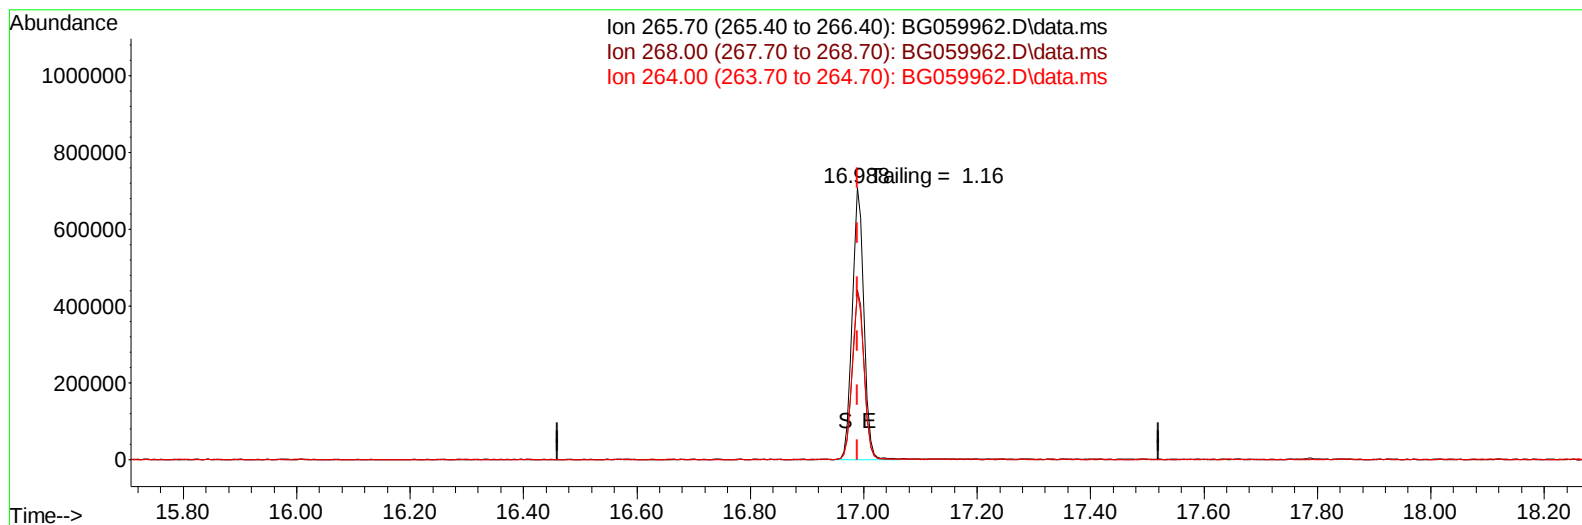

TIC: BG059962.D\data.ms

(70) Pentachlorophenol (C)

16.988min (-0.001) 366050.95 ng




response 1009884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	62.43
264.00	66.50	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120623\
Data File : BG059962.D
Acq On : 6 Dec 2023 9:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 07 01:38:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 05 02:26:15 2023
Response via : Initial Calibration

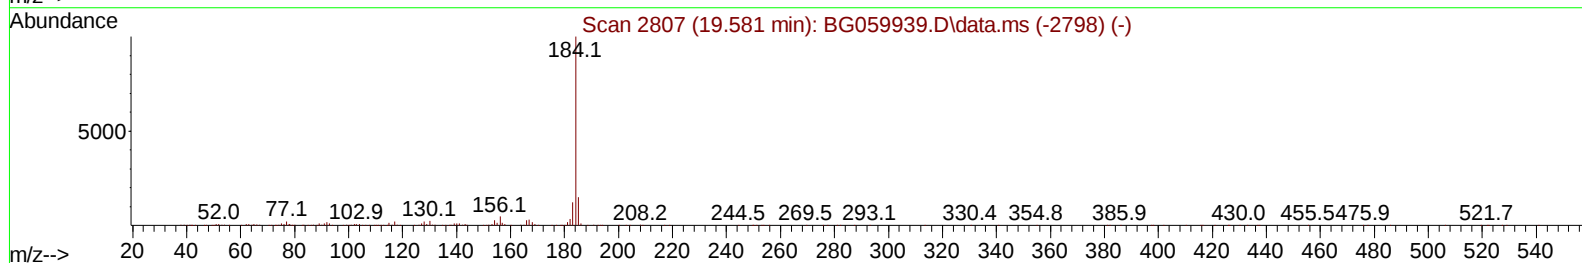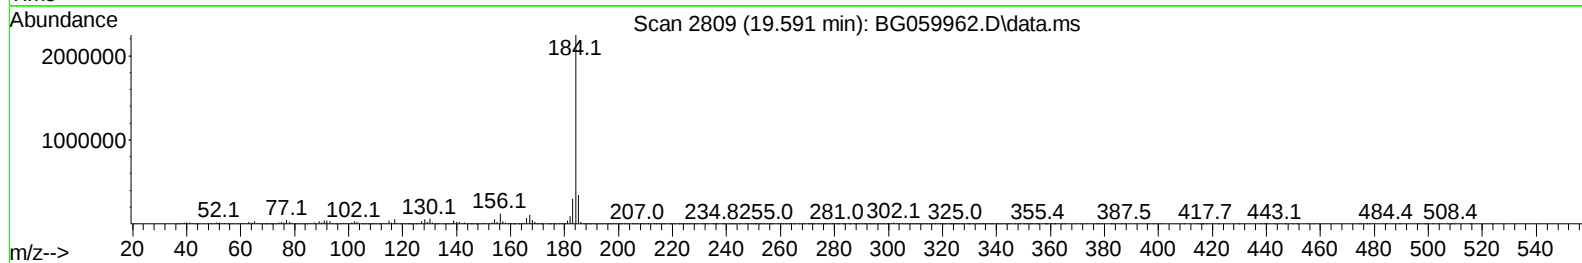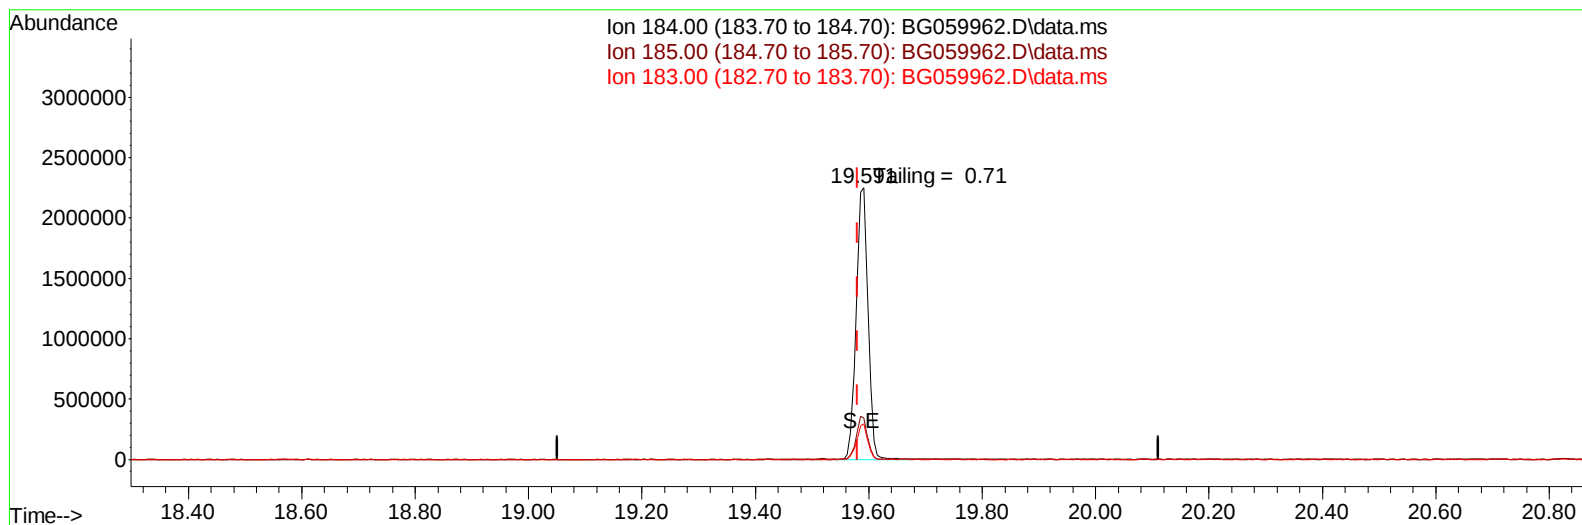

TIC: BG059962.D\data.ms

(77) Benzidine**19.591min (+ 0.010) 357485.10 ng****response 3296158**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.15
183.00	12.10	13.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2023	BNA_G	<u>BG059962.D</u>
Compound Name	Response	Retention Time
DDT	2207095	20.825
DDD	50180	20.384
DDE	1755	19.879
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
51935	2259030	2.30

Instrument :
BNA_G
ClientSampleId :
DFTPP