
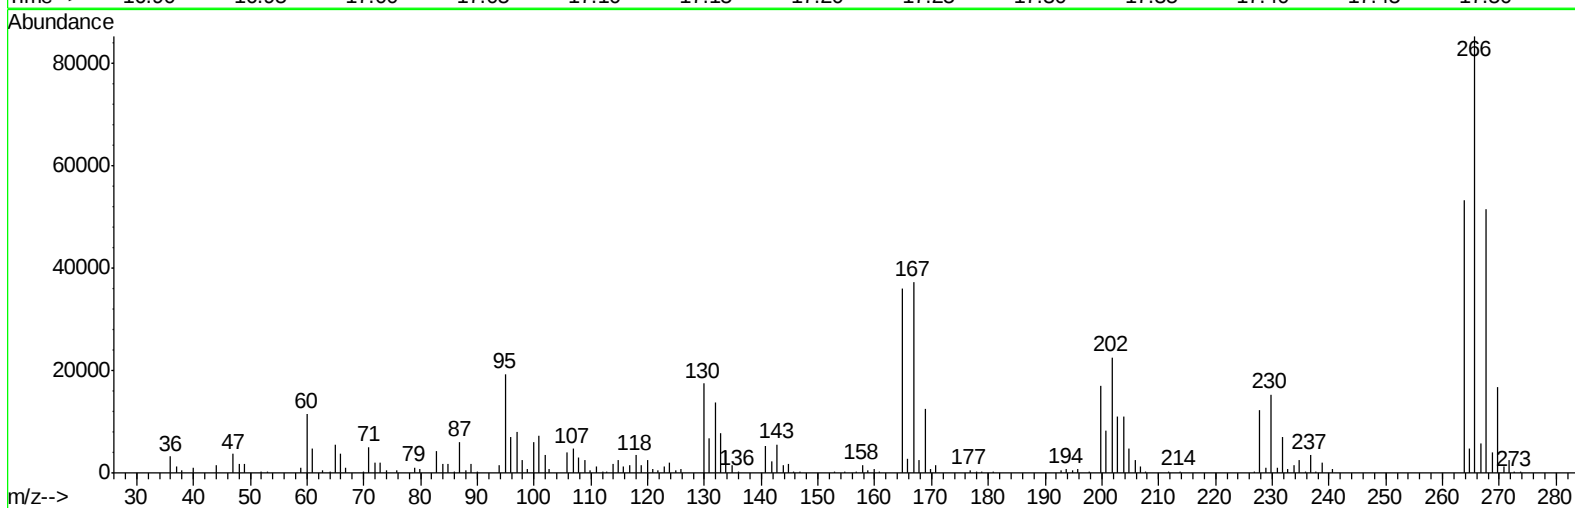


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120718\
Data File : BG038403.D
Acq On : 7 Dec 2018 14:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 05:58:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

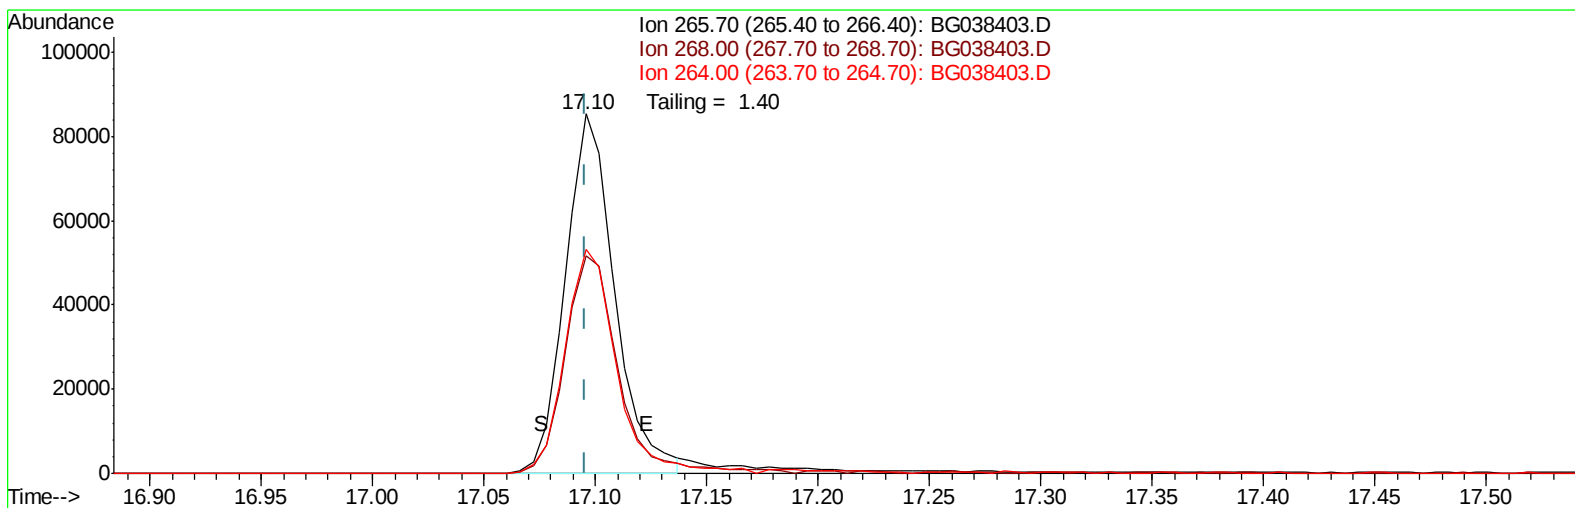

TIC: BG038403.D

(70) Pentachlorophenol (C)



17.096min (-0.000) 69997.70ng

response 138315

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	65.28
264.00	73.60	68.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120718\
Data File : BG038403.D
Acq On : 7 Dec 2018 14:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 05:58:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

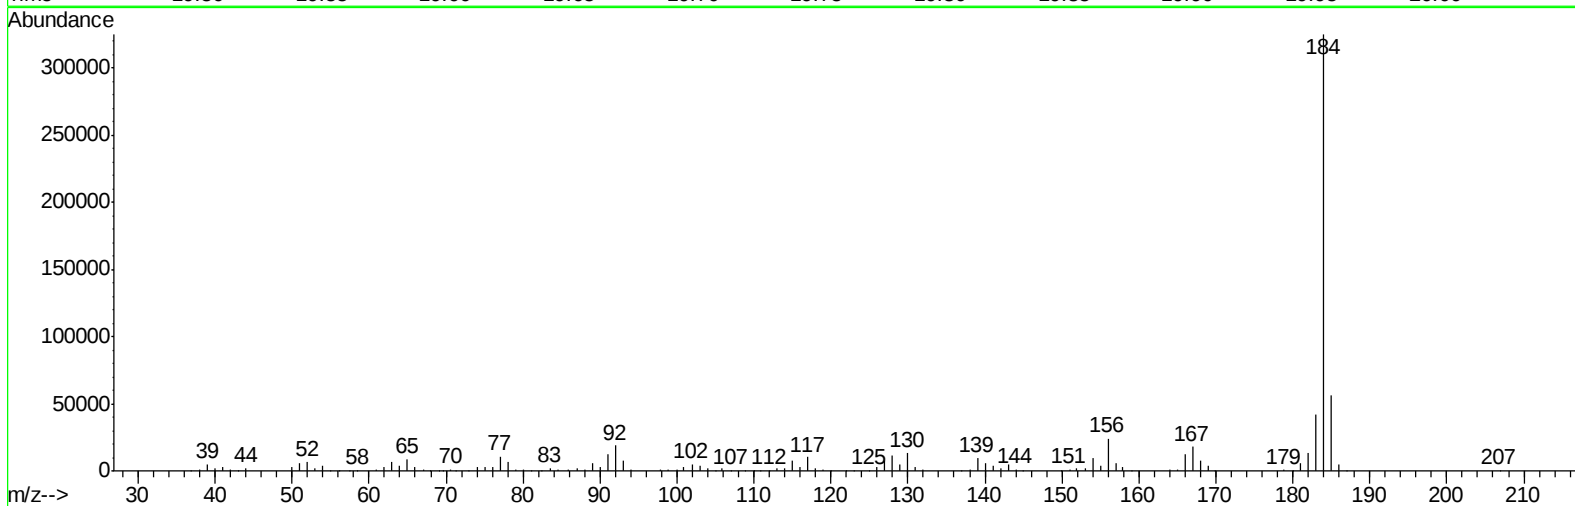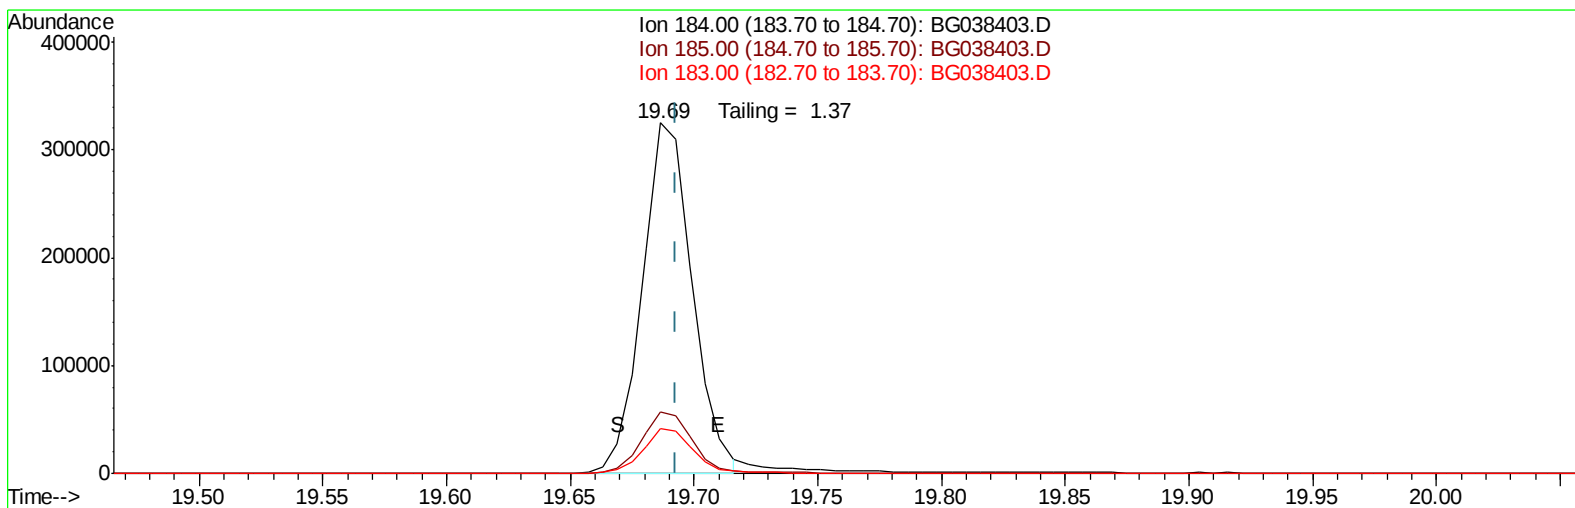

TIC: BG038403.D

(77) Benzidine

19.687min (-0.006) 6091.54ng

response 472781

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.44
183.00	12.70	12.86
0.00	0.00	0.00