
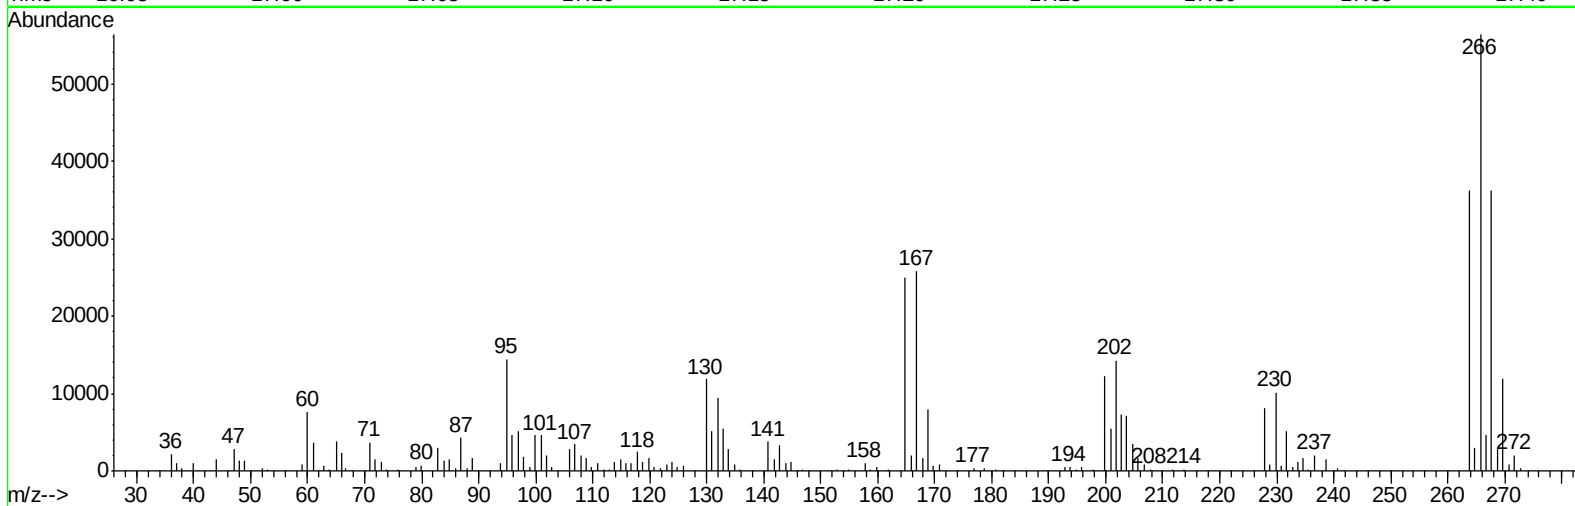


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120718\
Data File : BG038422.D
Acq On : 8 Dec 2018 4:39
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 06:05:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

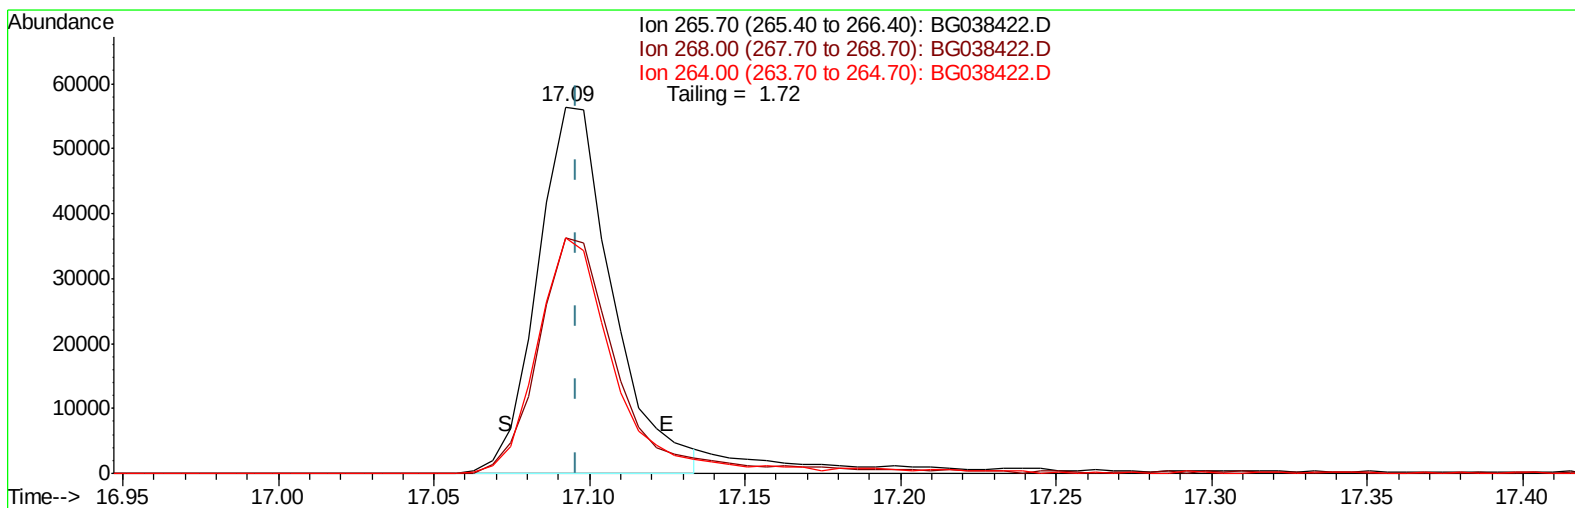

TIC: BG038422.D

(70) Pentachlorophenol (C)



17.092min (-0.004) 29504.72ng

response 100395

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.25
264.00	73.60	69.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120718\
Data File : BG038422.D
Acq On : 8 Dec 2018 4:39
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 06:05:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

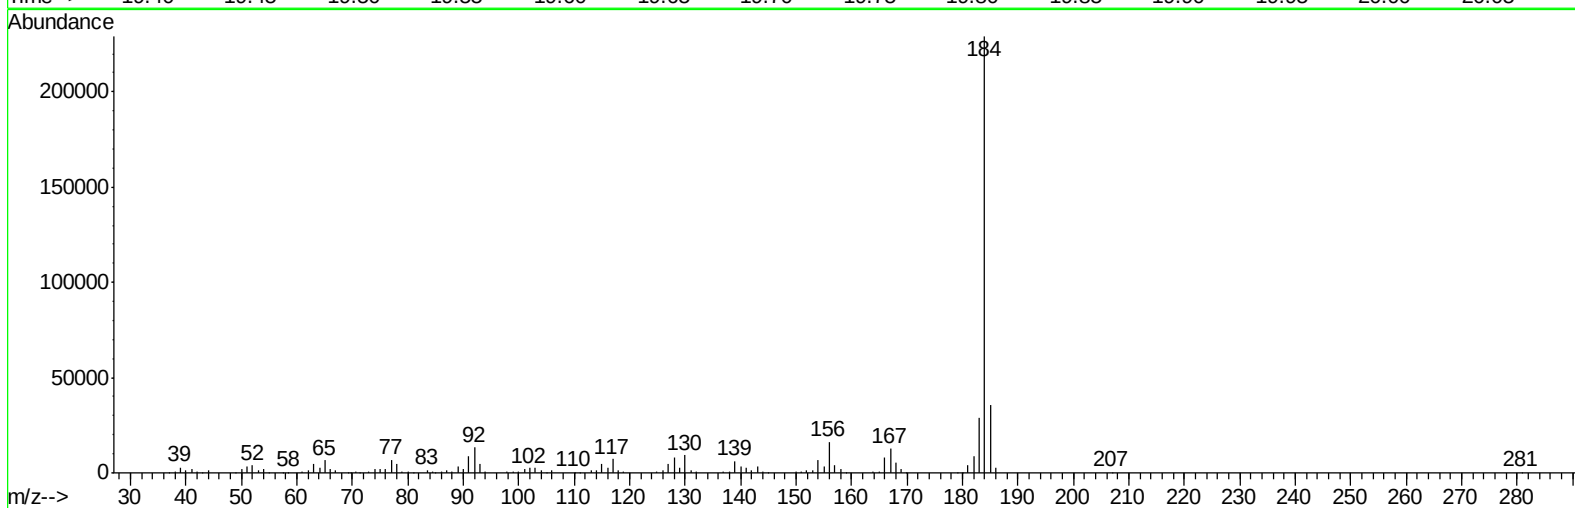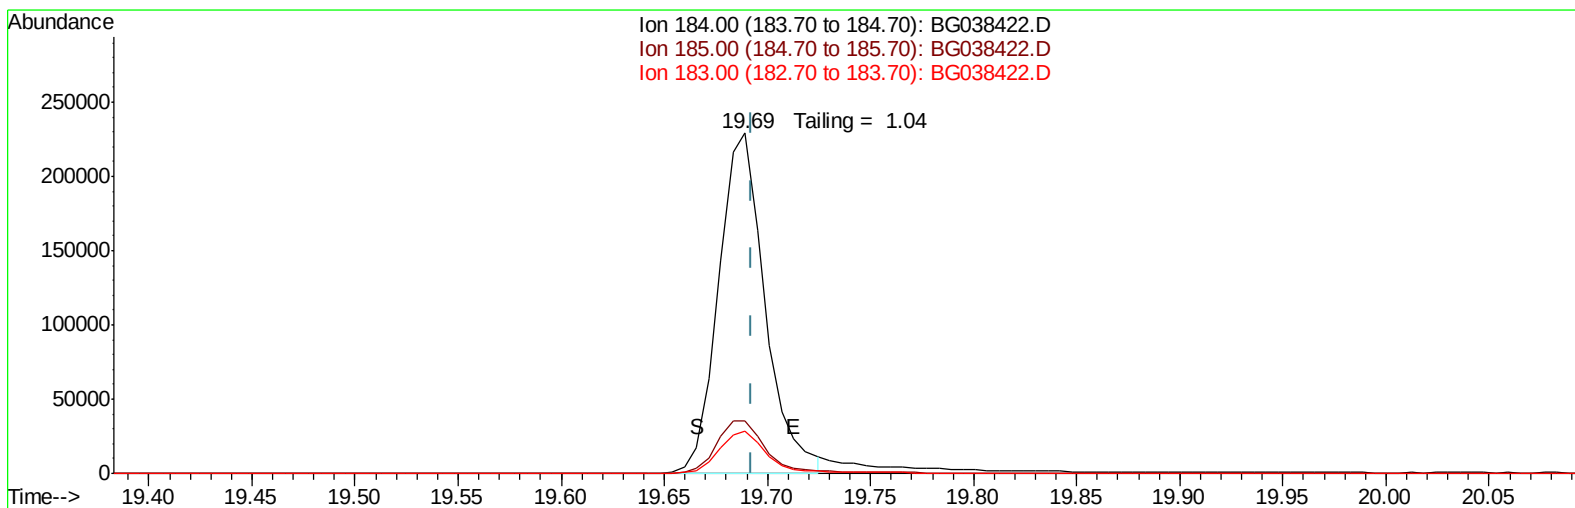

TIC: BG038422.D

(77) Benzidine

19.689min (-0.004) 52947.06ng

response 380563

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.54
183.00	12.70	12.59
0.00	0.00	0.00