

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120718\
 Data File : BG038433.D
 Acq On : 8 Dec 2018 11:54
 Operator : JU/SJ
 Sample : J6255-07RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 120518-TIPC-E-D-MRE

Quant Time: Dec 10 03:24:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 04 17:15:40 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	49373	20.00	ng	0.00
21) Naphthalene-d8	10.89	136	202370	20.00	ng	0.00
39) Acenaphthene-d10	14.70	164	135599	20.00	ng	0.00
64) Phenanthrene-d10	17.45	188	347078	20.00	ng	0.00
76) Chrysene-d12	21.73	240	485111	20.00	ng	-0.01
87) Perylene-d12	25.04	264	349265	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	62660	22.46	ng	0.00
7) Phenol-d6	7.22	99	54533	13.52	ng	0.00
23) Nitrobenzene-d5	9.24	82	245020	60.11	ng	0.00
42) 2,4,6-Tribromophenol	16.19	330	91213	54.79	ng	0.00
45) 2-Fluorobiphenyl	13.33	172	488153	51.30	ng	0.00
79) Terphenyl-d14	20.06	244	828785	36.60	ng	0.00
Target Compounds						
10) Phenol	7.25	94	9019	2.117	ng	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120718\
Data File : BG038433.D
Acq On : 8 Dec 2018 11:54
Operator : JU/SJ
Sample : J6255-07RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
120518-TIPC-E-D-MRE

Quant Time: Dec 10 03:24:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

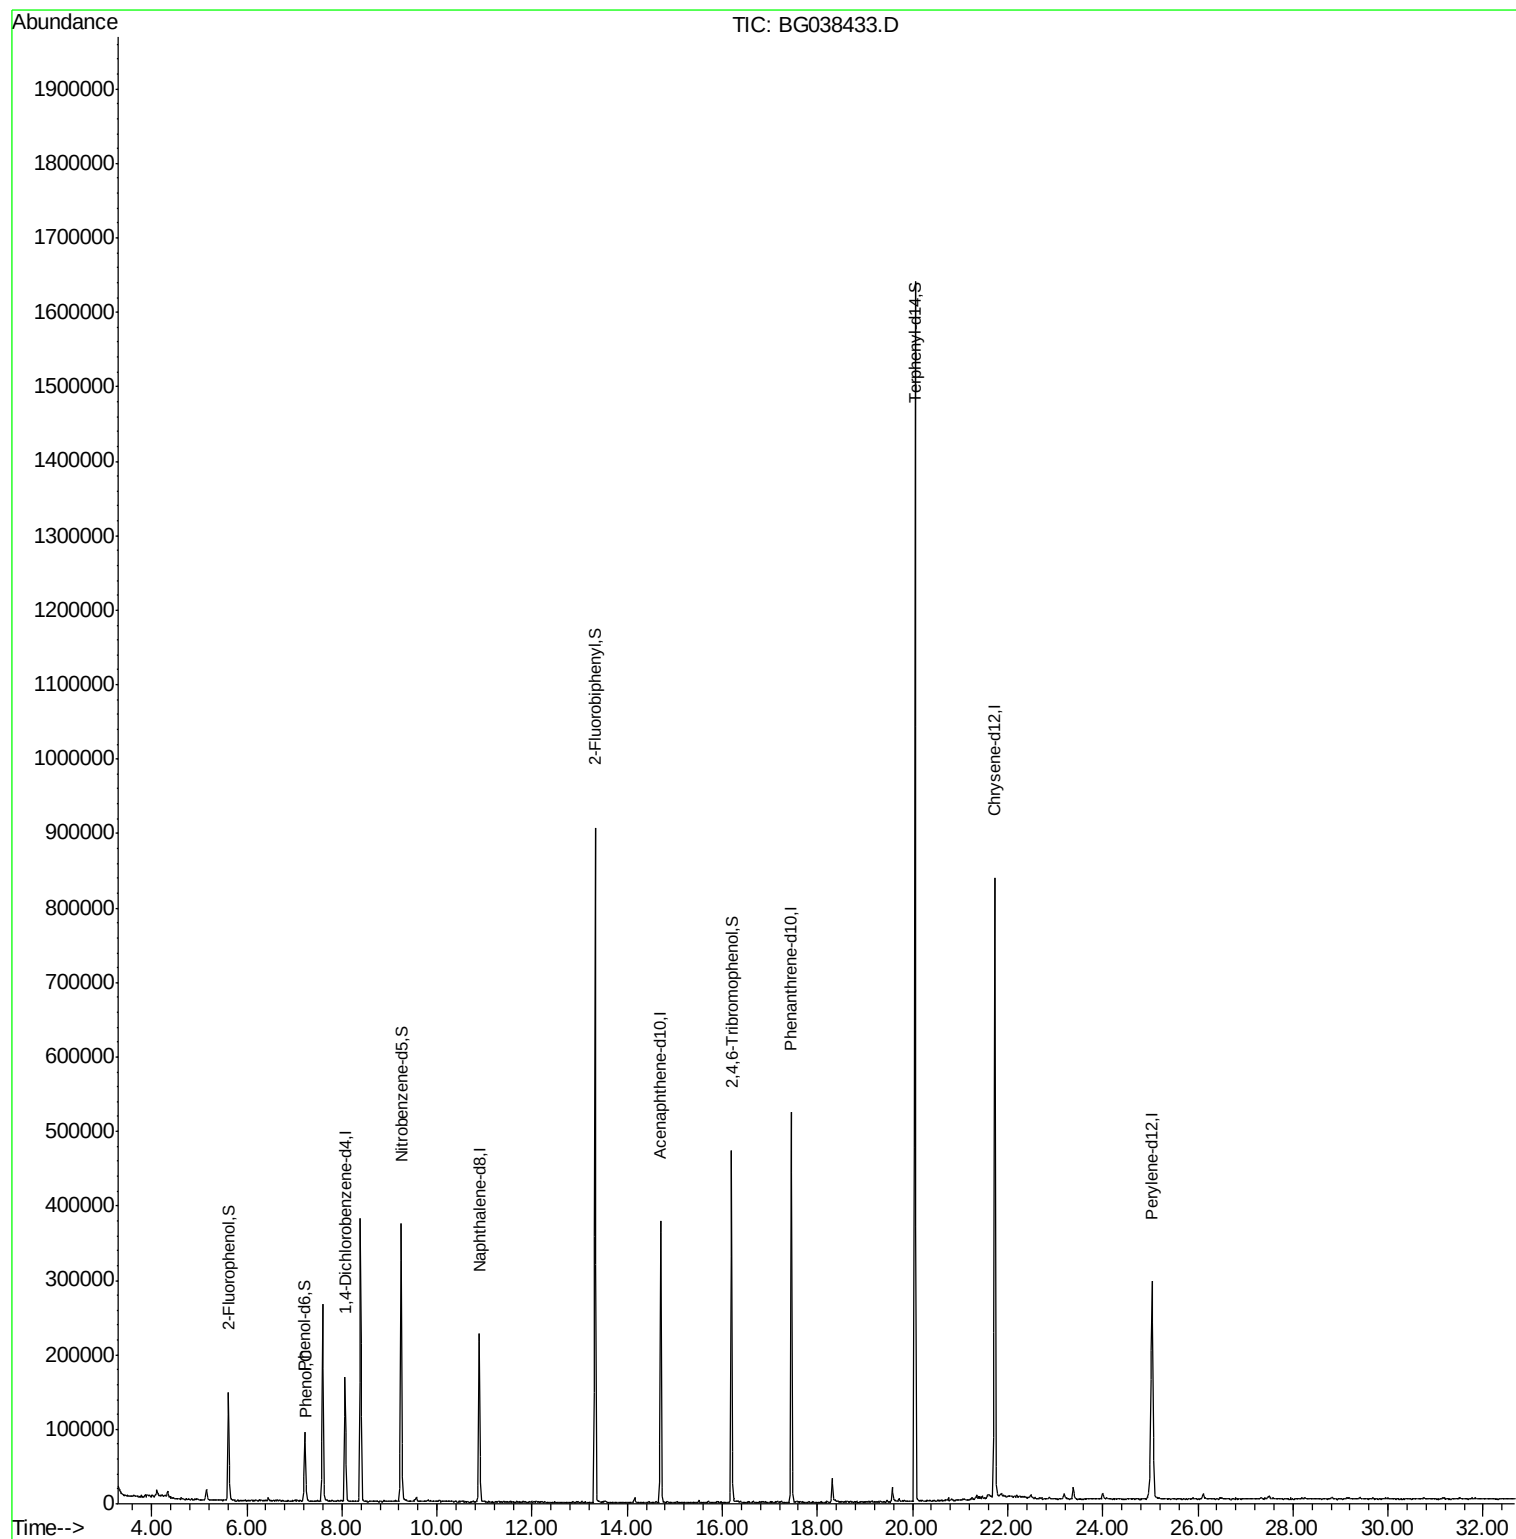

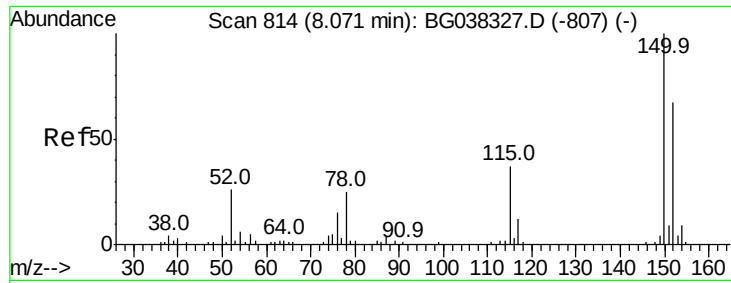


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 814
Delta R.T. -0.00 min
Lab File: BG038433.D
Acq: 8 Dec 2018 11:54

Instrument :
BNA_G
ClientSampleId :
120518-TIPC-E-D-MRE

Tot Ion:152 Resp: 49373
Ion Ratio Lower Upper
152 100
150 160.7 126.0 189.0
115 59.4 45.5 68.3

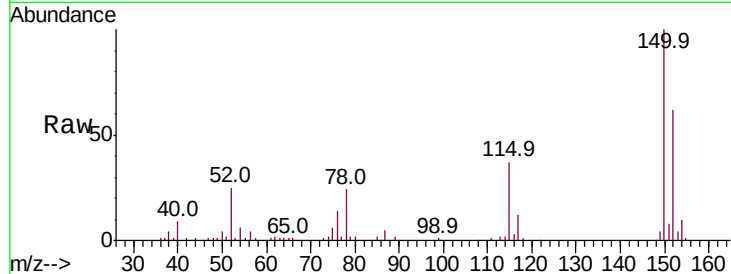


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

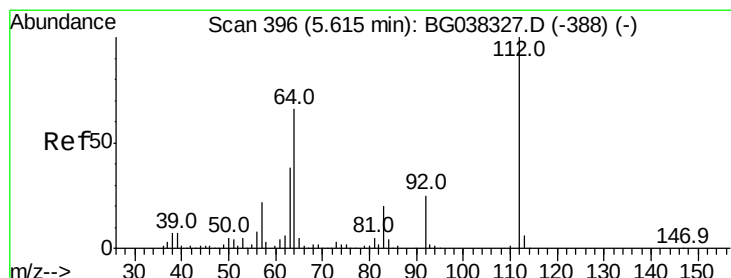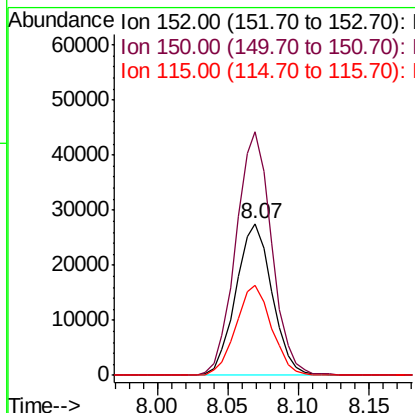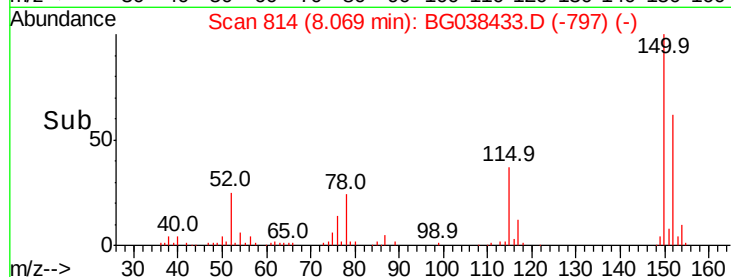



#5


2-Fluorophenol
Concen: 22.459 ng
RT: 5.61 min Scan# 396
Delta R.T. -0.00 min
Lab File: BG038433.D
Acq: 8 Dec 2018 11:54

Tgt Ion:112 Resp: 62660
Ion Ratio Lower Upper
112 100
64 65.3 53.1 79.7
63 38.4 27.3 40.9

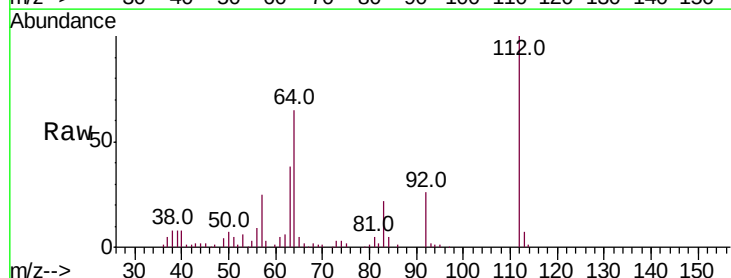

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

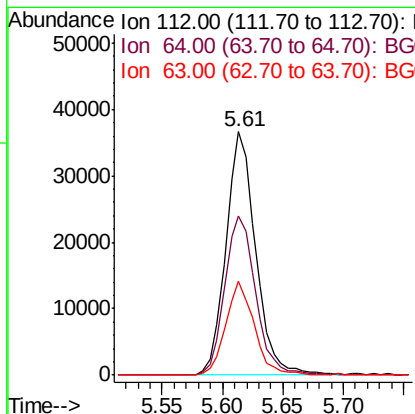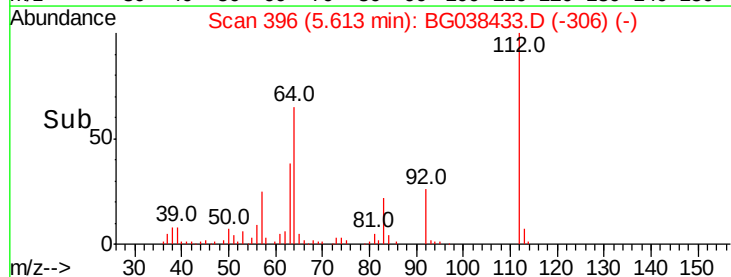

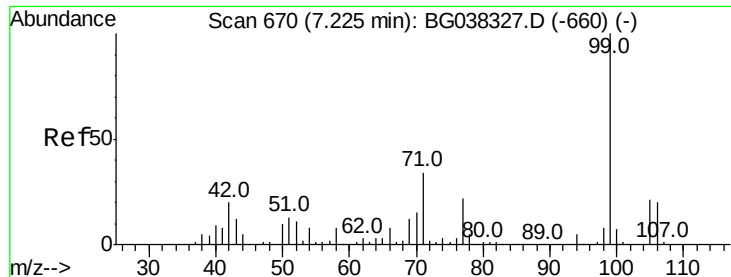

#7

Phenol-d6

Concen: 13.523 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BG038433.D

Acq: 8 Dec 2018 11:54

Instrument :

BNA_G

ClientSampleId :

120518-TIPC-E-D-MRE


Tot Ion: 99 Resp: 54533

Ion Ratio Lower Upper




99 100

42 22.1 15.0 22.4

71 34.1 25.5 38.3

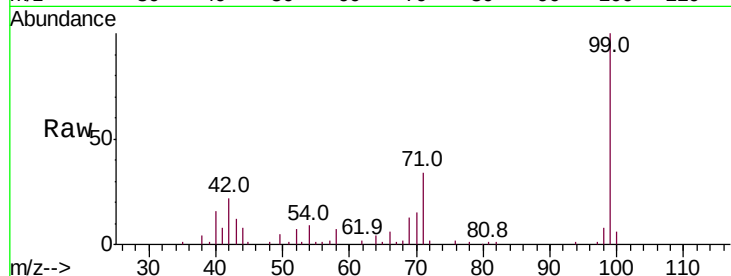

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

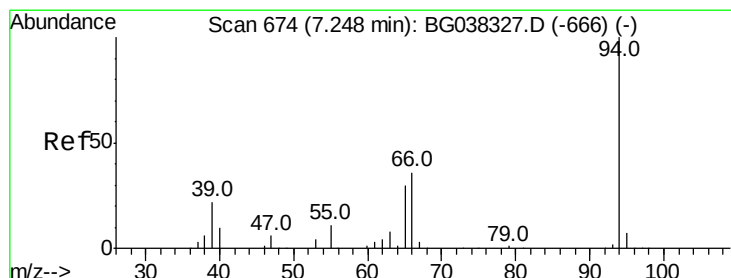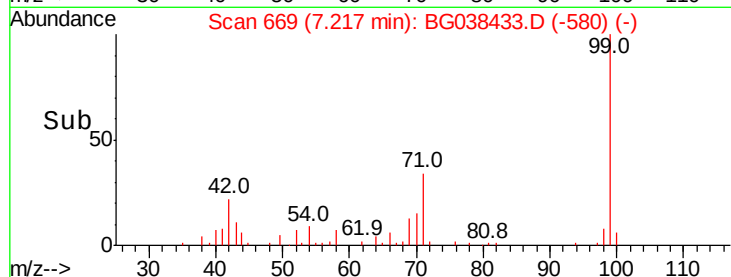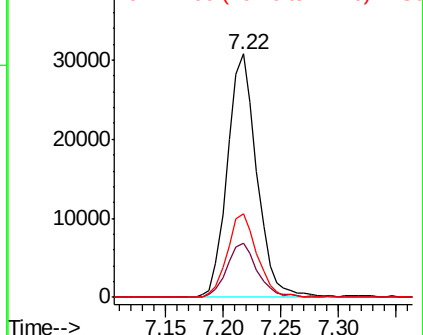

#10

Phenol

Concen: 2.117 ng

RT: 7.25 min Scan# 674

Delta R.T. -0.00 min

Lab File: BG038433.D

Acq: 8 Dec 2018 11:54


Tgt Ion: 94 Resp: 9019

Ion Ratio Lower Upper



94 100


65 38.2 9.7 49.7

66 45.7 15.9 55.9

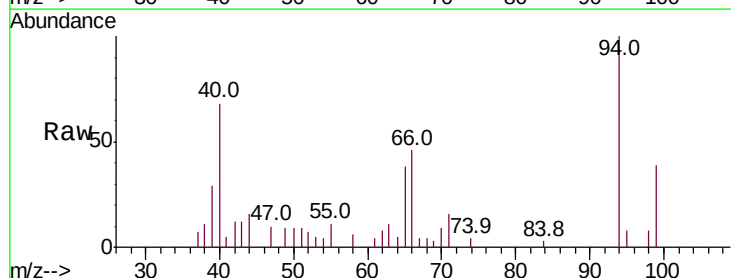

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

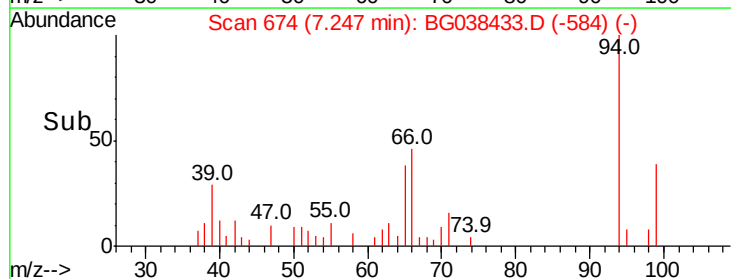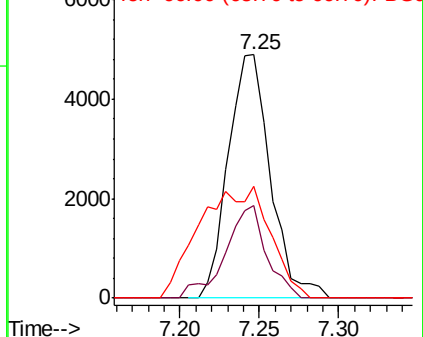


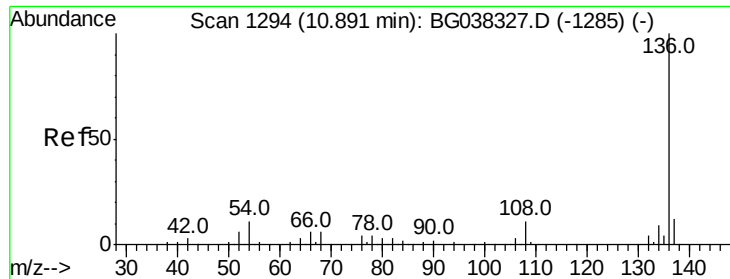




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.89 min Scan# 1294
Delta R.T. -0.00 min
Lab File: BG038433.D
Acq: 8 Dec 2018 11:54

Instrument :
BNA_G
ClientSampleId :
120518-TIPC-E-D-MRE

Tot Ion:	136	Resp:	202370
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.6	14.4
54	11.3	7.9	11.9
68	5.3	4.8	7.2

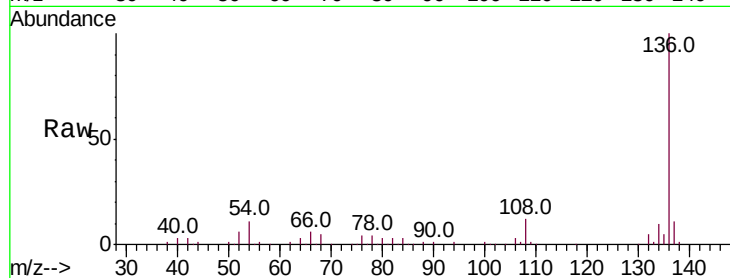


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

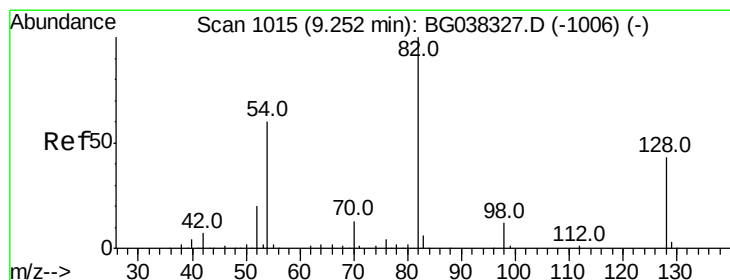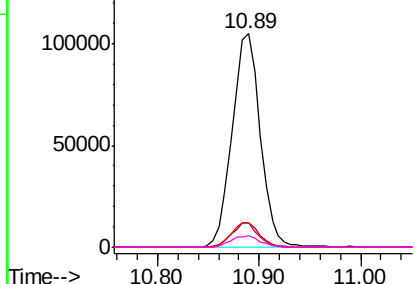
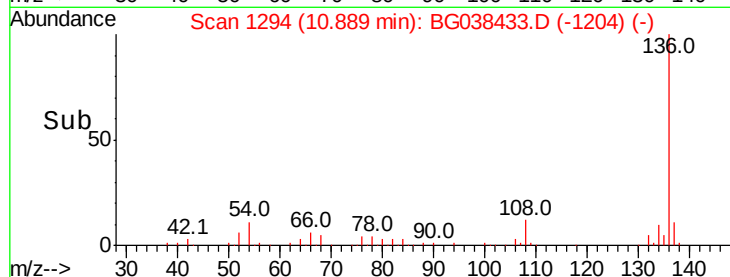



#23
Nitrobenzene-d5
Concen: 60.111 ng
RT: 9.24 min Scan# 1014
Delta R.T. -0.01 min
Lab File: BG038433.D
Acq: 8 Dec 2018 11:54

Tgt Ion:	82	Resp:	245020
Ion	Ratio	Lower	Upper
82	100		
128	44.8	34.6	51.8
54	61.3	45.3	67.9

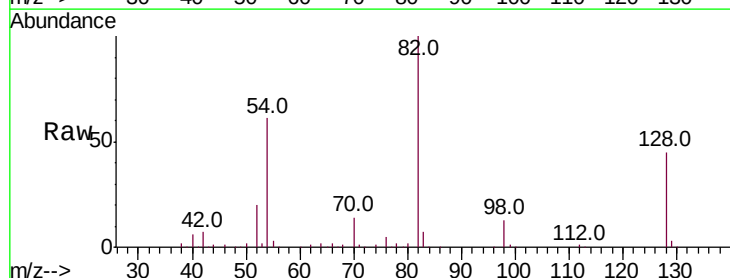

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

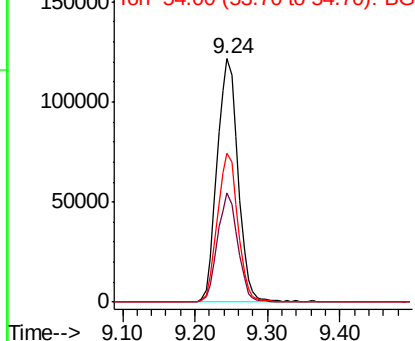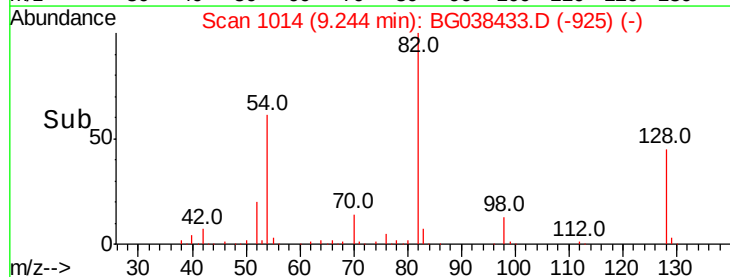

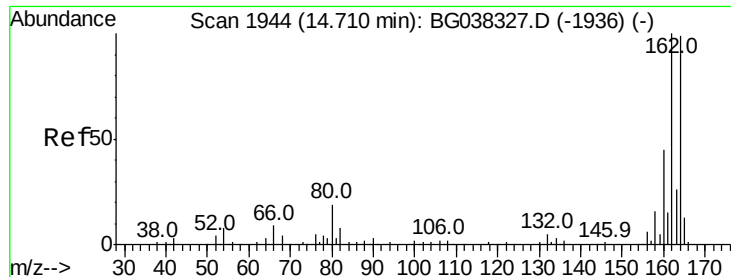

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.70 min Scan# 1943

Delta R.T. -0.01 min

Lab File: BG038433.D

Acq: 8 Dec 2018 11:54

Instrument :

BNA_G

ClientSampleId :

120518-TIPC-E-D-MRE


Tot Ion:164 Resp: 135599

Ion Ratio Lower Upper

164 100

162 104.6 81.3 121.9




160 47.3 36.3 54.5

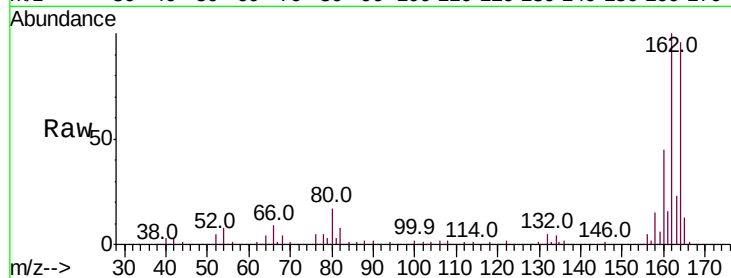

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

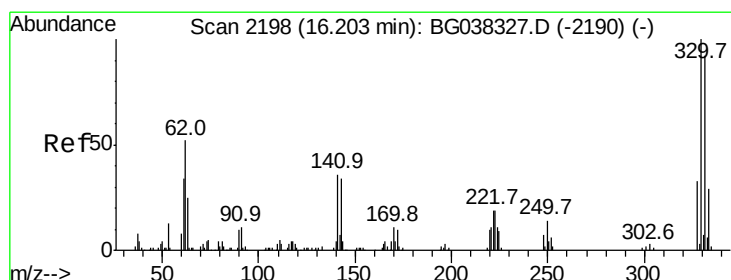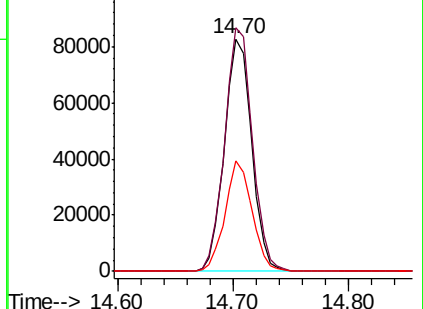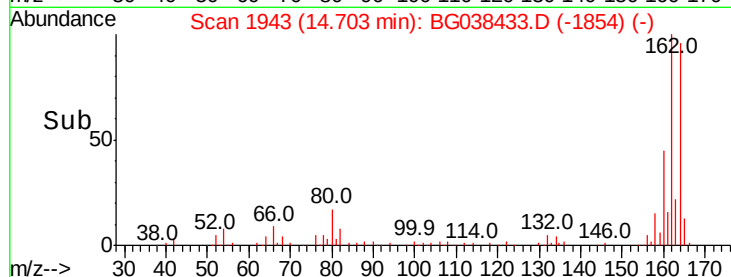

#42

2,4,6-Tribromophenol

Concen: 54.794 ng

RT: 16.19 min Scan# 2197

Delta R.T. -0.01 min

Lab File: BG038433.D

Acq: 8 Dec 2018 11:54


Tgt Ion:330 Resp: 91213

Ion Ratio Lower Upper

330 100

332 97.8 78.4 117.6



141 38.2 32.2 48.2

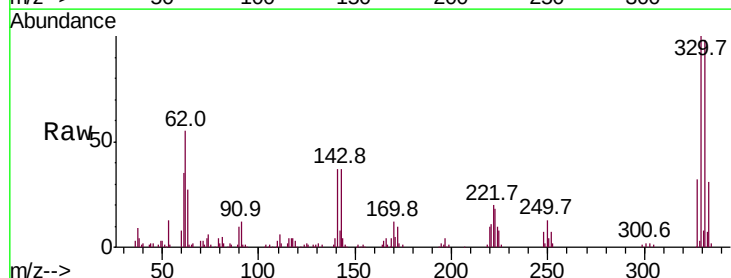


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



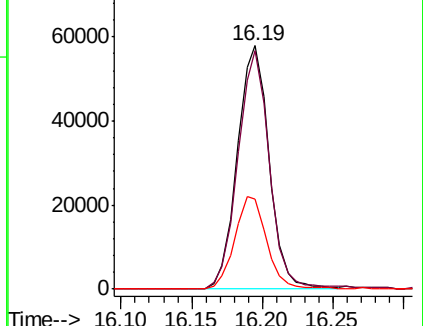
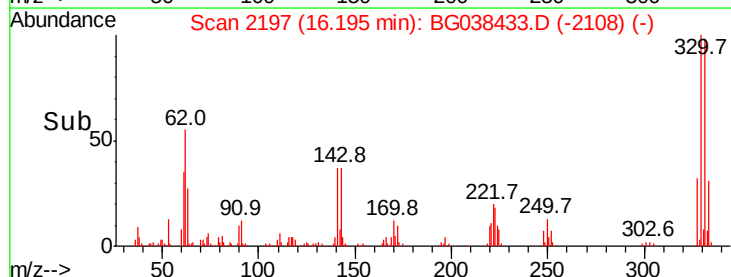


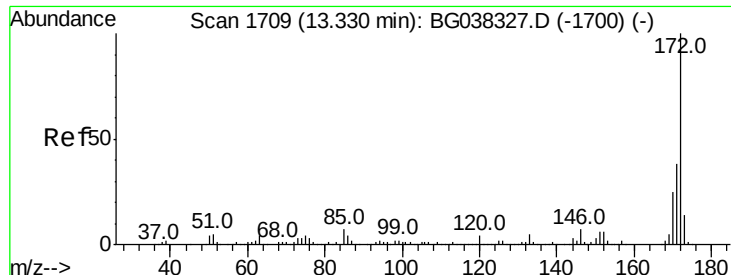

#45
 2-Fluorobiphenyl
 Concen: 51.297 ng
 RT: 13.33 min Scan# 1709
 Delta R.T. -0.00 min
 Lab File: BG038433.D
 Acq: 8 Dec 2018 11:54




Instrument :
 BNA_G
 ClientSampleId :
 120518-TIPC-E-D-MRE


Tot Ion:172 Resp: 488153
 Ion Ratio Lower Upper
 172 100
 171 36.8 31.0 46.4
 170 24.0 20.2 30.2

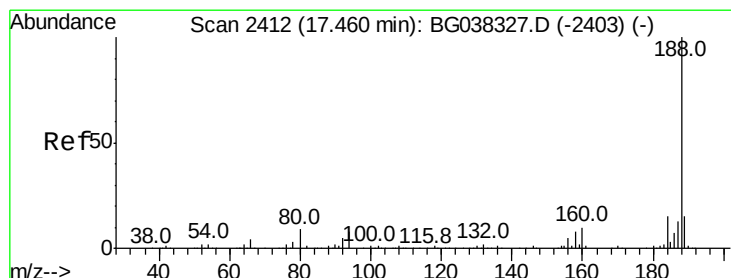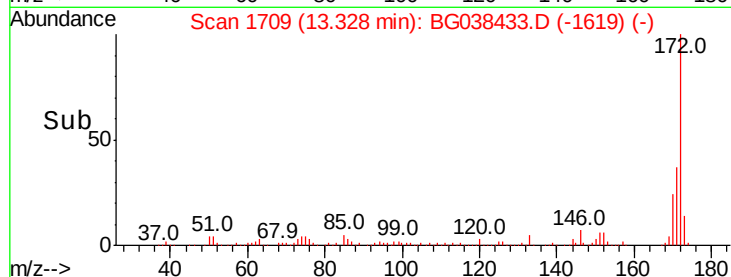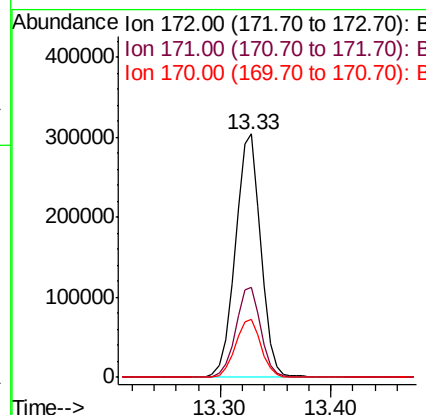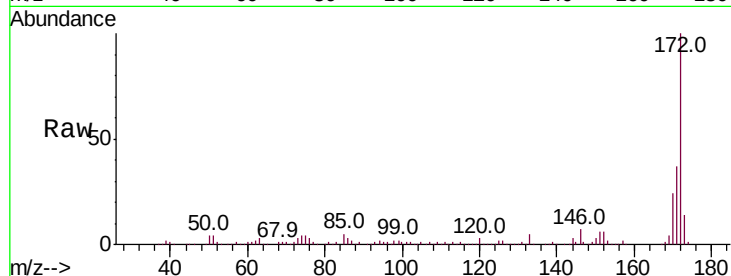

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.45 min Scan# 2411
 Delta R.T. -0.01 min
 Lab File: BG038433.D
 Acq: 8 Dec 2018 11:54

Tgt Ion:188 Resp: 347078
 Ion Ratio Lower Upper
 188 100
 94 7.0 7.2 10.8#
 80 8.5 7.7 11.5

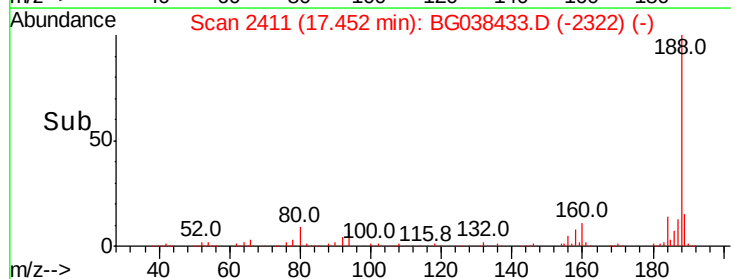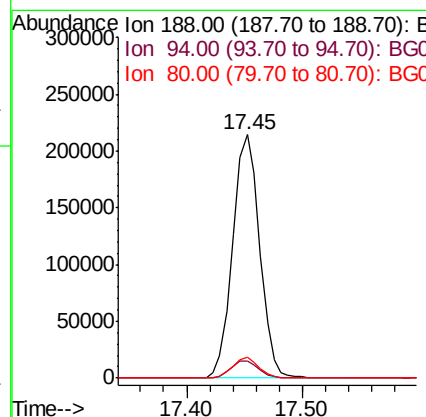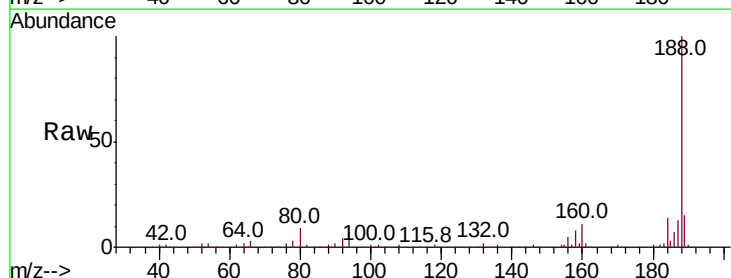

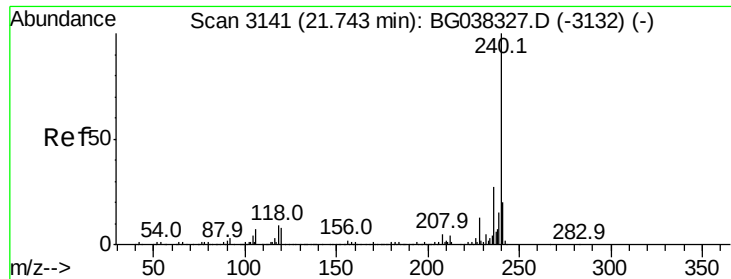

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.73 min Scan# 3139

Delta R.T. -0.01 min

Lab File: BG038433.D

Acq: 8 Dec 2018 11:54

Instrument :

BNA_G

ClientSampleId :

120518-TIPC-E-D-MRE


Tot Ion:240 Resp: 485111

Ion Ratio Lower Upper

240 100

120 11.5 8.1 12.1




236 27.7 21.4 32.0

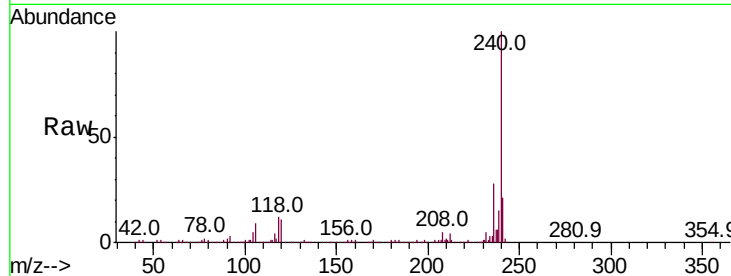

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

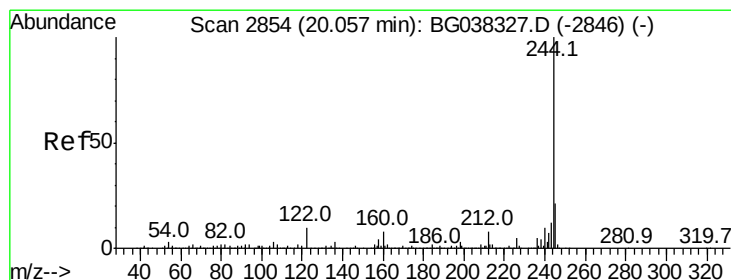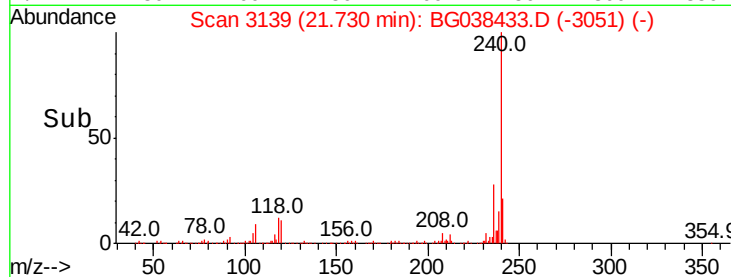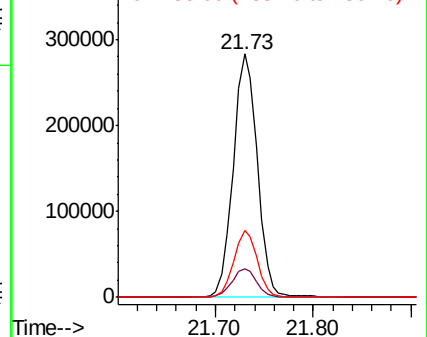

#79

Terphenyl-d14

Concen: 36.599 ng

RT: 20.06 min Scan# 2854

Delta R.T. -0.00 min

Lab File: BG038433.D

Acq: 8 Dec 2018 11:54


Tgt Ion:244 Resp: 828785

Ion Ratio Lower Upper

244 100

212 8.1 6.5 9.7



122 8.3 9.0 13.4#

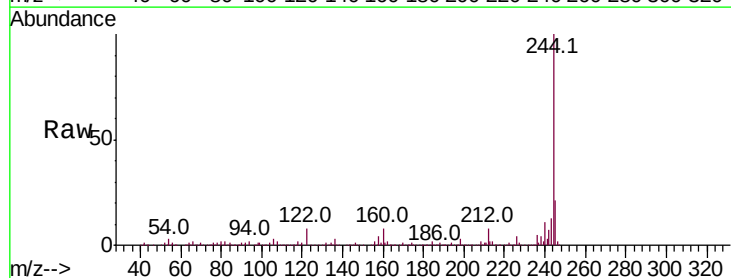


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

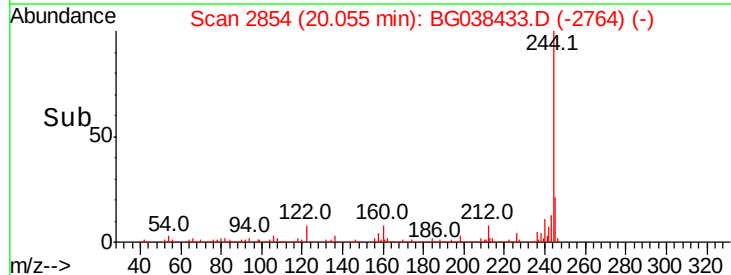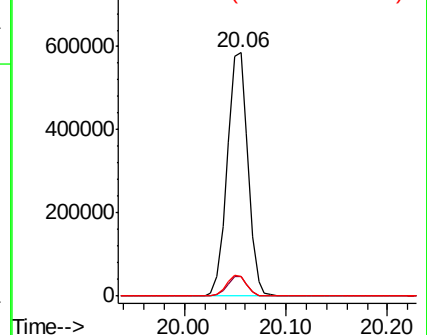

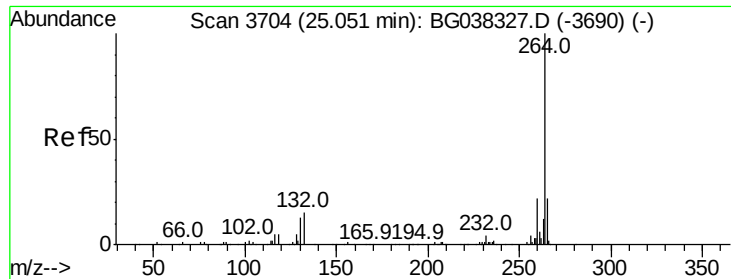

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.04 min Scan# 3702
Delta R.T. -0.01 min
Lab File: BG038433.D
Acq: 8 Dec 2018 11:54

Instrument :
BNA_G
ClientSampleId :
120518-TIPC-E-D-MRE

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	18.2	27.4
265	21.7	17.9	26.9

