


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120718\
 Data File : BG038403.D
 Acq On : 7 Dec 2018 14:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 04 17:15:40 2018

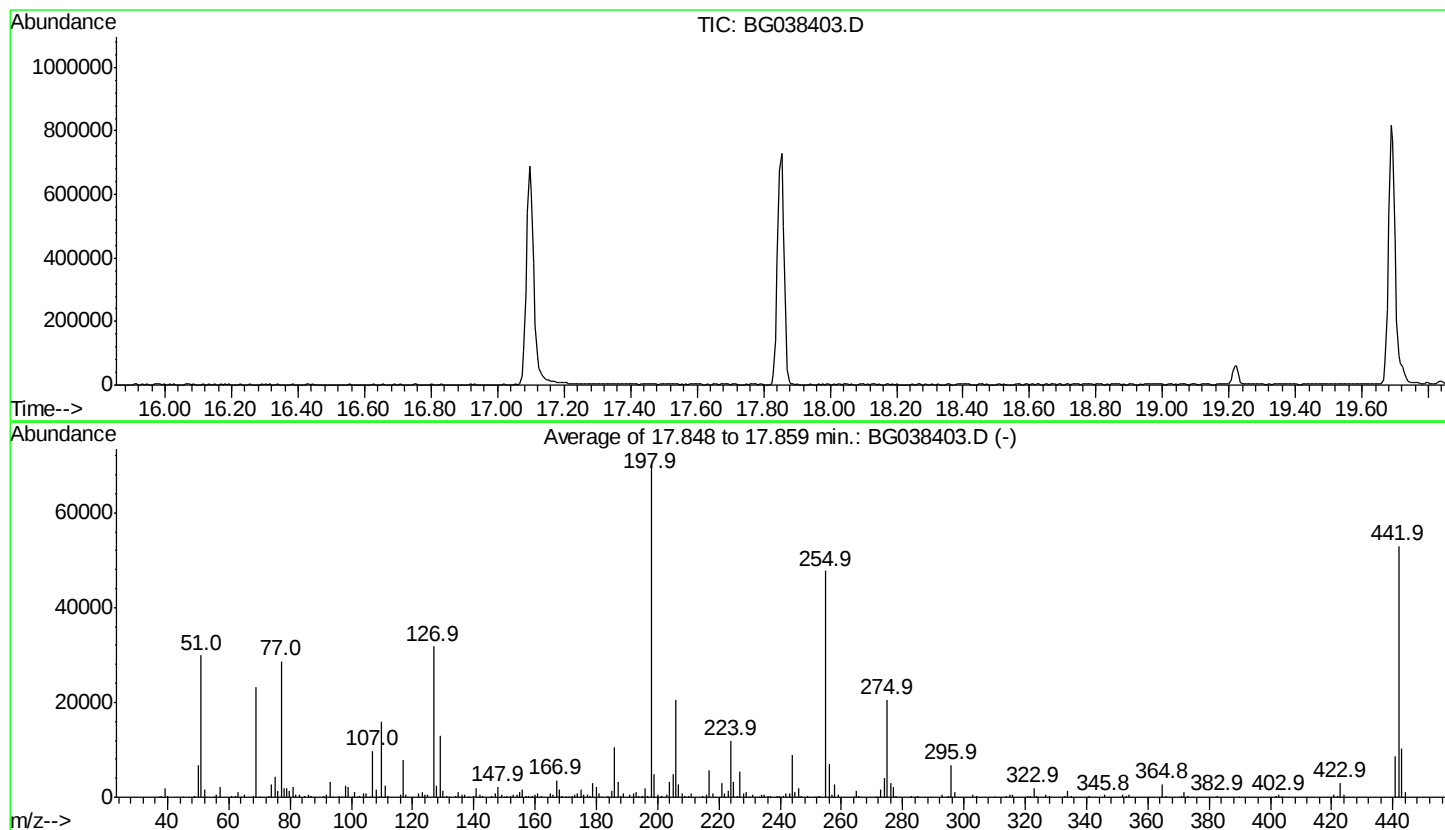

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	29898	PASS
68	69	0.00	2	0.8	178	PASS
69	198	0.00	100	33.1	23137	PASS
70	69	0.00	2	0.5	122	PASS
127	198	10	80	45.5	31794	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69925	PASS
199	198	5	9	7.0	4899	PASS
275	198	10	60	29.5	20613	PASS
365	198	1	100	3.9	2717	PASS
441	198	0.01	100	12.5	8713	PASS
442	198	50	100	75.9	53042	PASS
443	442	15	24	19.4	10283	PASS