
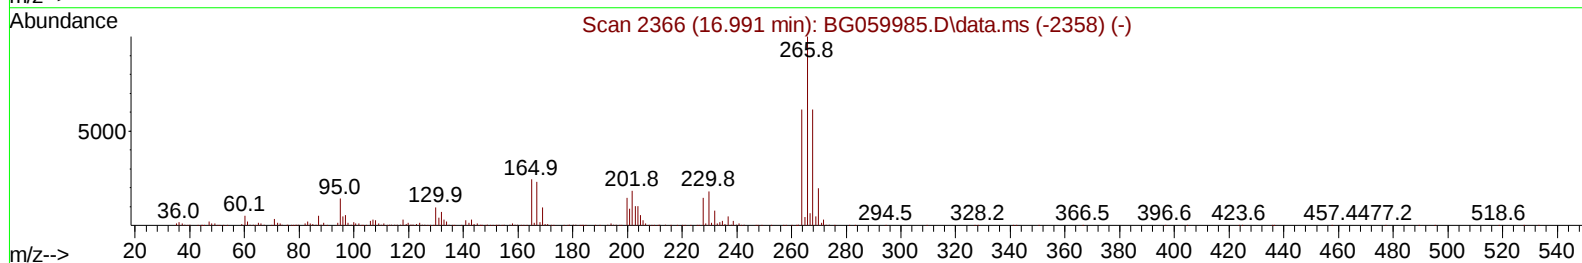
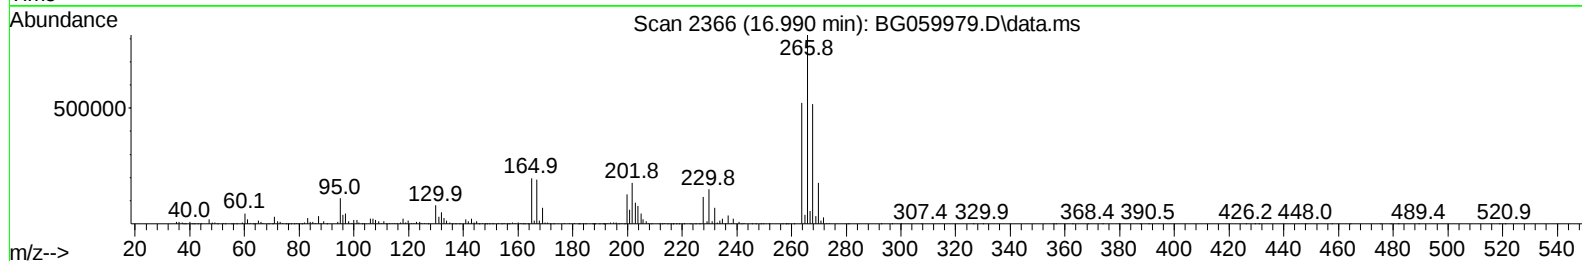


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120723\
Data File : BG059979.D
Acq On : 7 Dec 2023 9:56
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 18:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 07 17:14:16 2023
Response via : Initial Calibration

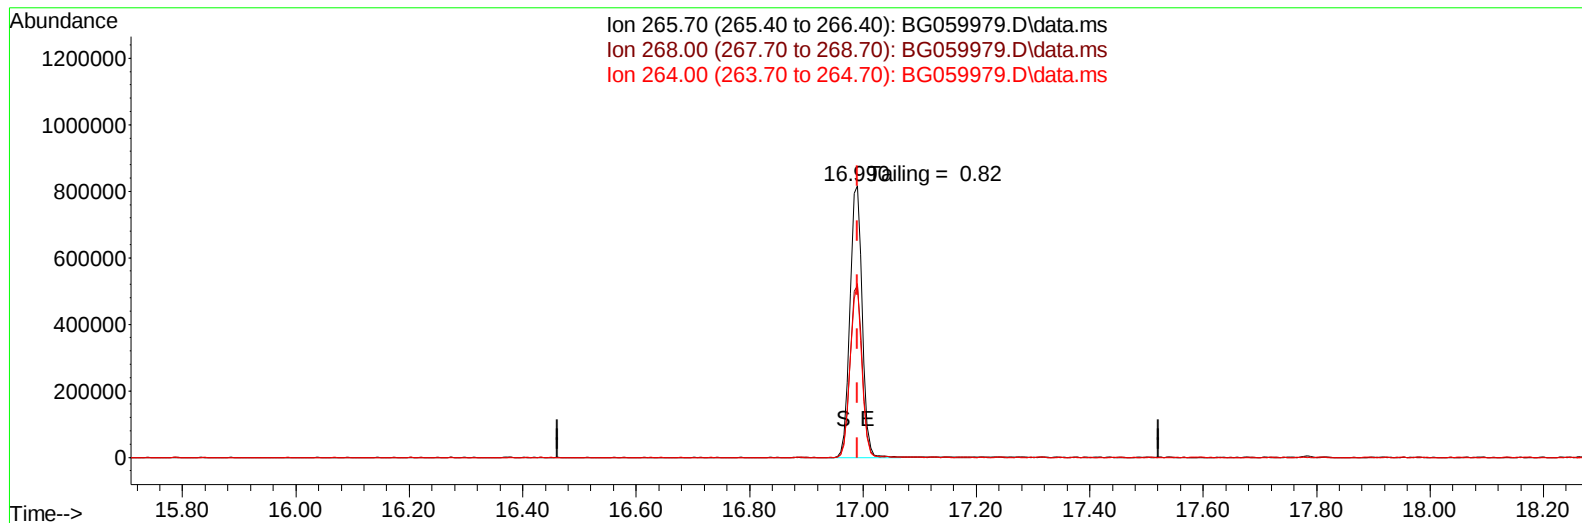




TIC: BG059979.D\data.ms

(70) Pentachlorophenol (C)**16.990min (-0.001) 902313.41 ng****response 1221749**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	63.29
264.00	61.40	63.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120723\
Data File : BG059979.D
Acq On : 7 Dec 2023 9:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 18:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 07 17:14:16 2023
Response via : Initial Calibration

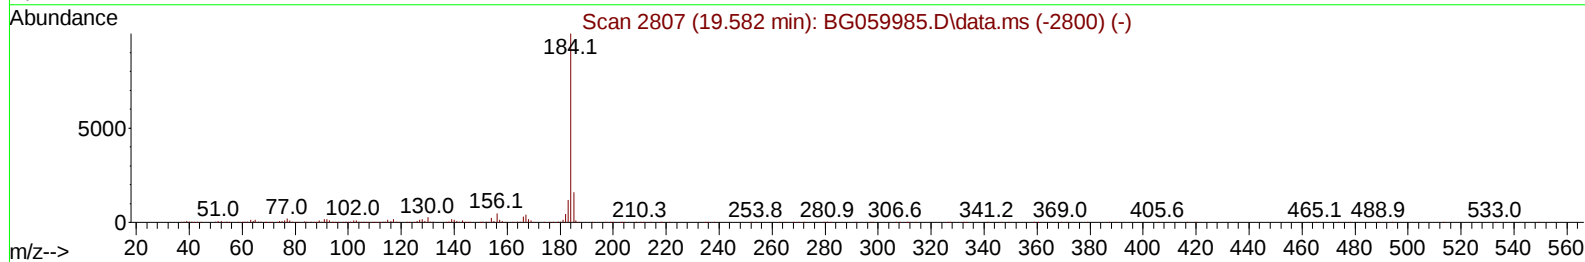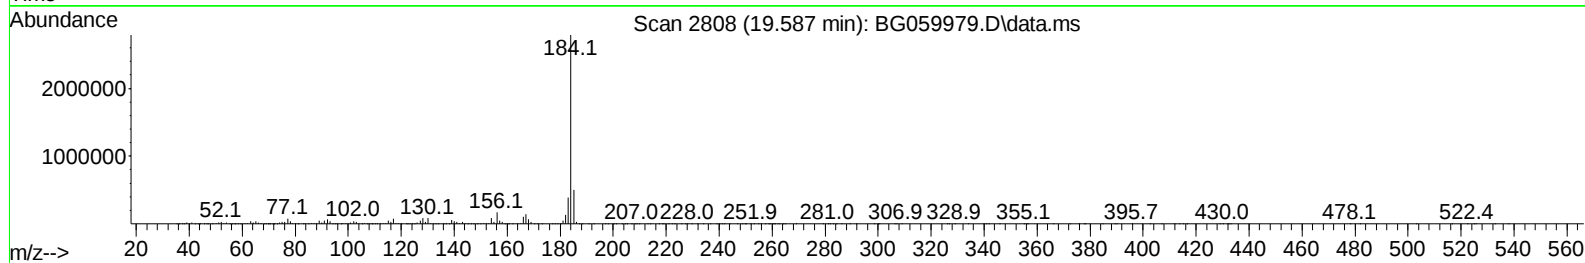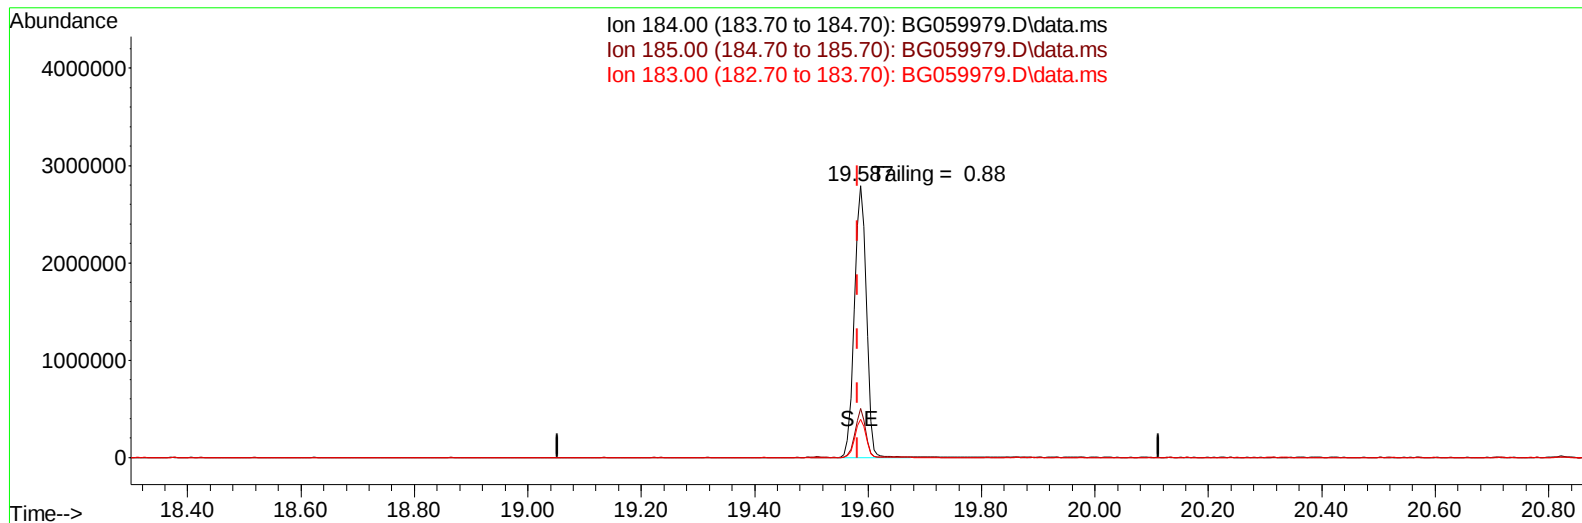

TIC: BG059979.D\data.ms

(77) Benzidine**19.587min (+ 0.005) 970544.01 ng****response 4122027**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.90	17.98
183.00	12.00	13.97
0.00	0.00	0.00