

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG120723\  
Data File : BG059990.D  
Acq On : 7 Dec 2023 17:22  
Operator : MA/JU  
Sample : PB157585BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157585BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG120723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG059990.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.530       | 406           | 415         | 422          | rBV      | 2642880        | 4143844       | 16.63%          | 5.676%        |
| 2         | 7.116       | 676           | 685         | 691          | rBV      | 2790077        | 4584221       | 18.40%          | 6.279%        |
| 3         | 7.956       | 821           | 828         | 836          | rBV      | 507989         | 800912        | 3.21%           | 1.097%        |
| 4         | 9.120       | 1017          | 1026        | 1037         | rVB      | 1478726        | 2558273       | 10.27%          | 3.504%        |
| 5         | 10.759      | 1298          | 1305        | 1314         | rVB      | 533395         | 951445        | 3.82%           | 1.303%        |
| 6         | 13.221      | 1715          | 1724        | 1733         | rBV      | 5858966        | 8993789       | 36.09%          | 12.319%       |
| 7         | 14.595      | 1952          | 1958        | 1964         | rBV      | 1045570        | 1617740       | 6.49%           | 2.216%        |
| 8         | 16.082      | 2204          | 2211        | 2220         | rBV      | 7776397        | 11372984      | 45.64%          | 15.577%       |
| 9         | 17.345      | 2419          | 2426        | 2432         | rBV      | 1891490        | 2835155       | 11.38%          | 3.883%        |
| 10        | 19.966      | 2866          | 2872        | 2878         | rBV      | 17697866       | 24918479      | 100.00%         | 34.130%       |
| 11        | 21.611      | 3146          | 3152        | 3159         | rVB2     | 3067839        | 4891829       | 19.63%          | 6.700%        |
| 12        | 24.807      | 3683          | 3696        | 3706         | rBV      | 1963848        | 5341198       | 21.43%          | 7.316%        |




Sum of corrected areas: 73009869

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG120723\  
Data File : BG059990.D  
Acq On : 7 Dec 2023 17:22  
Operator : MA/JU  
Sample : PB157585BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157585BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG120723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

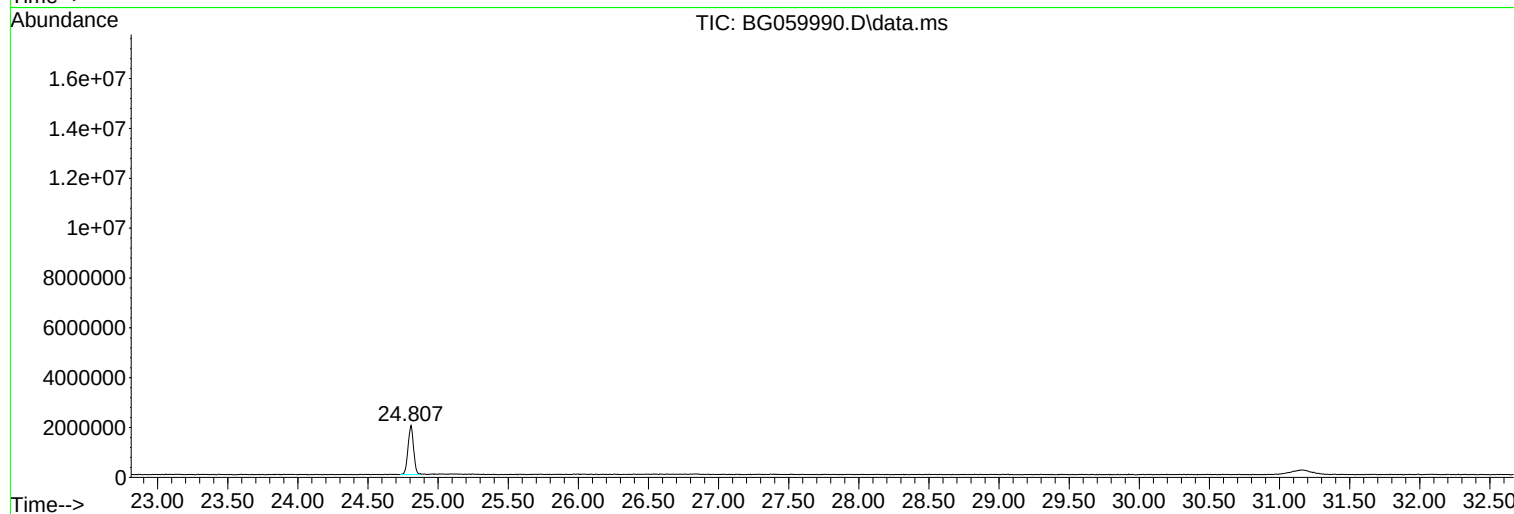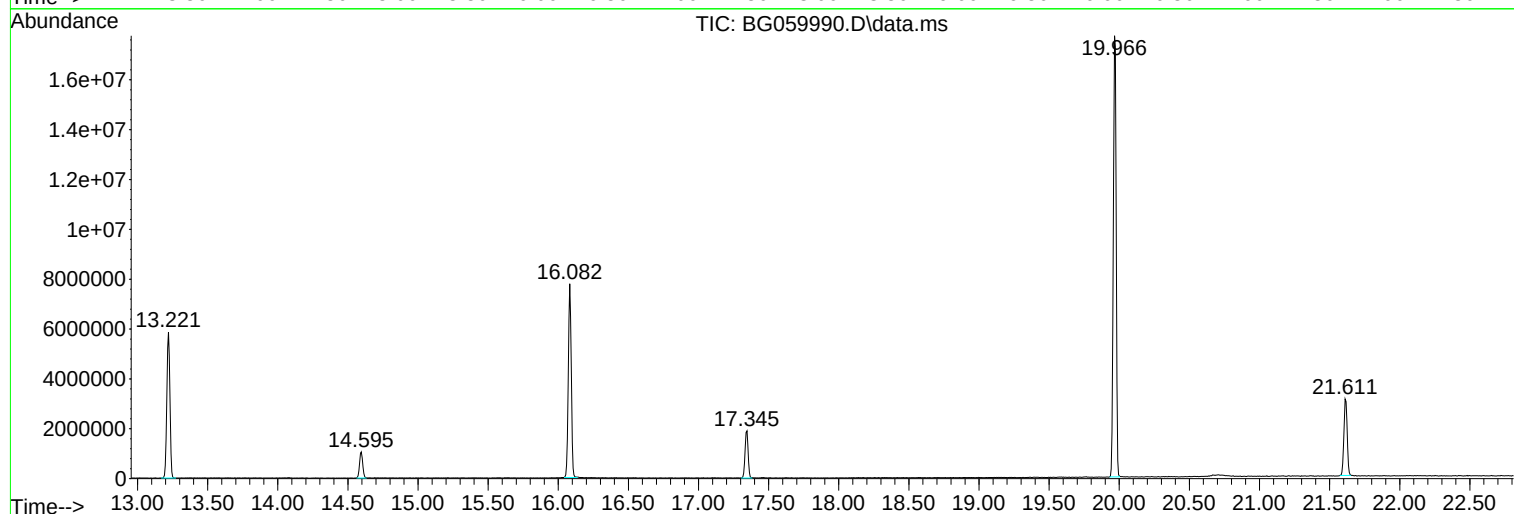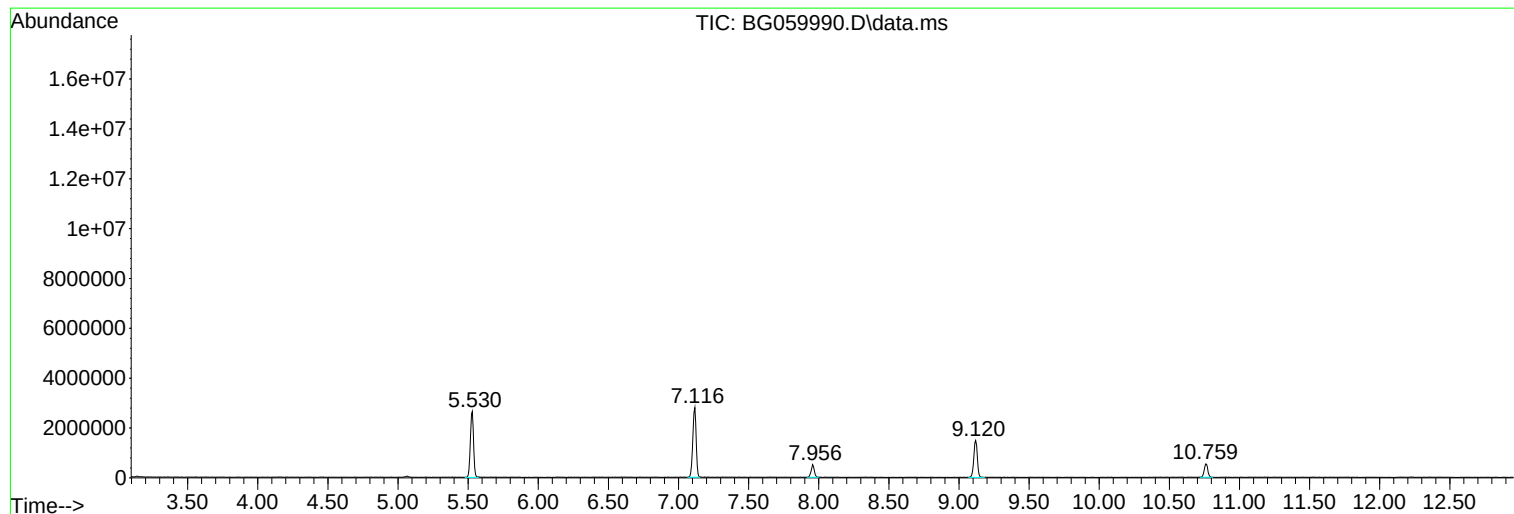

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG120723\  
Data File : BG059990.D  
Acq On : 7 Dec 2023 17:22  
Operator : MA/JU  
Sample : PB157585BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157585BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG120723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG120723\  
Data File : BG059990.D  
Acq On : 7 Dec 2023 17:22  
Operator : MA/JU  
Sample : PB157585BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157585BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG120723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|