


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120723\
Data File : BG059979.D
Acq On : 7 Dec 2023 9:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 08 02:35:41 2023

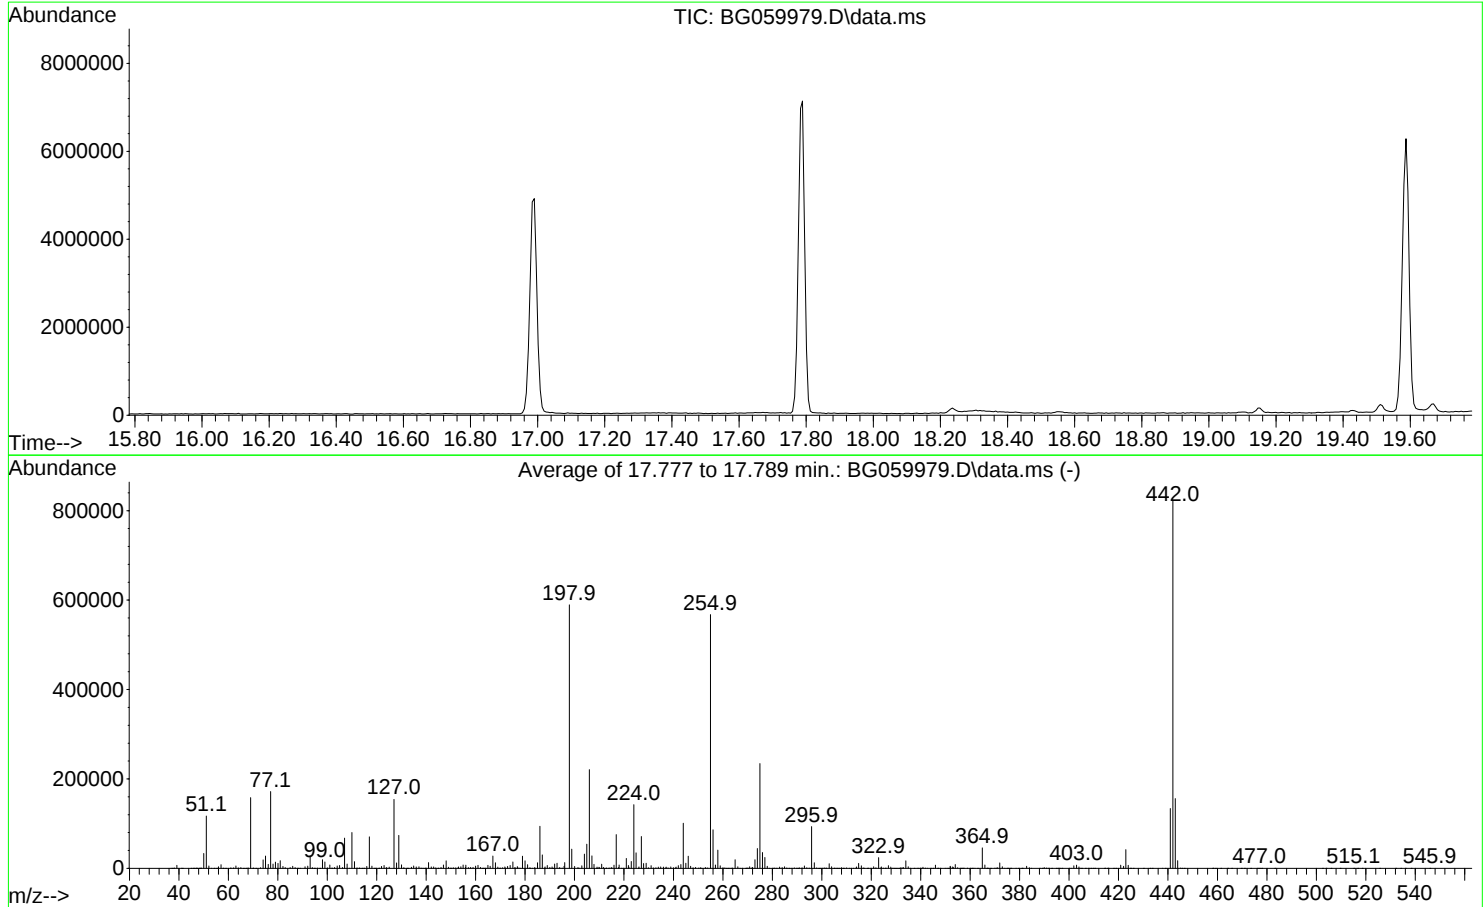




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.8	116864	PASS
68	69	0.00	2	0.6	982	PASS
69	198	0.00	100	26.8	158176	PASS
70	69	0.00	2	0.5	823	PASS
127	198	10	80	26.2	154461	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	589397	PASS
199	198	5	9	7.3	43123	PASS
275	198	10	60	39.8	234572	PASS
365	198	1	100	7.8	45952	PASS
441	198	0.01	100	22.7	134000	PASS
442	442	50	100	100.0	822784	PASS
443	442	15	24	19.0	155949	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120723\
Data File : BG059979.D
Acq On : 7 Dec 2023 9:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 07 18:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 07 17:14:16 2023
Response via : Initial Calibration

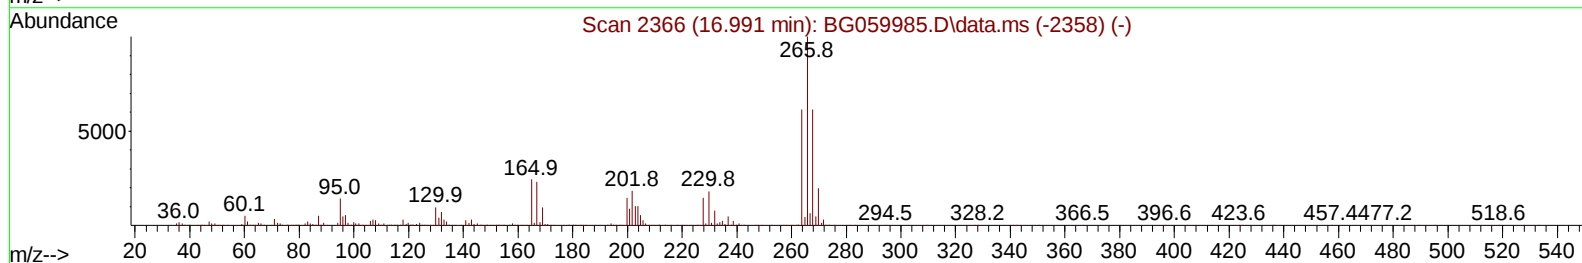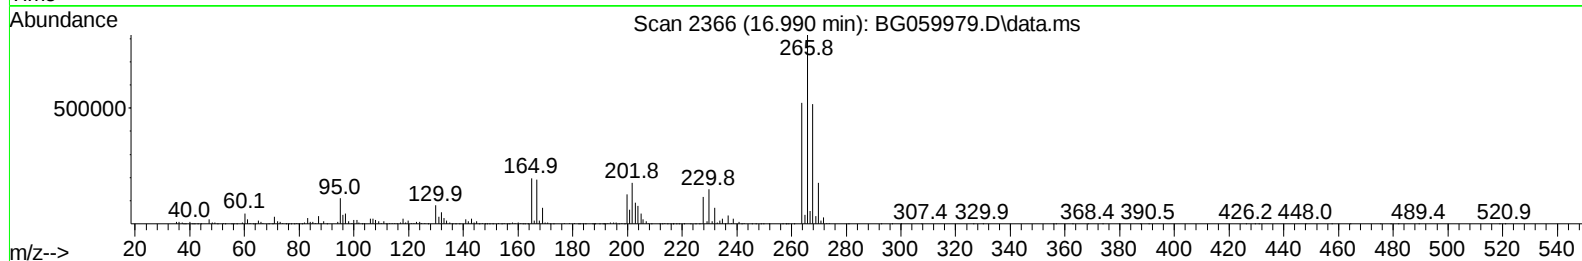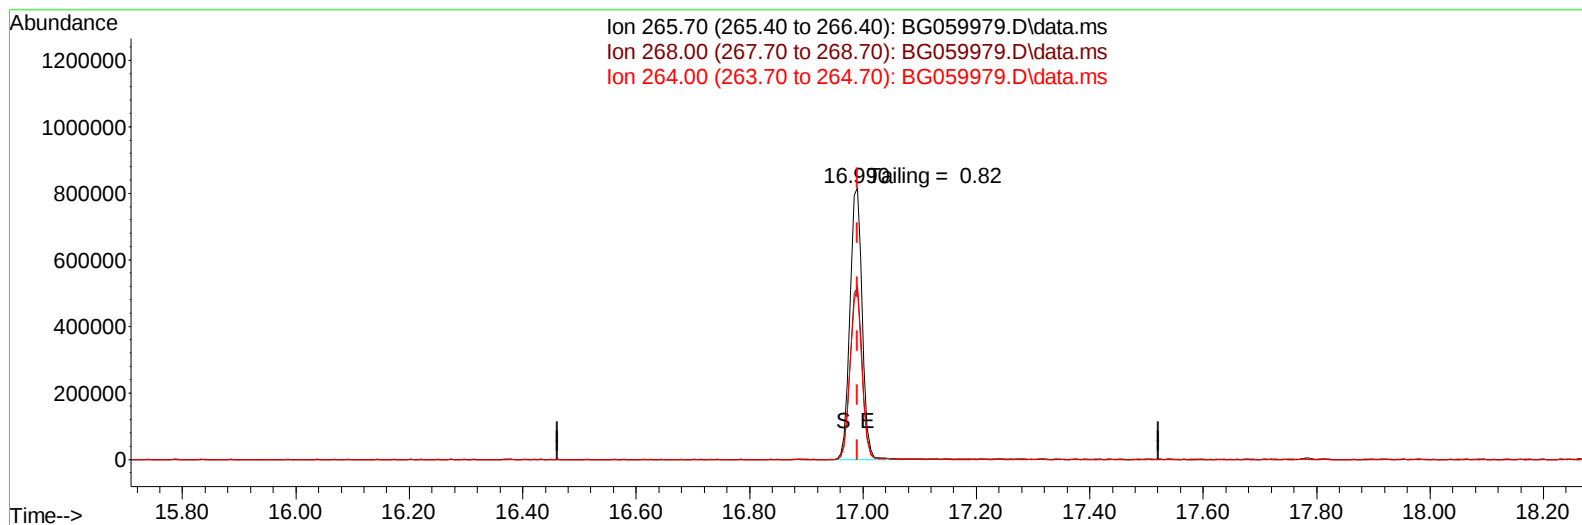

TIC: BG059979.D\data.ms

(70) Pentachlorophenol (C)

16.990min (-0.001) 902313.41 ng




response 1221749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	63.29
264.00	61.40	63.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120723\
Data File : BG059979.D
Acq On : 7 Dec 2023 9:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 07 18:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 07 17:14:16 2023
Response via : Initial Calibration

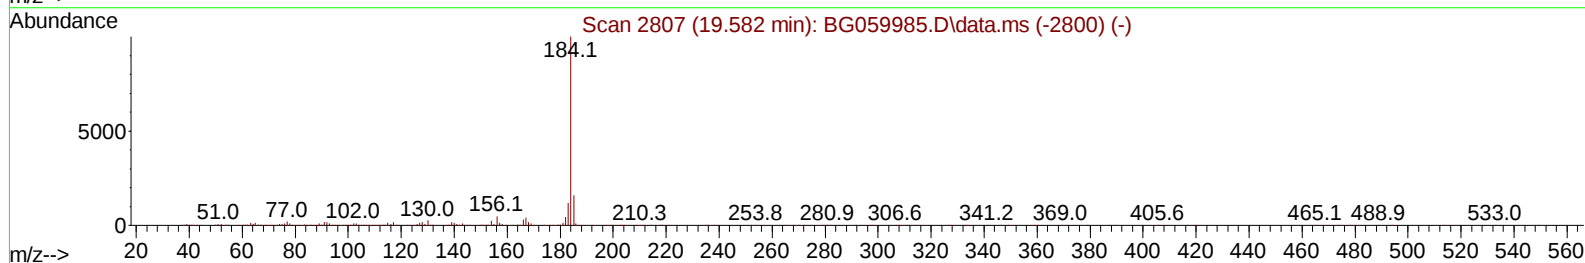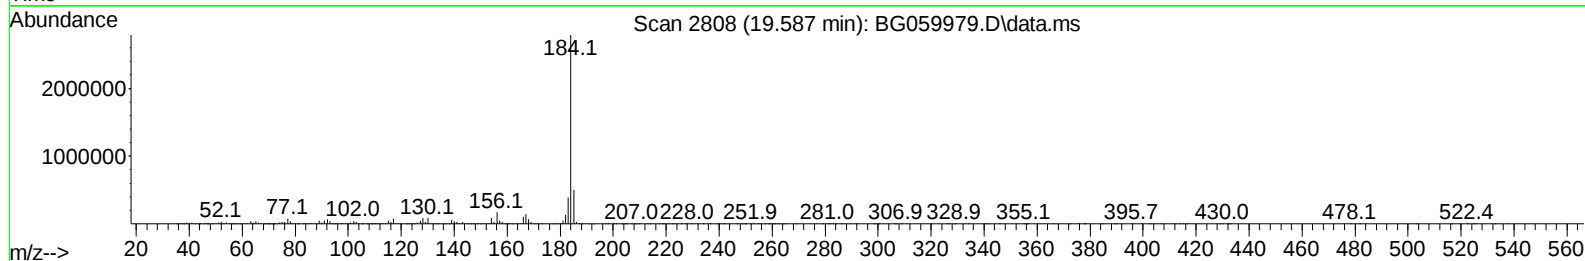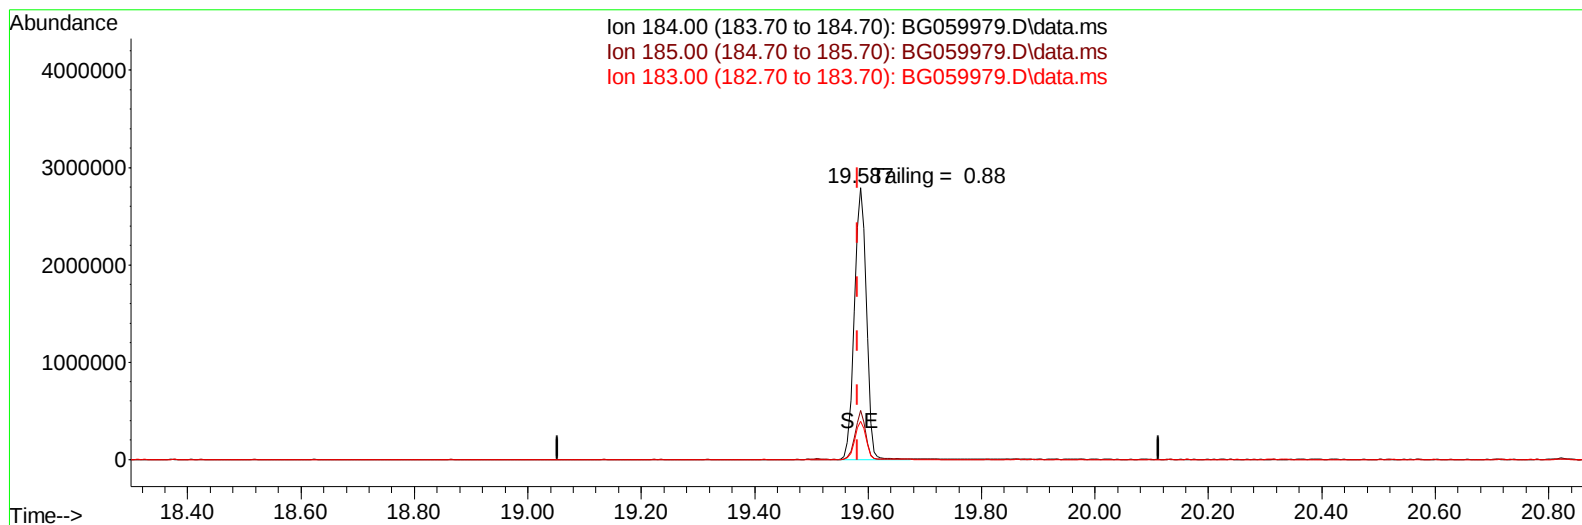

TIC: BG059979.D\data.ms

(77) Benzidine

19.587min (+ 0.005) 970544.01 ng

response 4122027

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.90	17.98
183.00	12.00	13.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2023	BNA_G	<u>BG059979.D</u>
Compound Name	Response	Retention Time
DDT	2546856	20.821
DDD	44484	20.433
DDE	1343	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45827	2592683	1.77

Instrument :
BNA_G
ClientSampleId :
DFTPP