

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG120817\
 Data File : BG031430.D
 Acq On : 8 Dec 2017 19:13
 Operator : SJ/JU
 Sample : PB104848BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 08 23:57:30 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 06 17:58:37 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	34535	20.00	ng	0.00
21) Naphthalene-d8	10.94	136	154477	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	114805	20.00	ng	0.00
63) Phenanthrene-d10	17.49	188	360800	20.00	ng	0.00
75) Chrysene-d12	21.77	240	432199	20.00	ng	0.00
86) Perylene-d12	25.06	264	406387	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	297961	147.95	ng	0.00
7) Phenol-d6	7.29	99	391425	144.26	ng	0.00
23) Nitrobenzene-d5	9.29	82	234587	89.99	ng	0.00
41) 2,4,6-Tribromophenol	16.24	330	195206	105.11	ng	0.00
44) 2-Fluorobiphenyl	13.37	172	716029	89.62	ng	0.00
78) Terphenyl-d14	20.08	244	1740352	88.91	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG120817\
Data File : BG031430.D
Acq On : 8 Dec 2017 19:13
Operator : SJ/JU
Sample : PB104848BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 08 23:57:30 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 06 17:58:37 2017
Response via : Initial Calibration

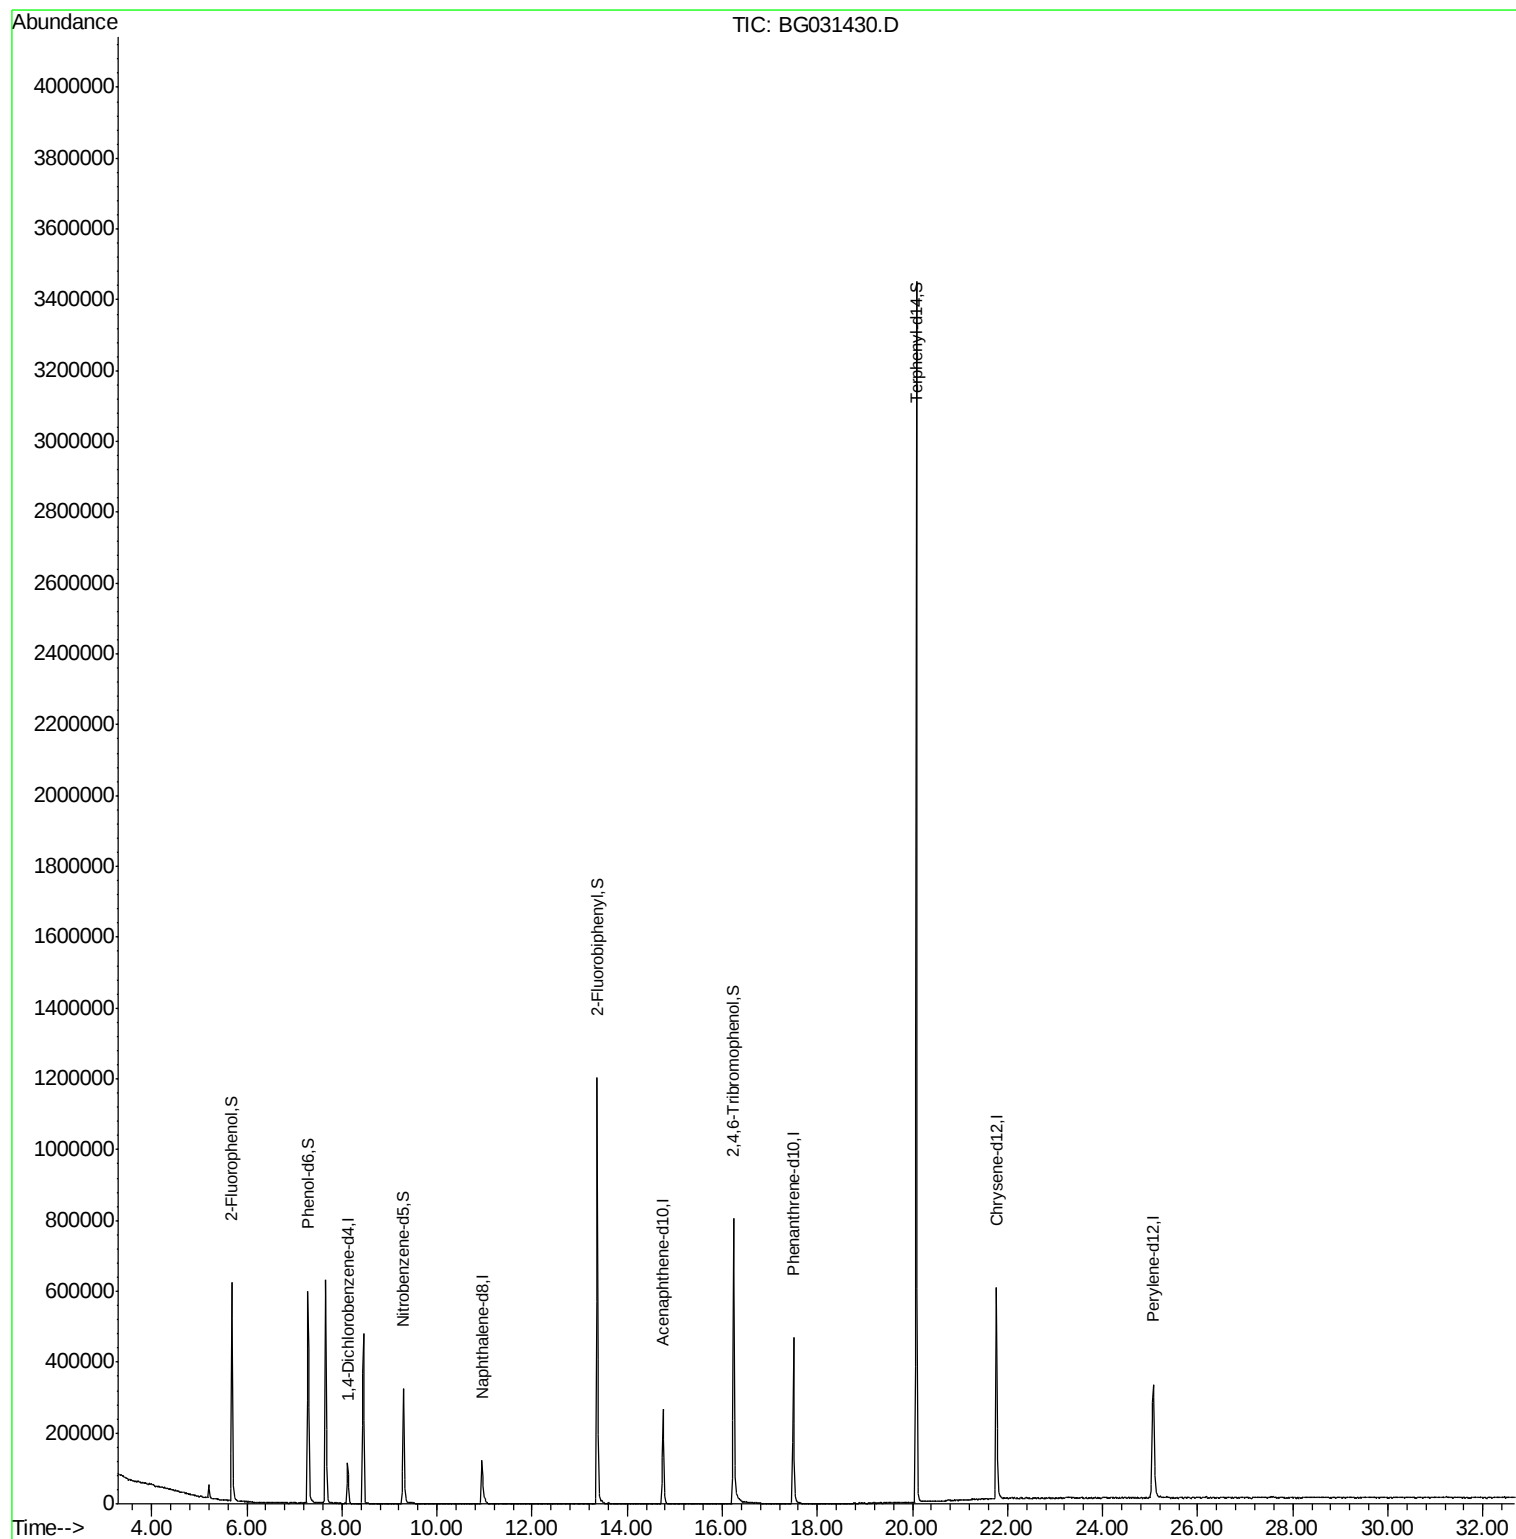

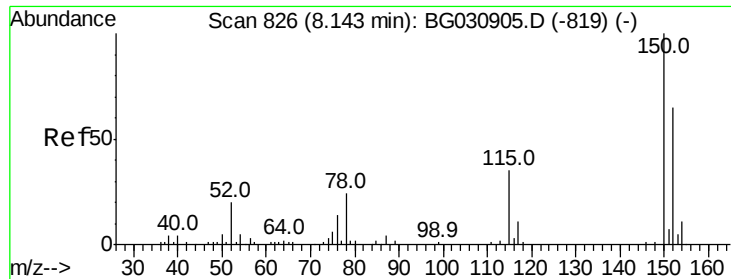


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.13 min Scan# 824
Delta R.T. 0.00 min
Lab File: BG031430.D
Acq: 8 Dec 2017 19:13

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 34535
Ion Ratio Lower Upper
152 100
150 166.2 126.6 189.8
115 51.2 53.0 79.4#

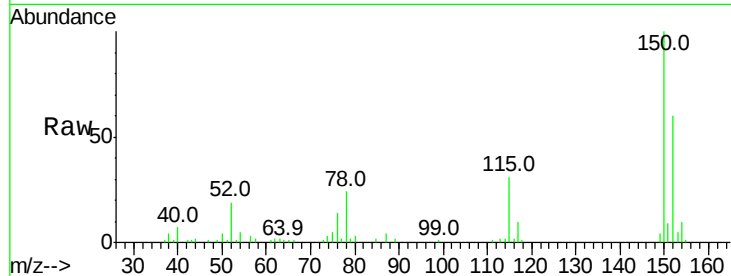


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

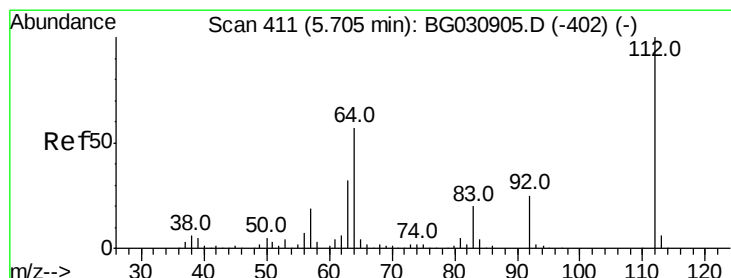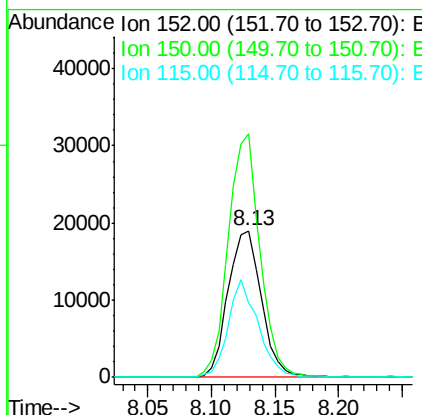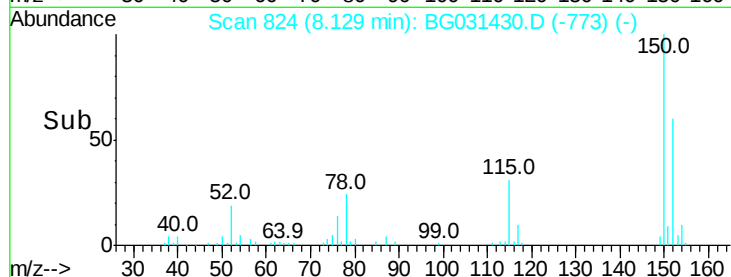



#5


2-Fluorophenol
Concen: 147.946 ng
RT: 5.68 min Scan# 408
Delta R.T. 0.00 min
Lab File: BG031430.D
Acq: 8 Dec 2017 19:13

Tgt Ion:112 Resp: 297961
Ion Ratio Lower Upper
112 100
64 58.1 56.3 84.5
63 31.9 30.1 45.1

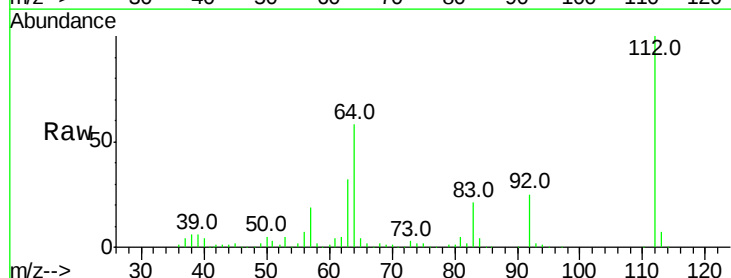

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

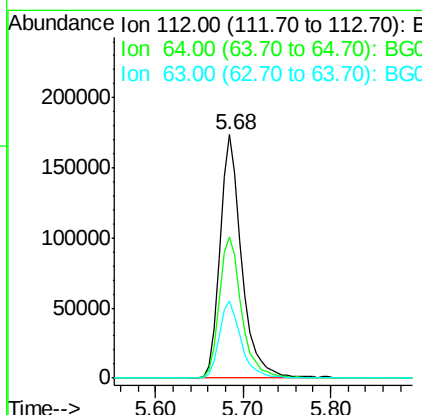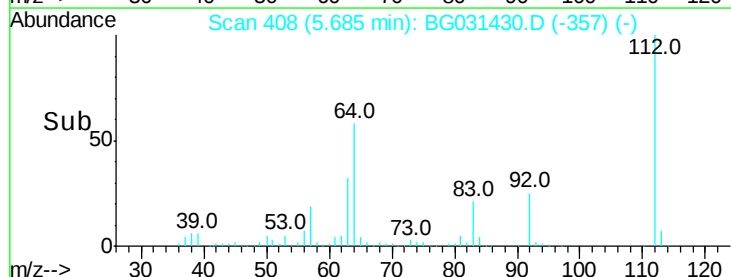

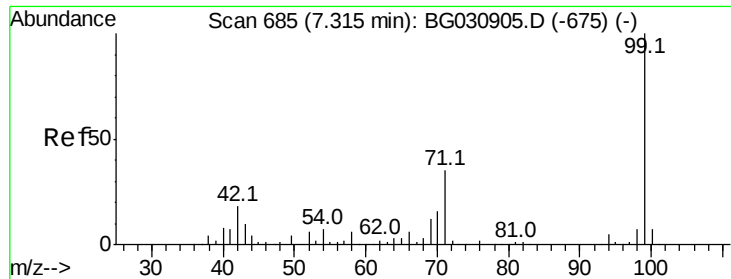

#7

Phenol-d6

Concen: 144.263 ng

RT: 7.29 min Scan# 681

Delta R.T. -0.01 min

Lab File: BG031430.D

Acq: 8 Dec 2017 19:13

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 391425

Ion Ratio Lower Upper




99 100

42 19.8 14.1 21.1

71 36.8 26.1 39.1

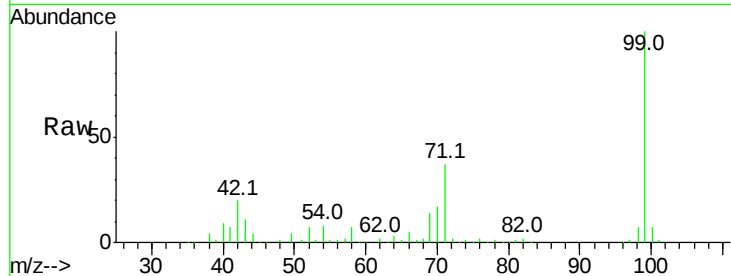

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

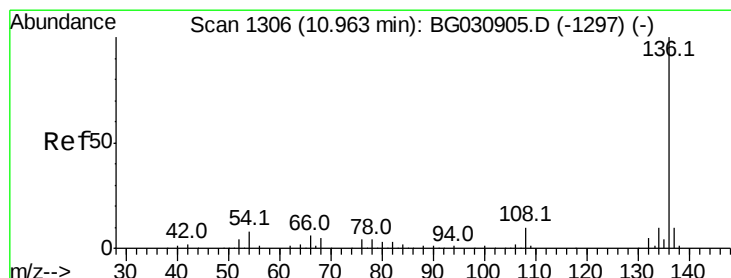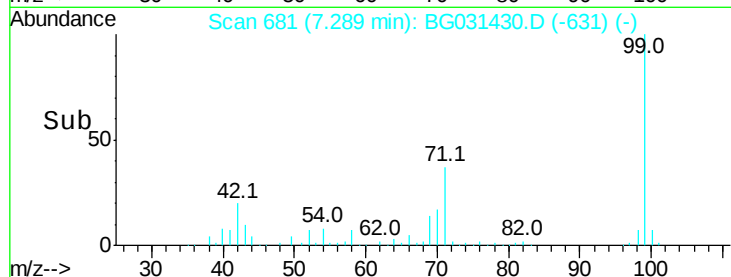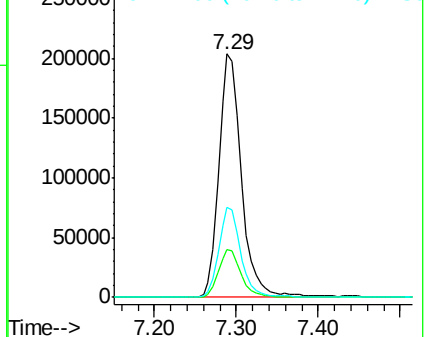

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.94 min Scan# 1303

Delta R.T. 0.00 min

Lab File: BG031430.D

Acq: 8 Dec 2017 19:13

Tgt Ion: 136 Resp: 154477


Ion Ratio Lower Upper

136 100



137 11.6 9.2 13.8


54 7.6 10.3 15.5#

68 5.0 4.5 6.7

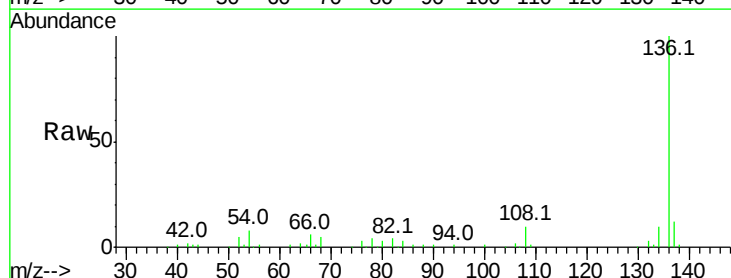

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

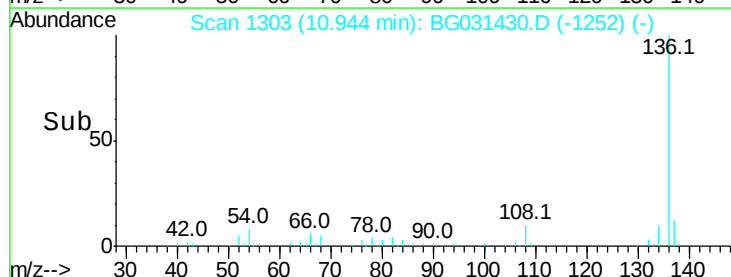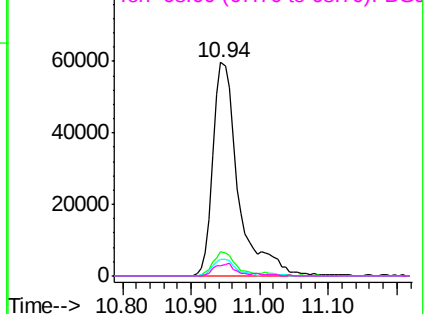


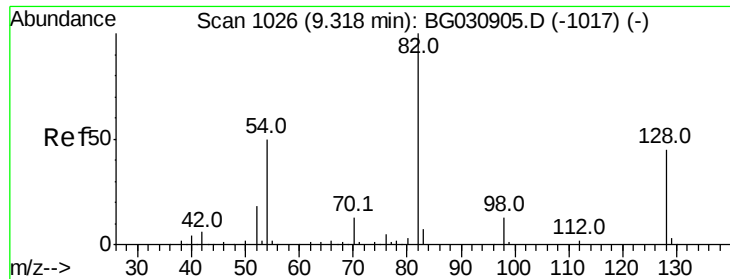




#23
 Nitrobenzene-d5
 Concen: 89.986 ng
 RT: 9.29 min Scan# 1022
 Delta R.T. -0.01 min
 Lab File: BG031430.D
 Acq: 8 Dec 2017 19:13

Instrument :
 BNA_G
 ClientSampled :

Tot Ion	82	Resp	234587
Ion Ratio	100	Lower	Upper
128	44.0	29.7	44.5
54	50.5	43.1	64.7

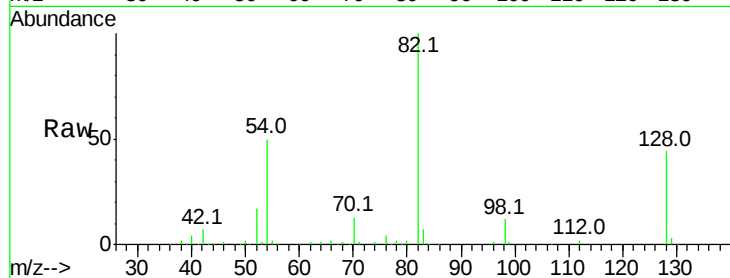


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

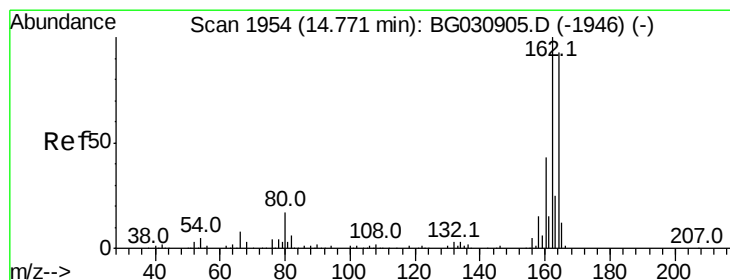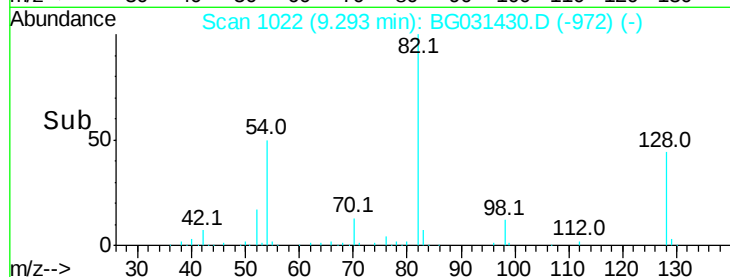
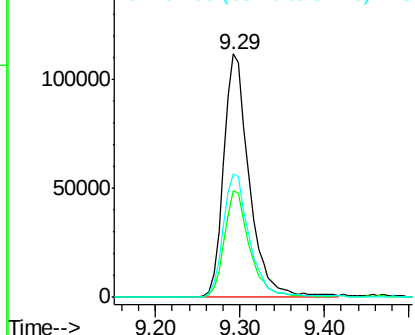



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.75 min Scan# 1951
 Delta R.T. 0.00 min
 Lab File: BG031430.D
 Acq: 8 Dec 2017 19:13

Tgt Ion	164	Resp	114805
Ion Ratio	100	Lower	Upper
162	103.9	78.8	118.2
160	46.4	35.4	53.0

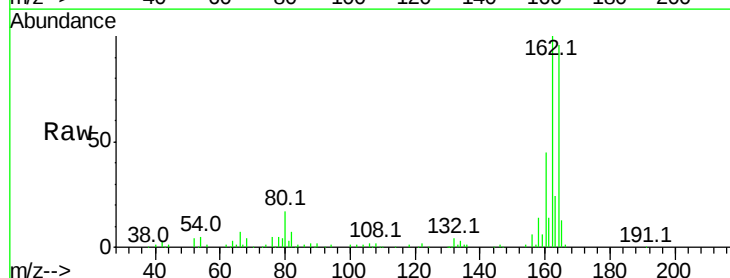

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

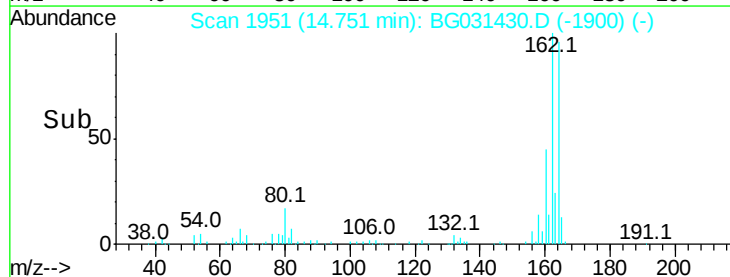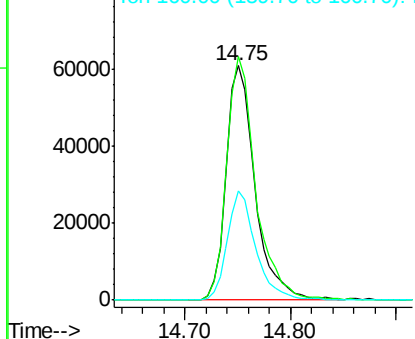


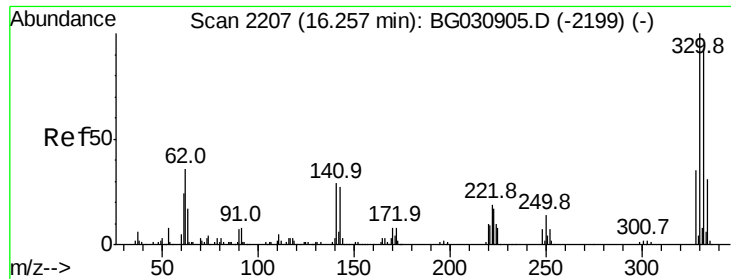




#41
 2,4,6-Tribromophenol
 Concen: 105.109 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. 0.00 min
 Lab File: BG031430.D
 Acq: 8 Dec 2017 19:13

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	93.7	77.0	115.6
141	38.2	25.2	37.8#

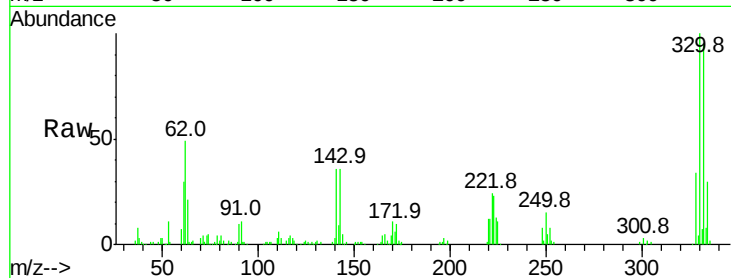


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

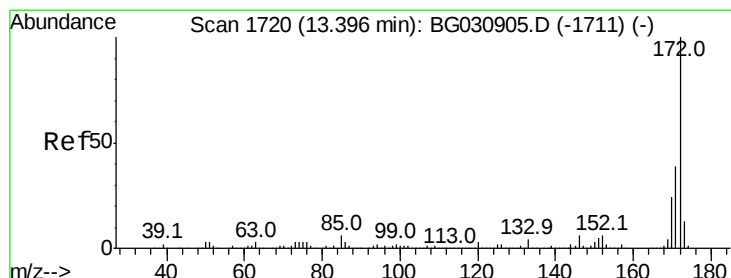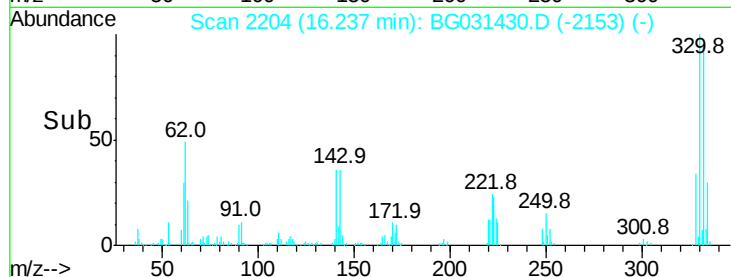
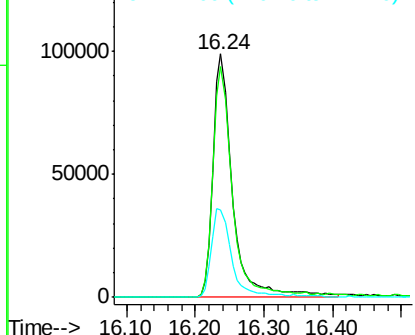



#44
 2-Fluorobiphenyl
 Concen: 89.618 ng
 RT: 13.37 min Scan# 1716
 Delta R.T. 0.00 min
 Lab File: BG031430.D
 Acq: 8 Dec 2017 19:13

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	30.0	45.0
170	23.9	19.5	29.3

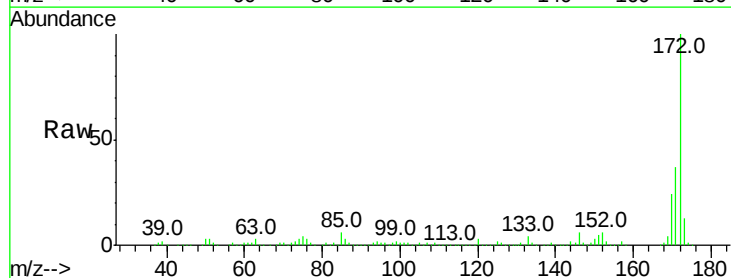

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



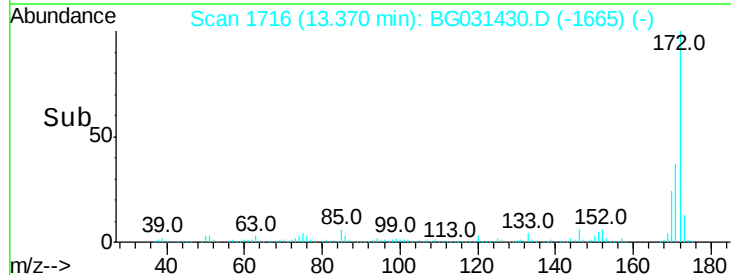
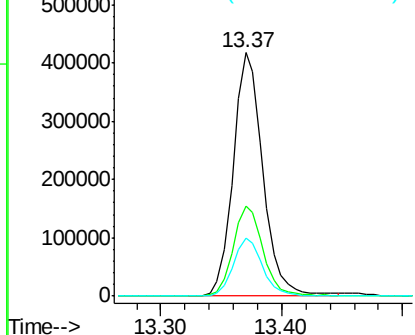


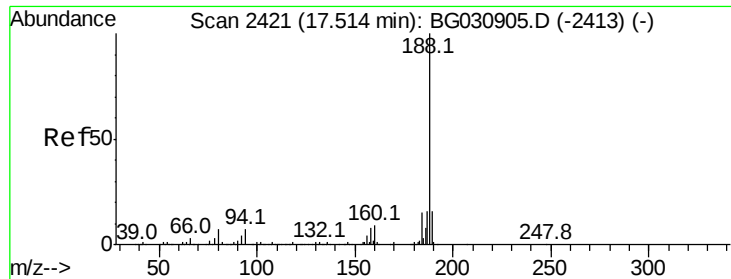

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.49 min Scan# 2417
Delta R.T. -0.01 min
Lab File: BG031430.D
Acq: 8 Dec 2017 19:13




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
188	100		
94	7.3	6.9	10.3
80	7.3	7.7	11.5#

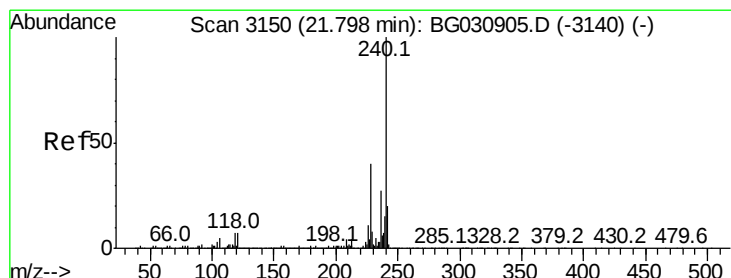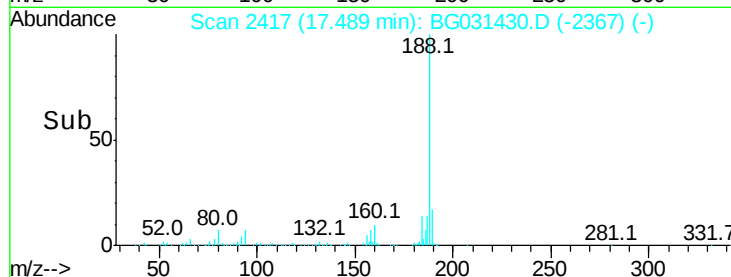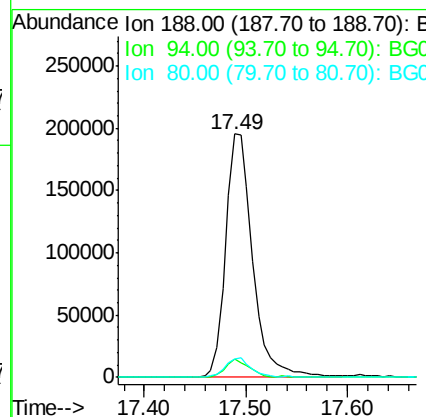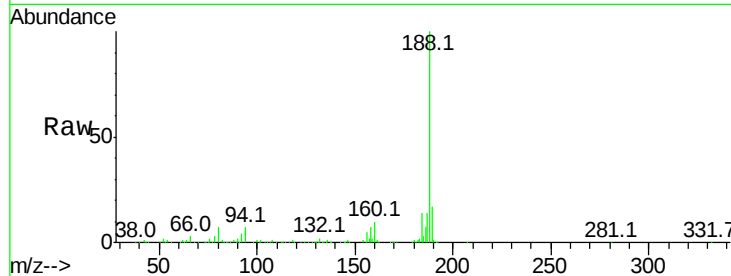

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.77 min Scan# 3145
Delta R.T. -0.01 min
Lab File: BG031430.D
Acq: 8 Dec 2017 19:13

Tgt Ion	Ratio	Lower	Upper
240	100		
120	7.4	6.8	10.2
236	25.5	20.9	31.3

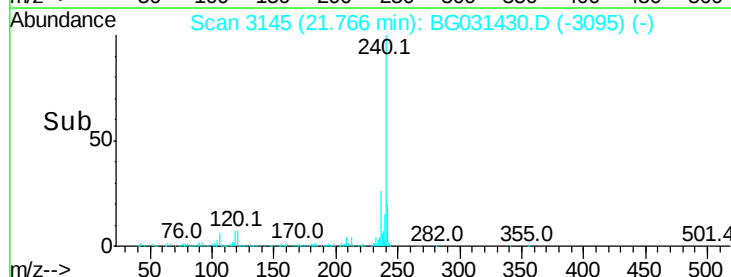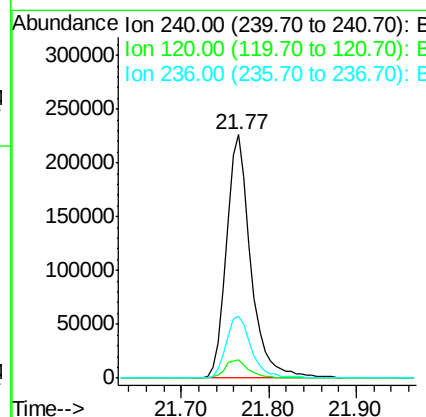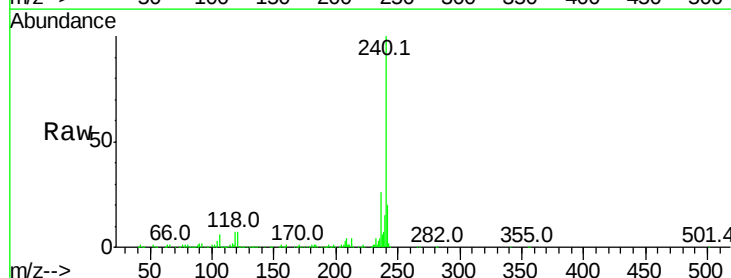

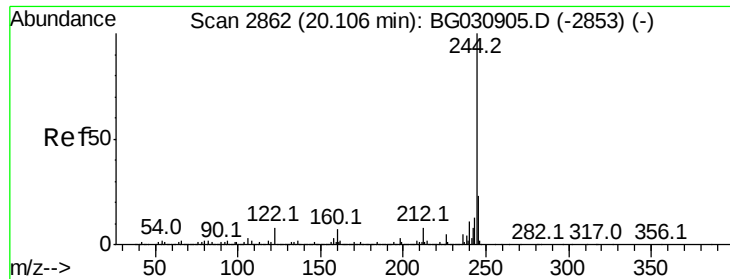

#78

Terphenyl-d14

Concen: 88.914 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG031430.D

Acq: 8 Dec 2017 19:13

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 1740352

Ion Ratio Lower Upper




244 100

212 8.6 5.8 8.8

122 8.5 7.0 10.4

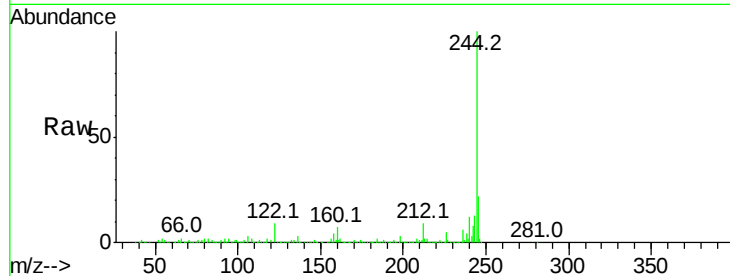

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

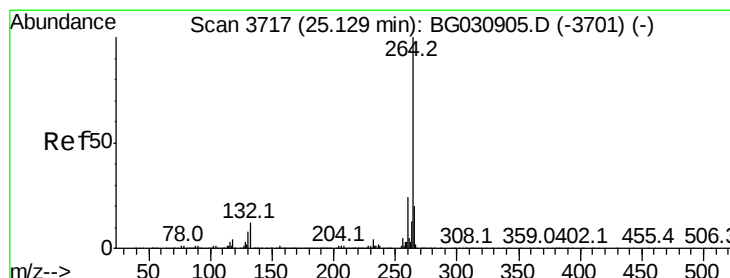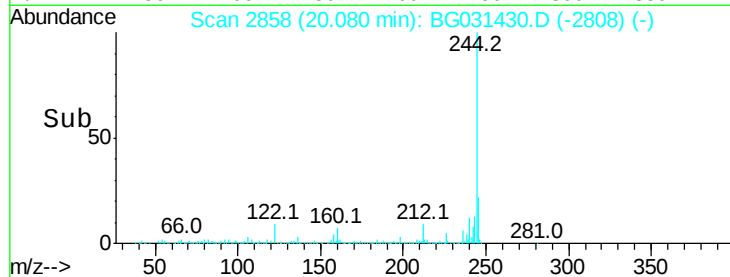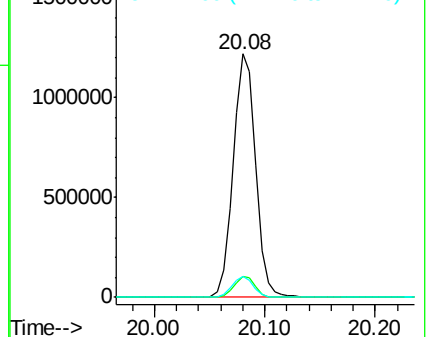

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.06 min Scan# 3706

Delta R.T. -0.01 min

Lab File: BG031430.D

Acq: 8 Dec 2017 19:13


Tgt Ion:264 Resp: 406387

Ion Ratio Lower Upper

264 100

260 24.2 17.4 26.0

265 22.0 17.7 26.5

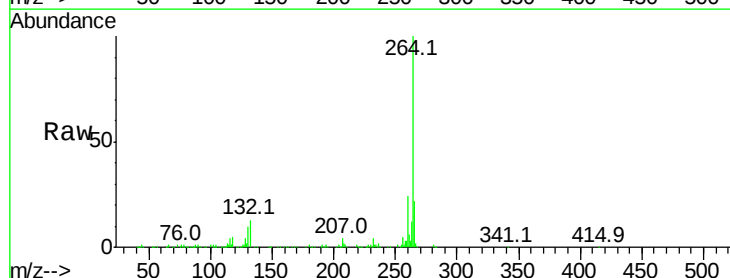

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

