


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG120817\
 Data File : BG031414.D
 Acq On : 8 Dec 2017 8:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 06 17:58:37 2017

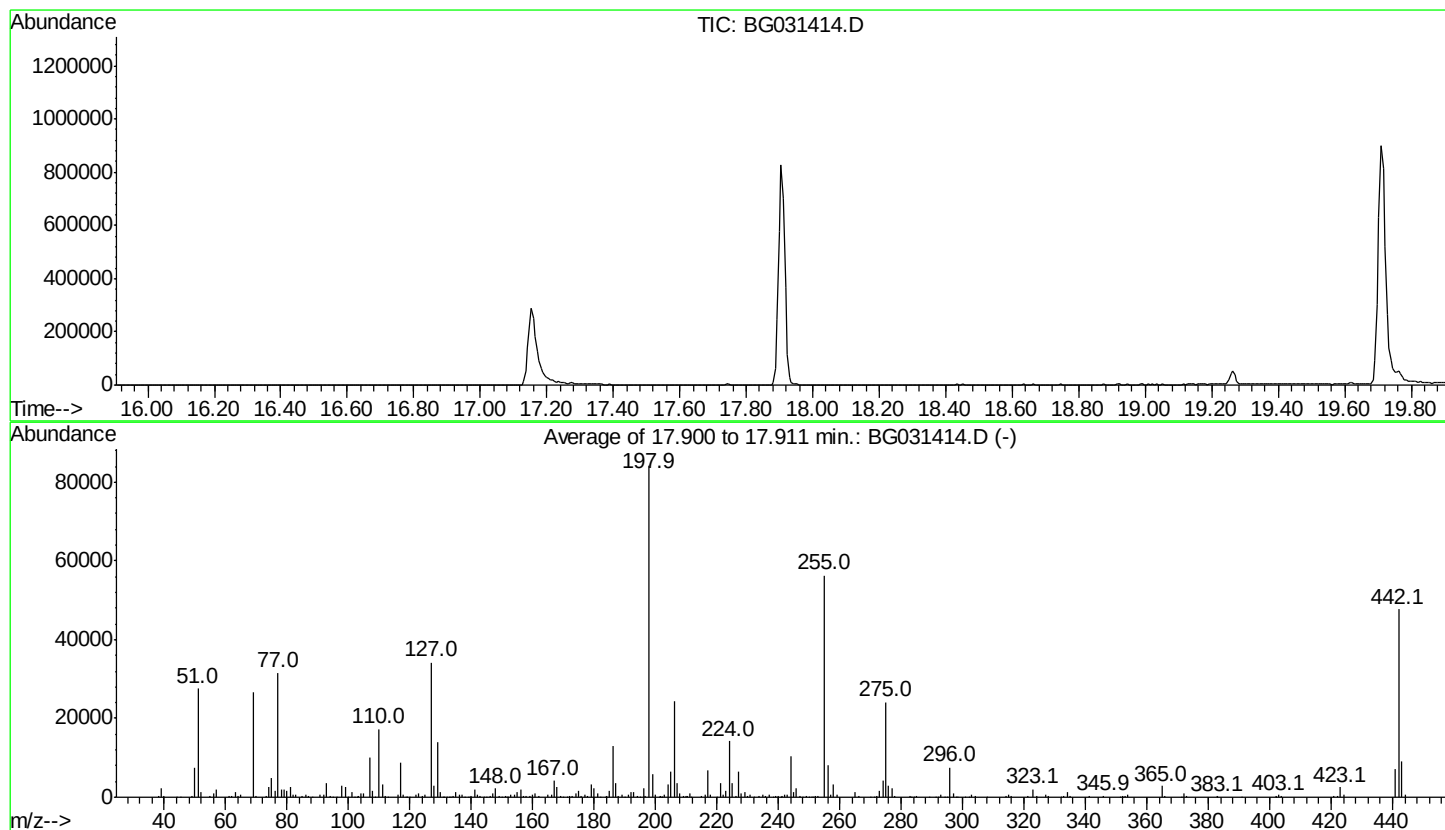

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	27602	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.8	26802	PASS
70	69	0.00	2	0.8	205	PASS
127	198	10	80	40.6	34157	PASS
197	198	0.00	2	0.3	261	PASS
198	198	100	100	100.0	84181	PASS
199	198	5	9	6.9	5801	PASS
275	198	10	60	28.7	24122	PASS
365	198	1	100	3.3	2800	PASS
441	442	0.01	24	15.1	7223	PASS
442	198	50	100	56.7	47706	PASS
443	442	15	24	19.2	9151	PASS