


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG120817\
 Data File : BG031432.D
 Acq On : 8 Dec 2017 21:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 06 17:58:37 2017

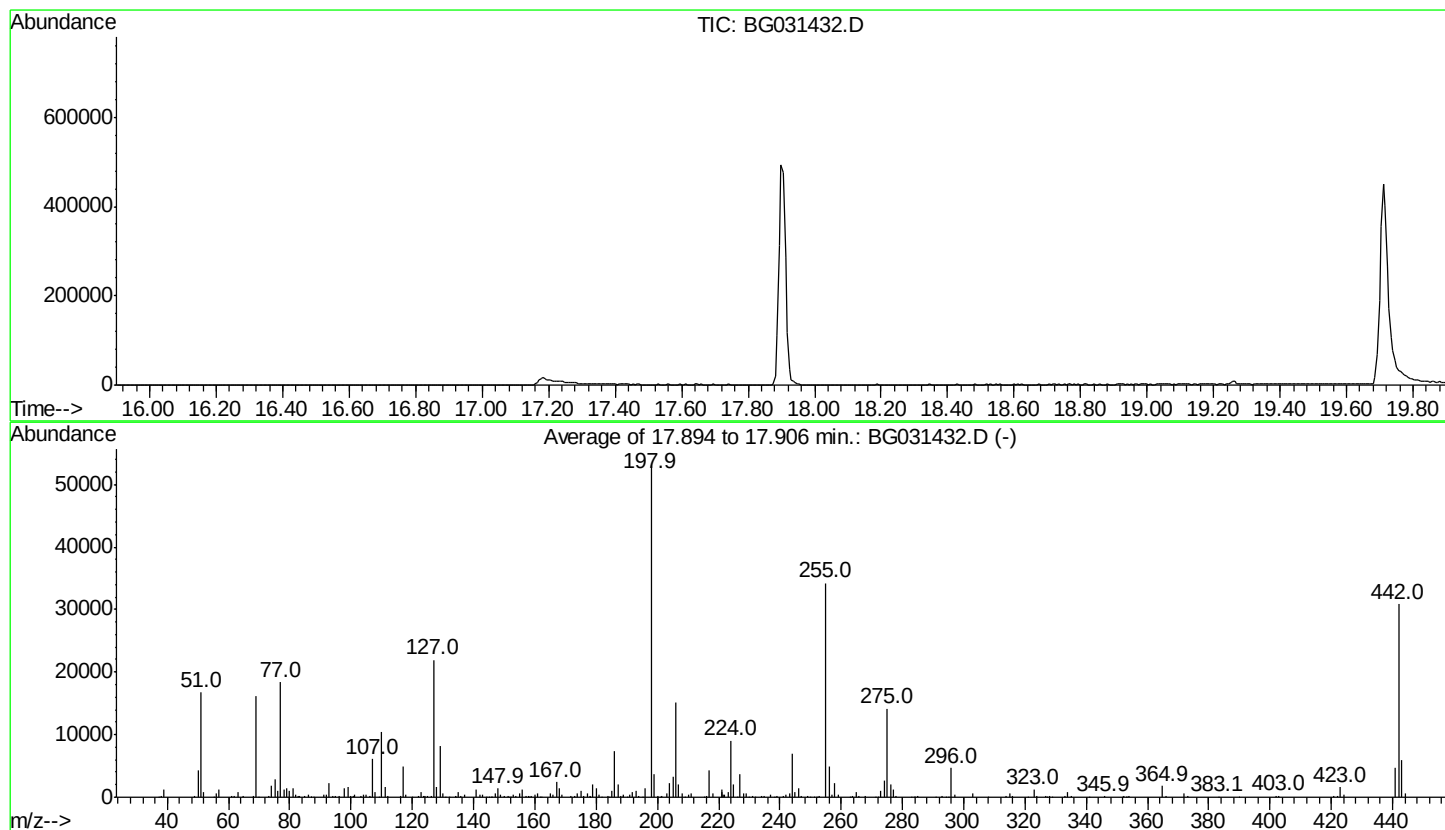

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	16770	PASS
68	69	0.00	2	1.6	262	PASS
69	198	0.00	100	30.7	16260	PASS
70	69	0.00	2	0.5	80	PASS
127	198	10	80	41.5	21981	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52997	PASS
199	198	5	9	7.0	3685	PASS
275	198	10	60	26.7	14124	PASS
365	198	1	100	3.3	1747	PASS
441	442	0.01	24	15.2	4691	PASS
442	198	50	100	58.2	30845	PASS
443	442	15	24	19.4	5972	PASS