

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047683.D
 Acq On : 9 Dec 2020 21:21
 Operator : CG/JU
 Sample : L4941-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 10 00:45:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 08 17:39:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.22	152	38188	20.00	ng/ul	0.00
18) Naphthalene-d8	11.04	136	139632	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.84	164	108228	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.58	188	269669	20.00	ng/ul	0.00
78) Chrysene-d12	21.85	240	264600	20.00	ng/ul	0.00
86) Perylene-d12	25.21	264	277766	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	1414	1.97	ng/uL	0.00
5) Phenol-d5	7.35	99	37920	11.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.53	67	20276	12.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.74	132	29362	11.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.91	113	28167	10.86	ng/ul	0.00
19) Nitrobenzene-d5	9.38	128	14218	12.49	ng/ul	0.00
22) 2-Nitrophenol-d4	10.11	143	16351	11.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	35510	11.92	ng/ul	0.00
29) 4-Chloroaniline-d4	11.17	131	34838	12.73	ng/ul	0.00
44) Dimethylphthalate-d6	14.23	166	112873	12.01	ng/ul	0.00
47) Acenaphthylene-d8	14.53	160	138085	12.86	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	14677	10.53	ng/ul	0.00
58) Fluorene-d10	15.82	176	103419	11.95	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.93	200	17050	9.34	ng/ul	0.00
71) Anthracene-d10	17.67	188	175487	13.05	ng/ul	0.00
79) Pyrene-d10	19.94	212	216484	13.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.98	264	213884	13.18	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	7.38	94	7494	2.427	ng/ul 92
45) Dimethylphthalate	14.27	163	19067	2.002	ng/ul# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
Data File : BG047683.D
Acq On : 9 Dec 2020 21:21
Operator : CG/JU
Sample : L4941-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 10 00:45:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 08 17:39:41 2020
Response via : Initial Calibration

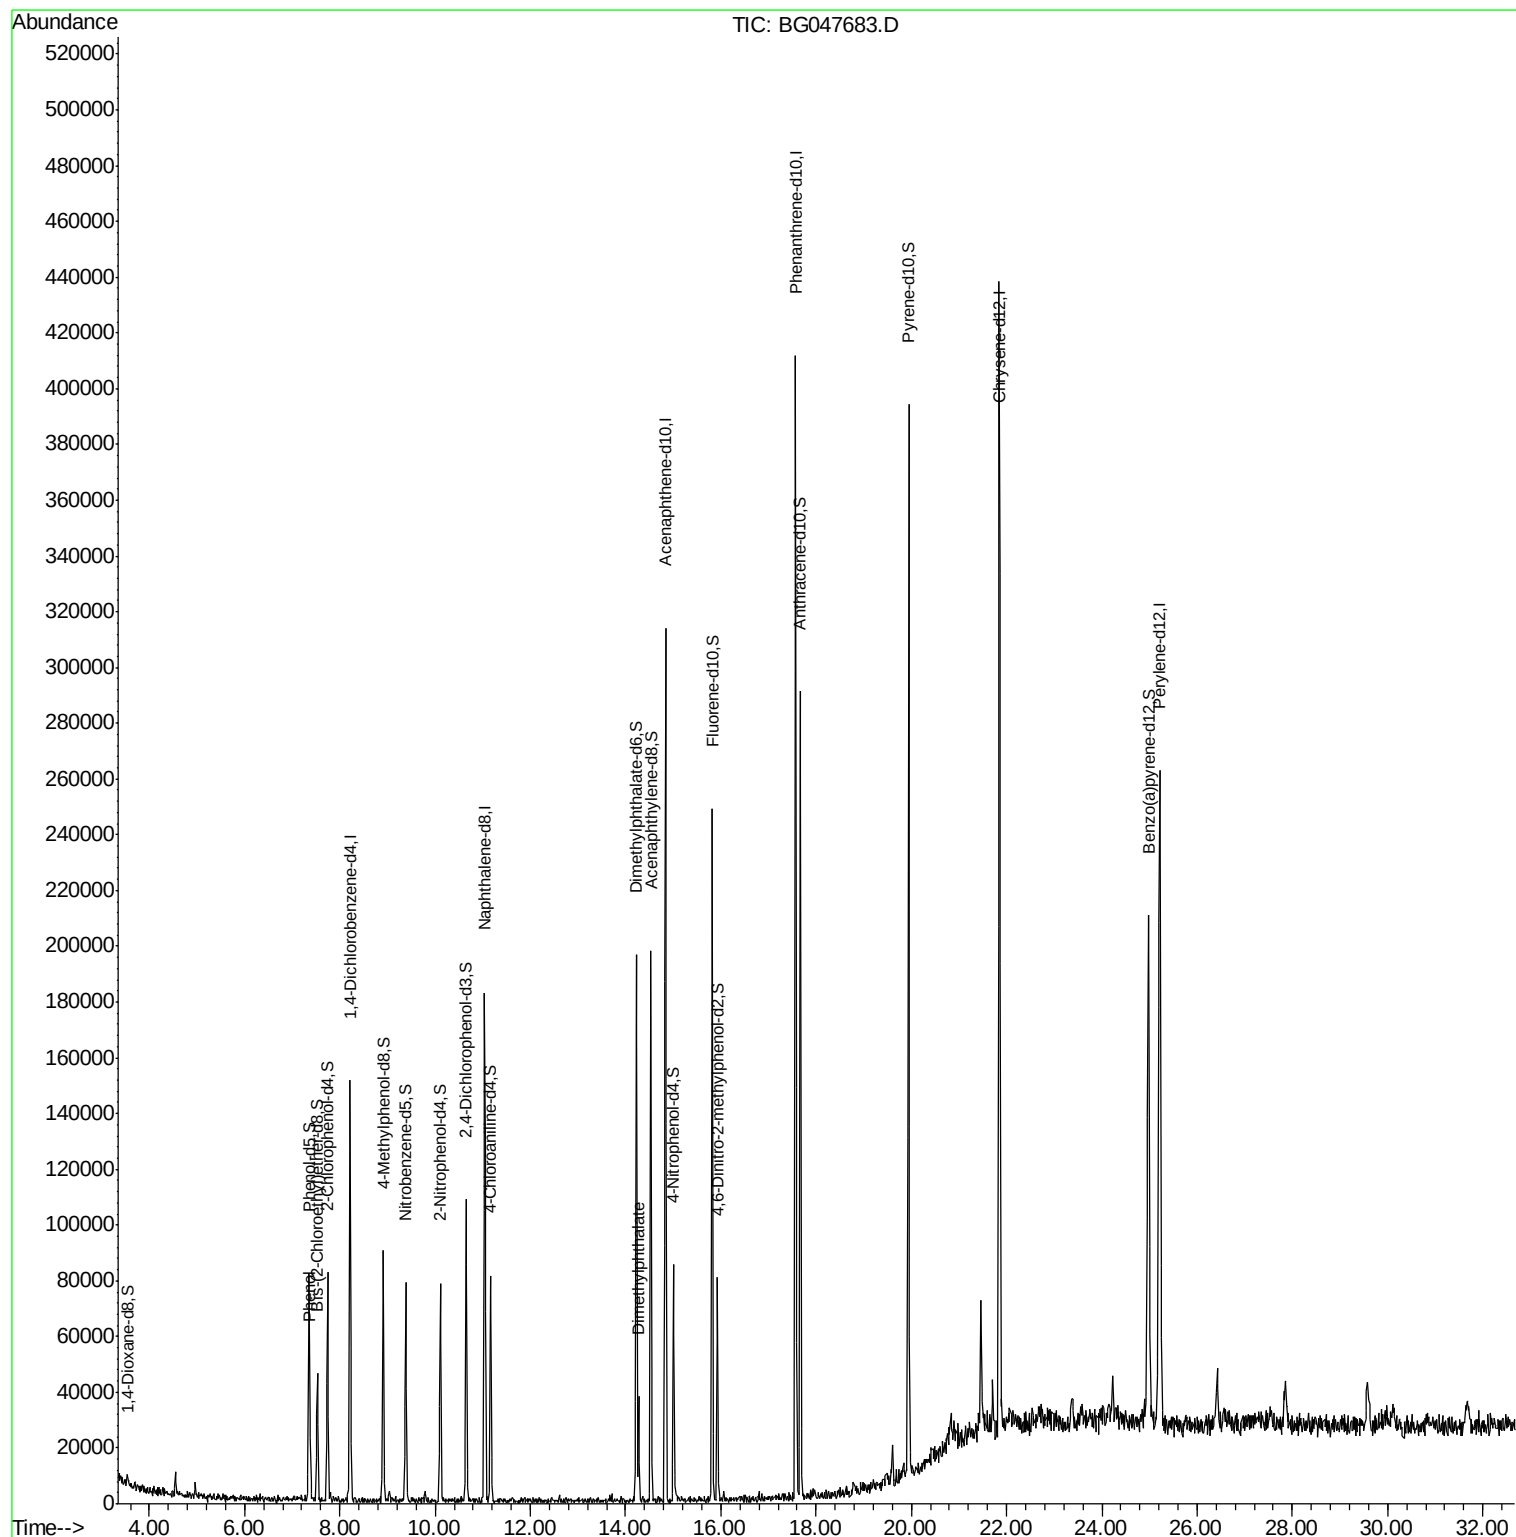

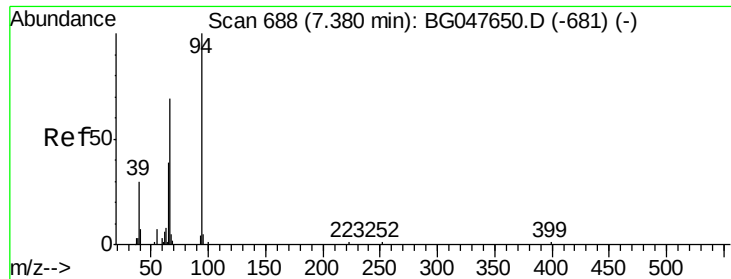

#6

Phenol

Concen: 2.427 ng/ul

RT: 7.38 min Scan# 687

Delta R.T. -0.00 min

Lab File: BG047683.D

Acq: 9 Dec 2020 21:21

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 94 Resp: 7494

Ion Ratio Lower Upper




94 100

65 36.4 35.9 53.9

66 66.3 50.1 75.1

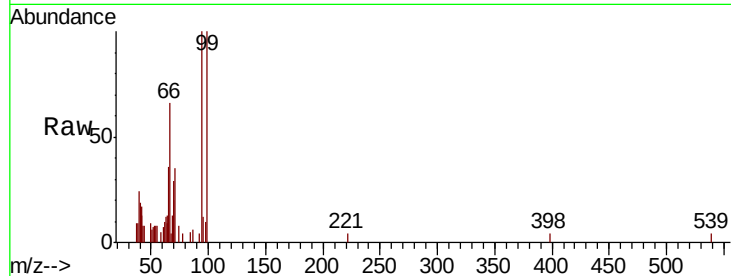

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

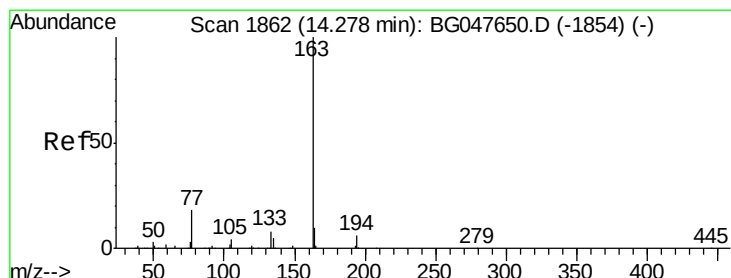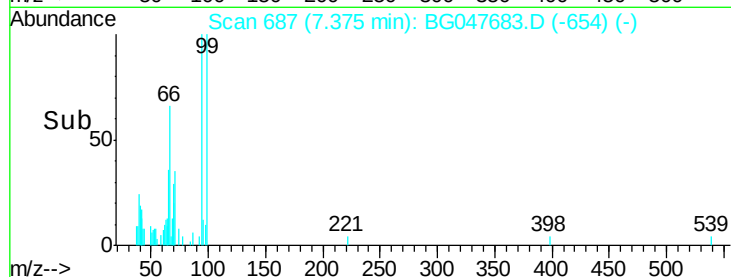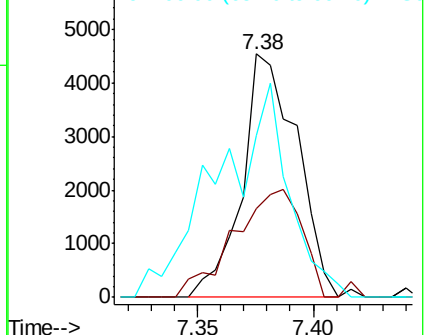

#45

Dimethylphthalate

Concen: 2.002 ng/ul

RT: 14.27 min Scan# 1861

Delta R.T. -0.00 min

Lab File: BG047683.D

Acq: 9 Dec 2020 21:21


Tgt Ion: 163 Resp: 19067

Ion Ratio Lower Upper

163 100

194 7.0 3.9 5.9#

164 12.7 7.4 11.2#

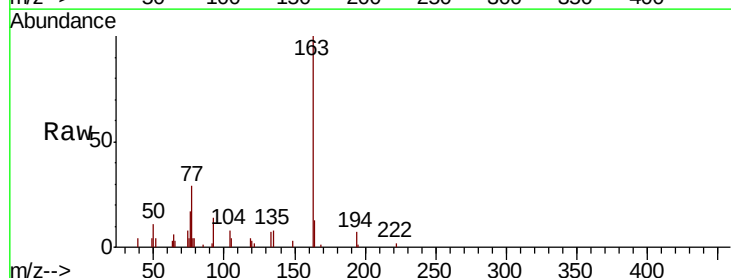

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

