

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047669.D
 Acq On : 9 Dec 2020 11:01
 Operator : CG/JU
 Sample : L4921-05DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0FW4DL

Manual Integrations
 APPROVED

mohammad
 12/9/2020 5:40:05 PM

Quant Time: Dec 09 12:20:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 08 17:39:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.22	152	27041	20.00	ng/ul	0.00
18) Naphthalene-d8	11.04	136	98958	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.83	164	81756	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.57	188	220410	20.00	ng/ul	0.00
78) Chrysene-d12	21.85	240	242535	20.00	ng/ul	0.00
86) Perylene-d12	25.21	264	244222	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.35	99	1622	0.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.53	67	4244	3.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.73	132	4576	2.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.90	113	2367	1.29	ng/ul	0.00
19) Nitrobenzene-d5	9.39	128	2653	3.29	ng/ul	0.00
22) 2-Nitrophenol-d4	10.10	143	3614	3.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	6345	3.00	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	14.23	166	20043	2.82	ng/ul	0.00
47) Acenaphthylene-d8	14.53	160	30769	3.79	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	538	0.51	ng/ul	0.00
58) Fluorene-d10	15.82	176	20622	3.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	17.67	188	42284m	3.85	ng/ul	0.00
79) Pyrene-d10	19.94	212	51064	3.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.98	264	53837	3.77	ng/ul	0.00
Target Compounds						
20) Nitrobenzene	9.42	77	23951	9.381	ng/ul#	89
37) 1,2,4,5-Tetrachlorobenzene	13.04	216	11896	3.661	ng/ul#	81
73) 1,2,3,4-Tetrachlorobenzene	13.65	216	36011	10.427	ng/uL	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
Data File : BG047669.D
Acq On : 9 Dec 2020 11:01
Operator : CG/JU
Sample : L4921-05DL 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0FW4DL

Quant Time: Dec 09 12:20:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 08 17:39:41 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
12/9/2020 5:40:05 PM

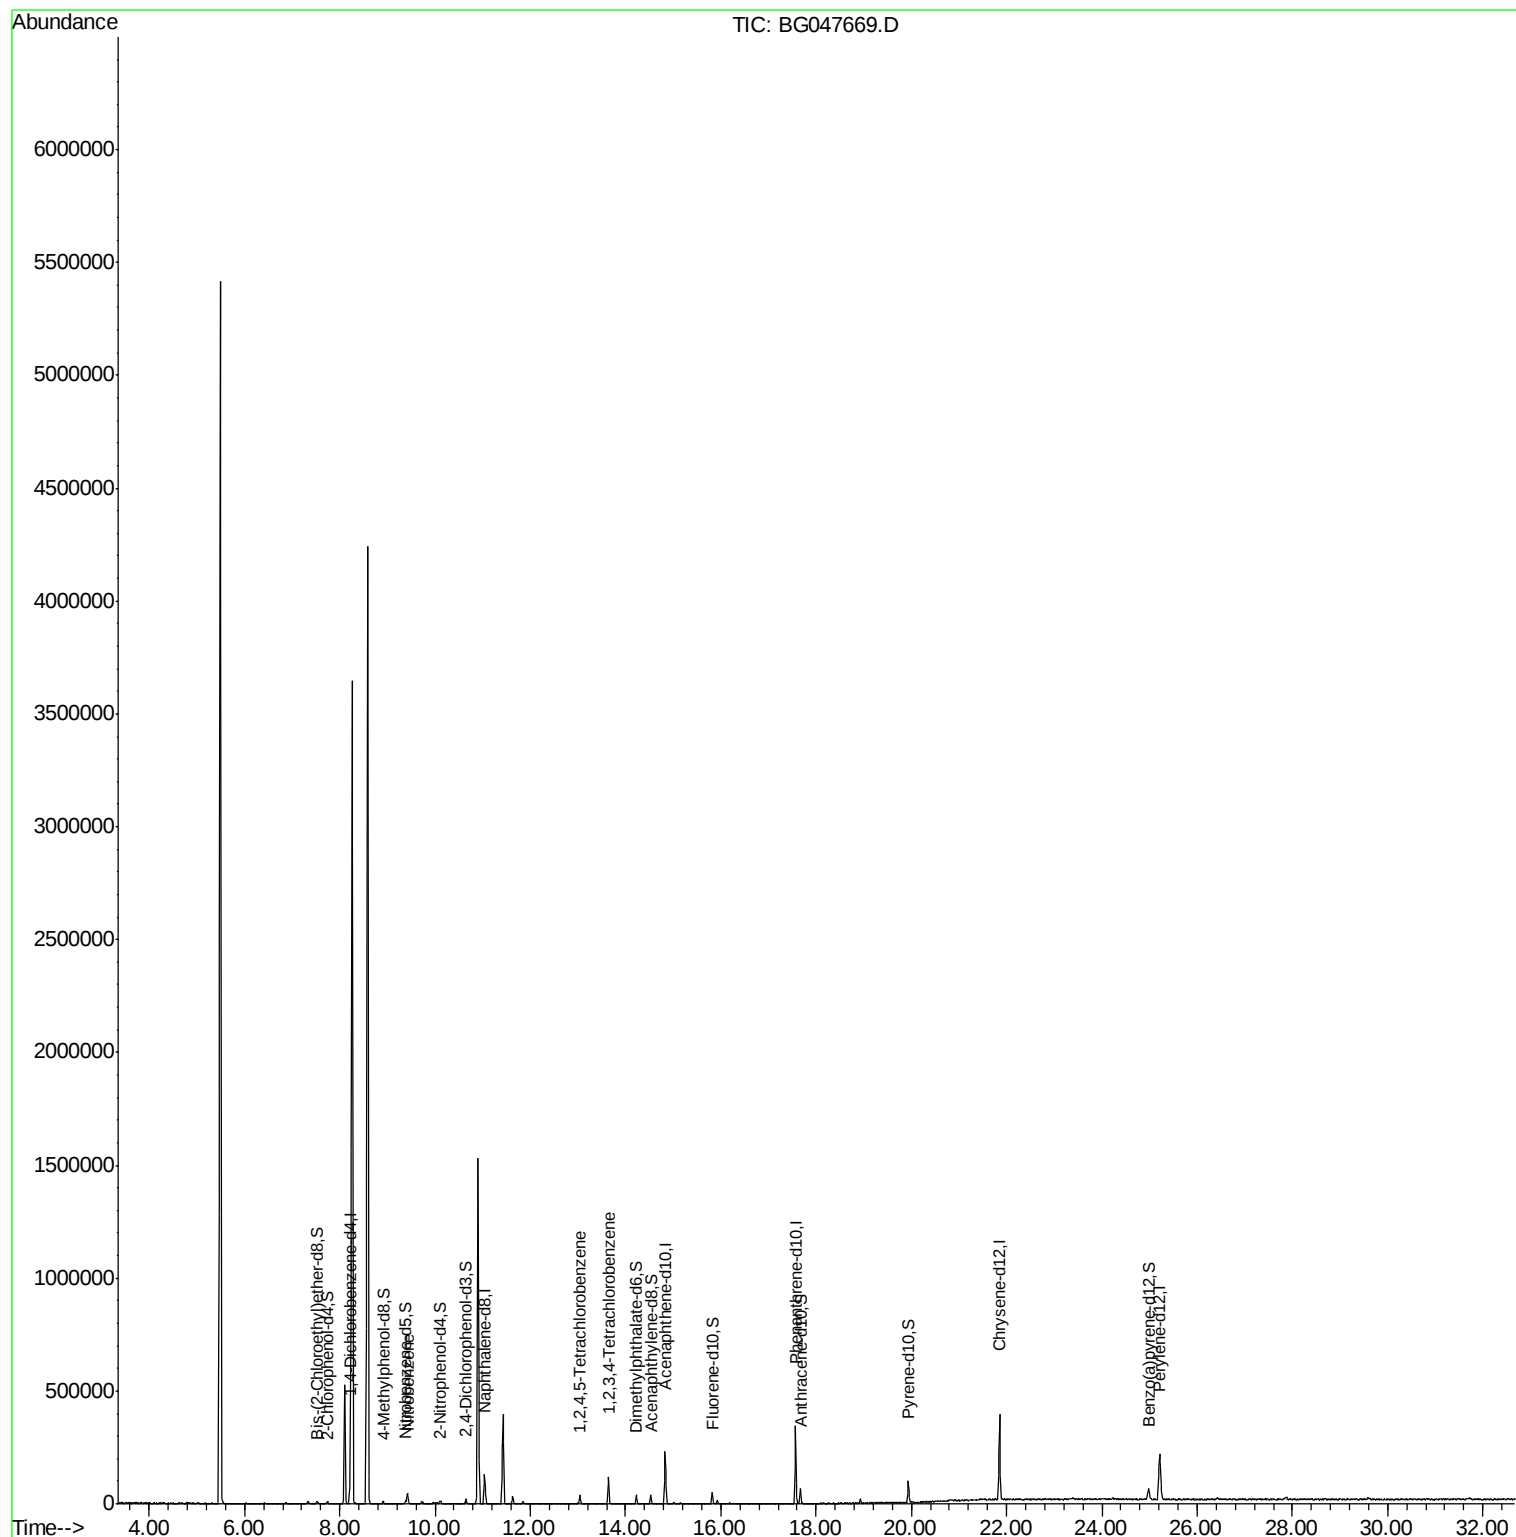

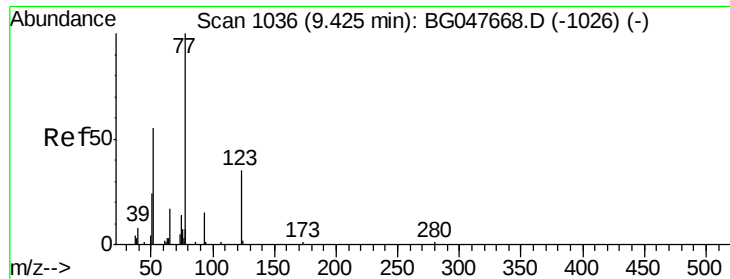





#20
Nitrobenzene
Concen: 9.381 ng/ul
RT: 9.42 min Scan# 1035
Delta R.T. -0.00 min
Lab File: BG047669.D
Acq: 9 Dec 2020 11:01

Instrument :
BNA_G
ClientSampleId :
C0FW4DL

Tot Ion	Ratio	Lower	Upper
77	100		
123	41.6	28.5	42.7
65	19.9	12.2	18.2




Manual Integrations
APPROVED


mohammad
12/9/2020 5:40:05 PM

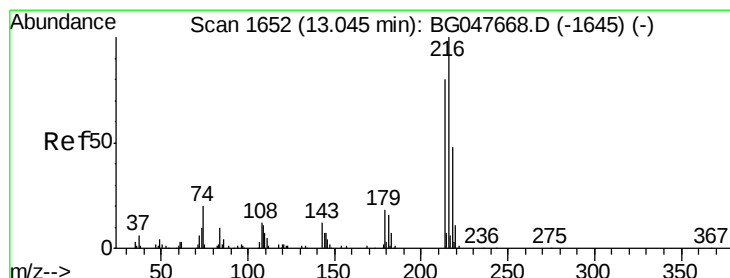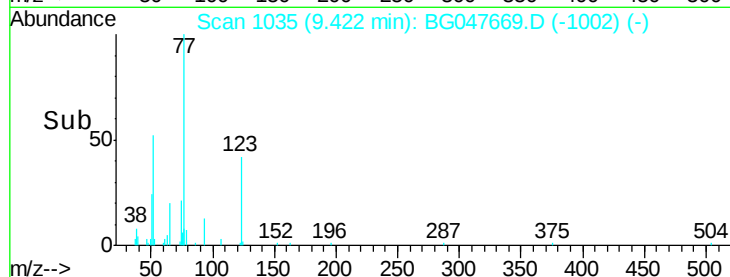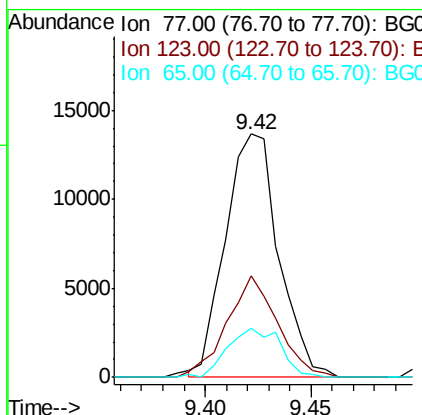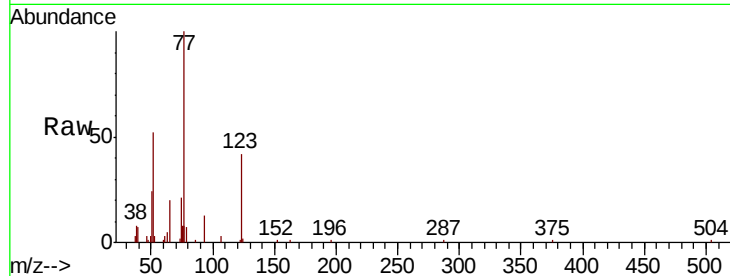

#37
1,2,4,5-Tetrachlorobenzene
Concen: 3.661 ng/ul
RT: 13.04 min Scan# 1651
Delta R.T. -0.00 min
Lab File: BG047669.D
Acq: 9 Dec 2020 11:01

Tgt Ion	Ratio	Lower	Upper
216	100		
214	96.8	62.5	93.7
179	26.8	15.0	22.6
108	21.1	14.5	21.7

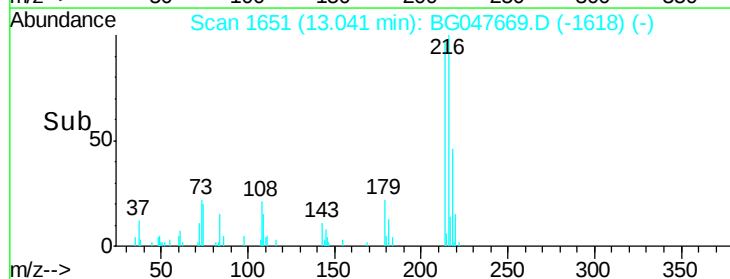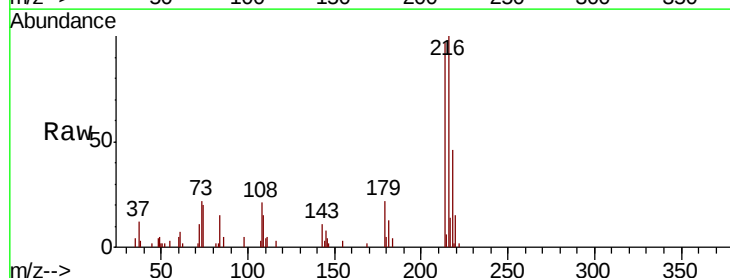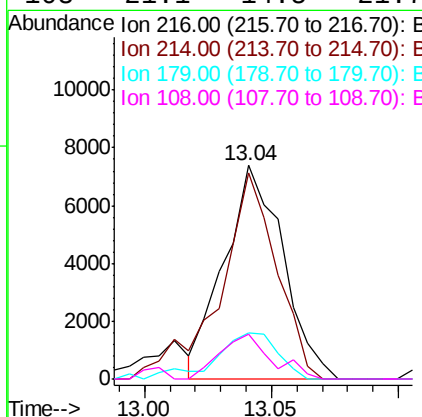

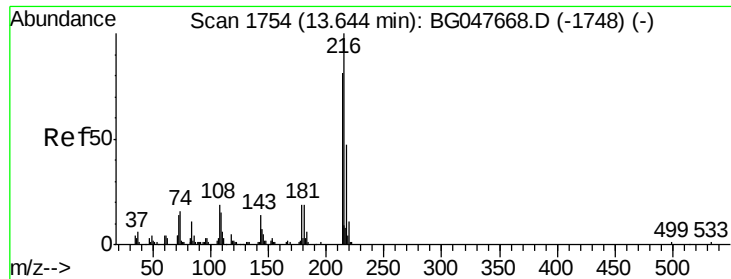

#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 10.427 ng/uL
 RT: 13.65 min Scan# 1754
 Delta R.T. 0.00 min
 Lab File: BG047669.D
 Acq: 9 Dec 2020 11:01

Instrument :
 BNA_G
 ClientSampleId :
 C0FW4DL

Tot Ion	Ion	Ratio	Resp	Lower	Upper
216	100				
214	80.5	61.7	92.5		
218	43.0	39.3	58.9		

Manual Integrations
 APPROVED

mohammad
 12/9/2020 5:40:05 PM

