

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047677.D
 Acq On : 9 Dec 2020 17:17
 Operator : CG/JU
 Sample : L4941-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.776	72	74	76	rVB2	4162	2519	0.42%	0.048%
2	4.175	140	142	145	rBV	1691	1770	0.30%	0.034%
3	4.351	171	172	174	rBV	2601	1542	0.26%	0.030%
4	4.387	177	178	181	rBV	2064	1841	0.31%	0.035%
5	4.534	201	203	204	rBV	4611	2849	0.48%	0.055%
6	4.816	249	251	254	rBV	1707	1721	0.29%	0.033%
7	5.203	314	317	320	rBV	2108	2681	0.45%	0.052%
8	5.274	326	329	331	rVB	2394	2598	0.43%	0.050%
9	5.421	352	354	357	rVB	2555	1606	0.27%	0.031%
10	5.579	378	381	382	rBV	1405	1512	0.25%	0.029%
11	5.644	390	392	394	rBV	2265	1563	0.26%	0.030%
12	6.008	451	454	457	rBV	1424	2084	0.35%	0.040%
13	6.055	459	462	464	rBV	1210	1532	0.26%	0.029%
14	6.261	494	497	499	rVB	2402	2373	0.40%	0.046%
15	6.337	508	510	514	rBV	1538	1793	0.30%	0.034%
16	6.384	517	518	523	rVB	1462	1827	0.31%	0.035%
17	6.431	523	526	527	rVB	2156	1670	0.28%	0.032%
18	6.484	531	535	536	rBV	1305	1606	0.27%	0.031%
19	6.948	612	614	617	rVB	2366	2063	0.34%	0.040%
20	7.066	632	634	637	rVB	1987	1523	0.25%	0.029%
21	7.095	637	639	642	rBV	1408	1763	0.29%	0.034%
22	7.236	660	663	665	rBV	1603	1805	0.30%	0.035%
23	7.354	677	683	695	rVB3	66191	137996	23.07%	2.654%
24	7.442	695	698	701	rBV3	1619	2419	0.40%	0.047%
25	7.524	706	712	720	rBV2	39307	68781	11.50%	1.323%
26	7.671	735	737	739	rBV2	1874	1538	0.26%	0.030%
27	7.742	743	749	756	rVV2	69279	121097	20.24%	2.329%
28	7.794	756	758	761	rVB	1839	2165	0.36%	0.042%
29	7.953	779	785	787	rBV	1124	1816	0.30%	0.035%
30	8.053	801	802	806	rVB	1748	1786	0.30%	0.034%
31	8.218	824	830	839	rVB	130930	224008	37.44%	4.309%
32	8.688	907	910	913	rVB	2026	1492	0.25%	0.029%
33	8.911	941	948	955	rBV3	70673	127230	21.27%	2.447%
34	9.046	967	971	977	rVB	3849	7602	1.27%	0.146%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047677.D
 Acq On : 9 Dec 2020 17:17
 Operator : CG/JU
 Sample : L4941-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

35	9.093	977	979	982	rVB	2313	1819	0.30%	0.035%
36	9.146	985	988	991	rVB	1826	1996	0.33%	0.038%
37	9.193	991	996	999	rBV	2342	3518	0.59%	0.068%
38	9.387	1022	1029	1035	rBV2	65326	120041	20.07%	2.309%
39	9.581	1060	1062	1066	rVB2	2332	2192	0.37%	0.042%
40	9.792	1091	1098	1100	rBV3	3891	6084	1.02%	0.117%
41	10.109	1143	1152	1161	rBV2	65927	124547	20.82%	2.396%
42	10.339	1187	1191	1193	rBV2	1709	1898	0.32%	0.037%
43	10.527	1220	1223	1226	rVB2	1260	1650	0.28%	0.032%
44	10.650	1238	1244	1253	rVB	90742	160436	26.82%	3.086%
45	11.044	1304	1311	1319	rBV	162429	287362	48.04%	5.528%
46	11.167	1325	1332	1340	rVB	68519	131605	22.00%	2.532%
47	11.943	1462	1464	1467	rVB	1190	1555	0.26%	0.030%
48	12.612	1575	1578	1580	rBV	1750	1768	0.30%	0.034%
49	12.800	1607	1610	1611	rVB	2121	1531	0.26%	0.029%
50	13.200	1675	1678	1679	rBV	1796	1478	0.25%	0.028%
51	13.288	1690	1693	1695	rVB	1678	1857	0.31%	0.036%
52	13.317	1695	1698	1699	rBV	1969	2068	0.35%	0.040%
53	13.570	1736	1741	1744	rVB	1377	2321	0.39%	0.045%
54	13.599	1744	1746	1748	rBV	1522	1542	0.26%	0.030%
55	14.058	1823	1824	1827	rVB	1757	1509	0.25%	0.029%
56	14.228	1847	1853	1857	rBV	172443	242681	40.57%	4.668%
57	14.269	1858	1860	1869	rVB2	17362	25146	4.20%	0.484%
58	14.534	1899	1905	1912	rBV	173355	266558	44.56%	5.127%
59	14.839	1950	1957	1963	rBV	272108	440279	73.60%	8.469%
60	15.004	1979	1985	1996	rBV2	67809	117581	19.65%	2.262%
61	15.297	2032	2035	2036	rBV2	1797	1565	0.26%	0.030%
62	15.344	2042	2043	2046	rBV2	2376	2212	0.37%	0.043%
63	15.433	2054	2058	2060	rBV2	1284	2055	0.34%	0.040%
64	15.820	2118	2124	2132	rVB	217748	336945	56.32%	6.481%
65	15.926	2137	2142	2148	rBV2	59355	95172	15.91%	1.831%
66	16.132	2173	2177	2179	rVB	1614	1535	0.26%	0.030%
67	16.355	2213	2215	2218	rBV	1876	2168	0.36%	0.042%
68	16.496	2235	2239	2243	rBV2	3629	6030	1.01%	0.116%
69	16.590	2254	2255	2257	rBV2	2926	1816	0.30%	0.035%
70	16.843	2296	2298	2300	rVB	2170	1659	0.28%	0.032%
71	17.013	2324	2327	2328	rBV	1508	1639	0.27%	0.032%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047677.D
 Acq On : 9 Dec 2020 17:17
 Operator : CG/JU
 Sample : L4941-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

72	17.119	2341	2345	2346	rBV	2152	2367	0.40%	0.046%
73	17.295	2373	2375	2381	rVB3	3470	4584	0.77%	0.088%
74	17.571	2416	2422	2433	rBV	382799	598233	100.00%	11.507%
75	17.671	2433	2439	2446	rBV	260329	380259	63.56%	7.315%
76	18.071	2506	2507	2508	rBV	2832	1583	0.26%	0.030%
77	18.353	2553	2555	2557	rBV2	2954	2461	0.41%	0.047%
78	19.939	2820	2825	2835	rBV	335042	501413	83.82%	9.645%
79	21.849	3145	3150	3157	rVB	329904	563804	94.24%	10.845%


Sum of corrected areas: 5198693

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
Data File : BG047677.D
Acq On : 9 Dec 2020 17:17
Operator : CG/JU
Sample : L4941-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AX8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

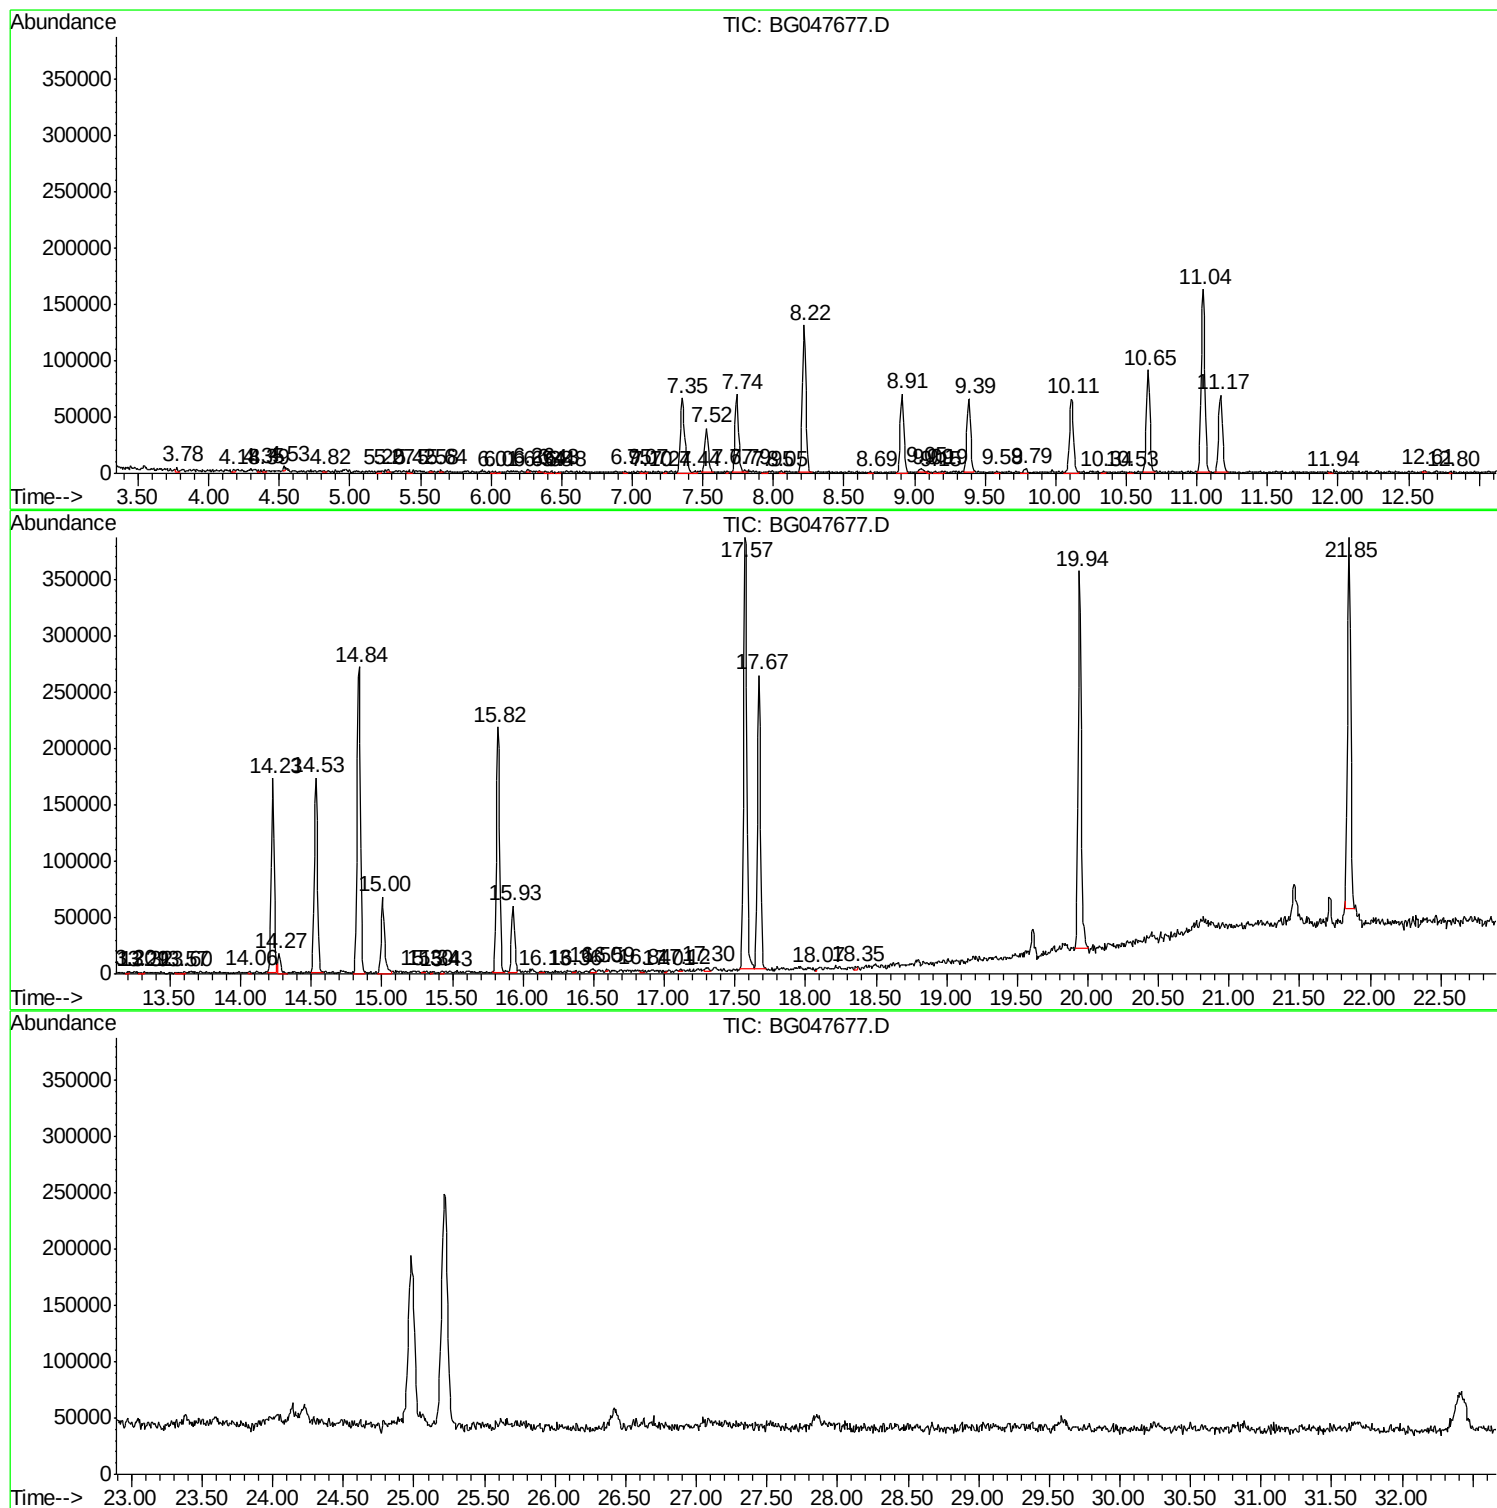

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120820\
Data File : BG047677.D
Acq On : 9 Dec 2020 17:17
Operator : CG/JU
Sample : L4941-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AX8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120820\
Data File : BG047677.D
Acq On : 9 Dec 2020 17:17
Operator : CG/JU
Sample : L4941-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AX8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc