

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047681.D
 Acq On : 9 Dec 2020 19:59
 Operator : CG/JU
 Sample : L4941-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.729	64	66	68	rBV2	2464	2925	0.46%	0.059%
2	3.929	97	100	101	rBV	2532	1965	0.31%	0.039%
3	4.082	122	126	130	rBV3	5612	8309	1.30%	0.167%
4	4.140	135	136	139	rBV	2068	1906	0.30%	0.038%
5	4.234	150	152	156	rBV	1317	1866	0.29%	0.037%
6	4.317	163	166	169	rBV3	2429	3662	0.57%	0.074%
7	4.575	207	210	211	rBV	2101	1740	0.27%	0.035%
8	4.622	216	218	219	rBV	2339	1721	0.27%	0.035%
9	4.798	244	248	249	rBV	2935	2980	0.47%	0.060%
10	4.963	272	276	281	rBV2	2510	4184	0.65%	0.084%
11	5.104	299	300	303	rBV	1609	1786	0.28%	0.036%
12	5.198	314	316	317	rBV	1638	1646	0.26%	0.033%
13	5.268	324	328	331	rBV	1909	3276	0.51%	0.066%
14	5.404	349	351	354	rBV	1490	2023	0.32%	0.041%
15	5.662	393	395	396	rBV	2251	1640	0.26%	0.033%
16	5.921	436	439	442	rVB	1714	1874	0.29%	0.038%
17	6.197	483	486	488	rBV	1862	2088	0.33%	0.042%
18	6.244	490	494	496	rVV	2291	2493	0.39%	0.050%
19	6.261	496	497	501	rVB	2604	2515	0.39%	0.050%
20	6.814	588	591	594	rBV	2272	2754	0.43%	0.055%
21	6.978	616	619	621	rBV	2233	2410	0.38%	0.048%
22	7.354	675	683	694	rVB3	58141	132094	20.65%	2.652%
23	7.530	707	713	721	rVB	30506	57526	8.99%	1.155%
24	7.742	743	749	755	rBV3	54068	97299	15.21%	1.954%
25	7.989	788	791	792	rBV3	1938	2028	0.32%	0.041%
26	8.042	796	800	803	rBV3	1476	2275	0.36%	0.046%
27	8.218	823	830	836	rVB2	134631	236274	36.93%	4.744%
28	8.664	900	906	907	rBV2	1904	2375	0.37%	0.048%
29	8.758	919	922	924	rBV2	1689	1731	0.27%	0.035%
30	8.911	940	948	954	rBV2	40436	72182	11.28%	1.449%
31	9.046	964	971	973	rBV2	5265	9269	1.45%	0.186%
32	9.099	979	980	986	rVB2	2580	2762	0.43%	0.055%
33	9.158	986	990	992	rBV2	1375	1796	0.28%	0.036%
34	9.381	1021	1028	1036	rBV2	55922	103732	16.21%	2.083%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047681.D
 Acq On : 9 Dec 2020 19:59
 Operator : CG/JU
 Sample : L4941-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

35	9.787	1093	1097	1102	rBV2	5880	7815	1.22%	0.157%
36	10.110	1145	1152	1160	rBV2	57964	103212	16.13%	2.072%
37	10.263	1177	1178	1184	rBV2	1487	2303	0.36%	0.046%
38	10.650	1237	1244	1252	rVB2	72780	129885	20.30%	2.608%
39	10.921	1286	1290	1293	rBV2	1532	2163	0.34%	0.043%
40	11.044	1304	1311	1321	rVB	169546	311073	48.62%	6.246%
41	11.167	1325	1332	1338	rBV3	49124	90473	14.14%	1.817%
42	11.367	1365	1366	1369	rBV3	2272	1683	0.26%	0.034%
43	12.225	1508	1512	1516	rBV3	1317	1857	0.29%	0.037%
44	12.266	1516	1519	1522	rVB3	1344	1962	0.31%	0.039%
45	12.654	1583	1585	1589	rVB3	1785	1733	0.27%	0.035%
46	12.807	1607	1611	1614	rBV3	1191	1917	0.30%	0.038%
47	12.906	1625	1628	1632	rBV3	1660	2224	0.35%	0.045%
48	13.165	1669	1672	1673	rBV3	1501	1711	0.27%	0.034%
49	13.271	1688	1690	1692	rBV	2388	2019	0.32%	0.041%
50	13.312	1695	1697	1700	rVB	1671	1729	0.27%	0.035%
51	13.335	1700	1701	1704	rBV	1614	1819	0.28%	0.037%
52	13.435	1716	1718	1723	rVB2	2347	3258	0.51%	0.065%
53	13.653	1751	1755	1756	rBV2	1695	2127	0.33%	0.043%
54	13.717	1762	1766	1769	rBV2	4254	5757	0.90%	0.116%
55	14.070	1822	1826	1828	rBV2	1831	3177	0.50%	0.064%
56	14.223	1846	1852	1857	rBV	136523	204755	32.00%	4.111%
57	14.270	1857	1860	1865	rVB2	18977	25615	4.00%	0.514%
58	14.352	1871	1874	1876	rBV2	1835	1829	0.29%	0.037%
59	14.534	1898	1905	1911	rBV	142849	224627	35.11%	4.510%
60	14.840	1949	1957	1965	rVB	286596	468584	73.24%	9.409%
61	15.004	1979	1985	1991	rBV3	58387	97898	15.30%	1.966%
62	15.086	1996	1999	2003	rBV	1634	2014	0.31%	0.040%
63	15.298	2034	2035	2038	rBV	1539	1688	0.26%	0.034%
64	15.445	2057	2060	2063	rBV	1170	1899	0.30%	0.038%
65	15.597	2082	2086	2089	rBV	3047	3843	0.60%	0.077%
66	15.821	2118	2124	2130	rBV2	188975	282402	44.14%	5.670%
67	15.926	2138	2142	2149	rVV2	50426	79322	12.40%	1.593%
68	16.003	2153	2155	2156	rVB	2982	1666	0.26%	0.033%
69	16.050	2161	2163	2164	rBV	3344	2386	0.37%	0.048%
70	16.120	2173	2175	2177	rVB	2541	2208	0.35%	0.044%
71	16.414	2222	2225	2227	rVB	1662	1970	0.31%	0.040%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047681.D
 Acq On : 9 Dec 2020 19:59
 Operator : CG/JU
 Sample : L4941-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

72	16.449	2227	2231	2232	rBV	2140	1857	0.29%	0.037%
73	16.485	2235	2237	2241	rVV	2814	2776	0.43%	0.056%
74	17.002	2322	2325	2326	rBV	1617	1778	0.28%	0.036%
75	17.096	2338	2341	2347	rBV3	10202	14564	2.28%	0.292%
76	17.295	2373	2375	2378	rBV2	2784	3211	0.50%	0.064%
77	17.572	2415	2422	2428	rBV	426545	639776	100.00%	12.846%
78	17.672	2433	2439	2445	rVV	215473	313088	48.94%	6.286%
79	17.818	2460	2464	2466	rBV2	2153	2570	0.40%	0.052%
80	17.959	2487	2488	2489	rBV2	4121	2330	0.36%	0.047%
81	18.083	2506	2509	2512	rBV	3671	3833	0.60%	0.077%
82	18.612	2597	2599	2600	rBV2	3221	2684	0.42%	0.054%
83	19.605	2765	2768	2774	rVB	34287	44929	7.02%	0.902%
84	19.939	2820	2825	2835	rBV2	284398	456296	71.32%	9.162%
85	21.849	3145	3150	3157	rVB2	371427	631015	98.63%	12.670%


Sum of corrected areas: 4980416

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
Data File : BG047681.D
Acq On : 9 Dec 2020 19:59
Operator : CG/JU
Sample : L4941-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AW6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

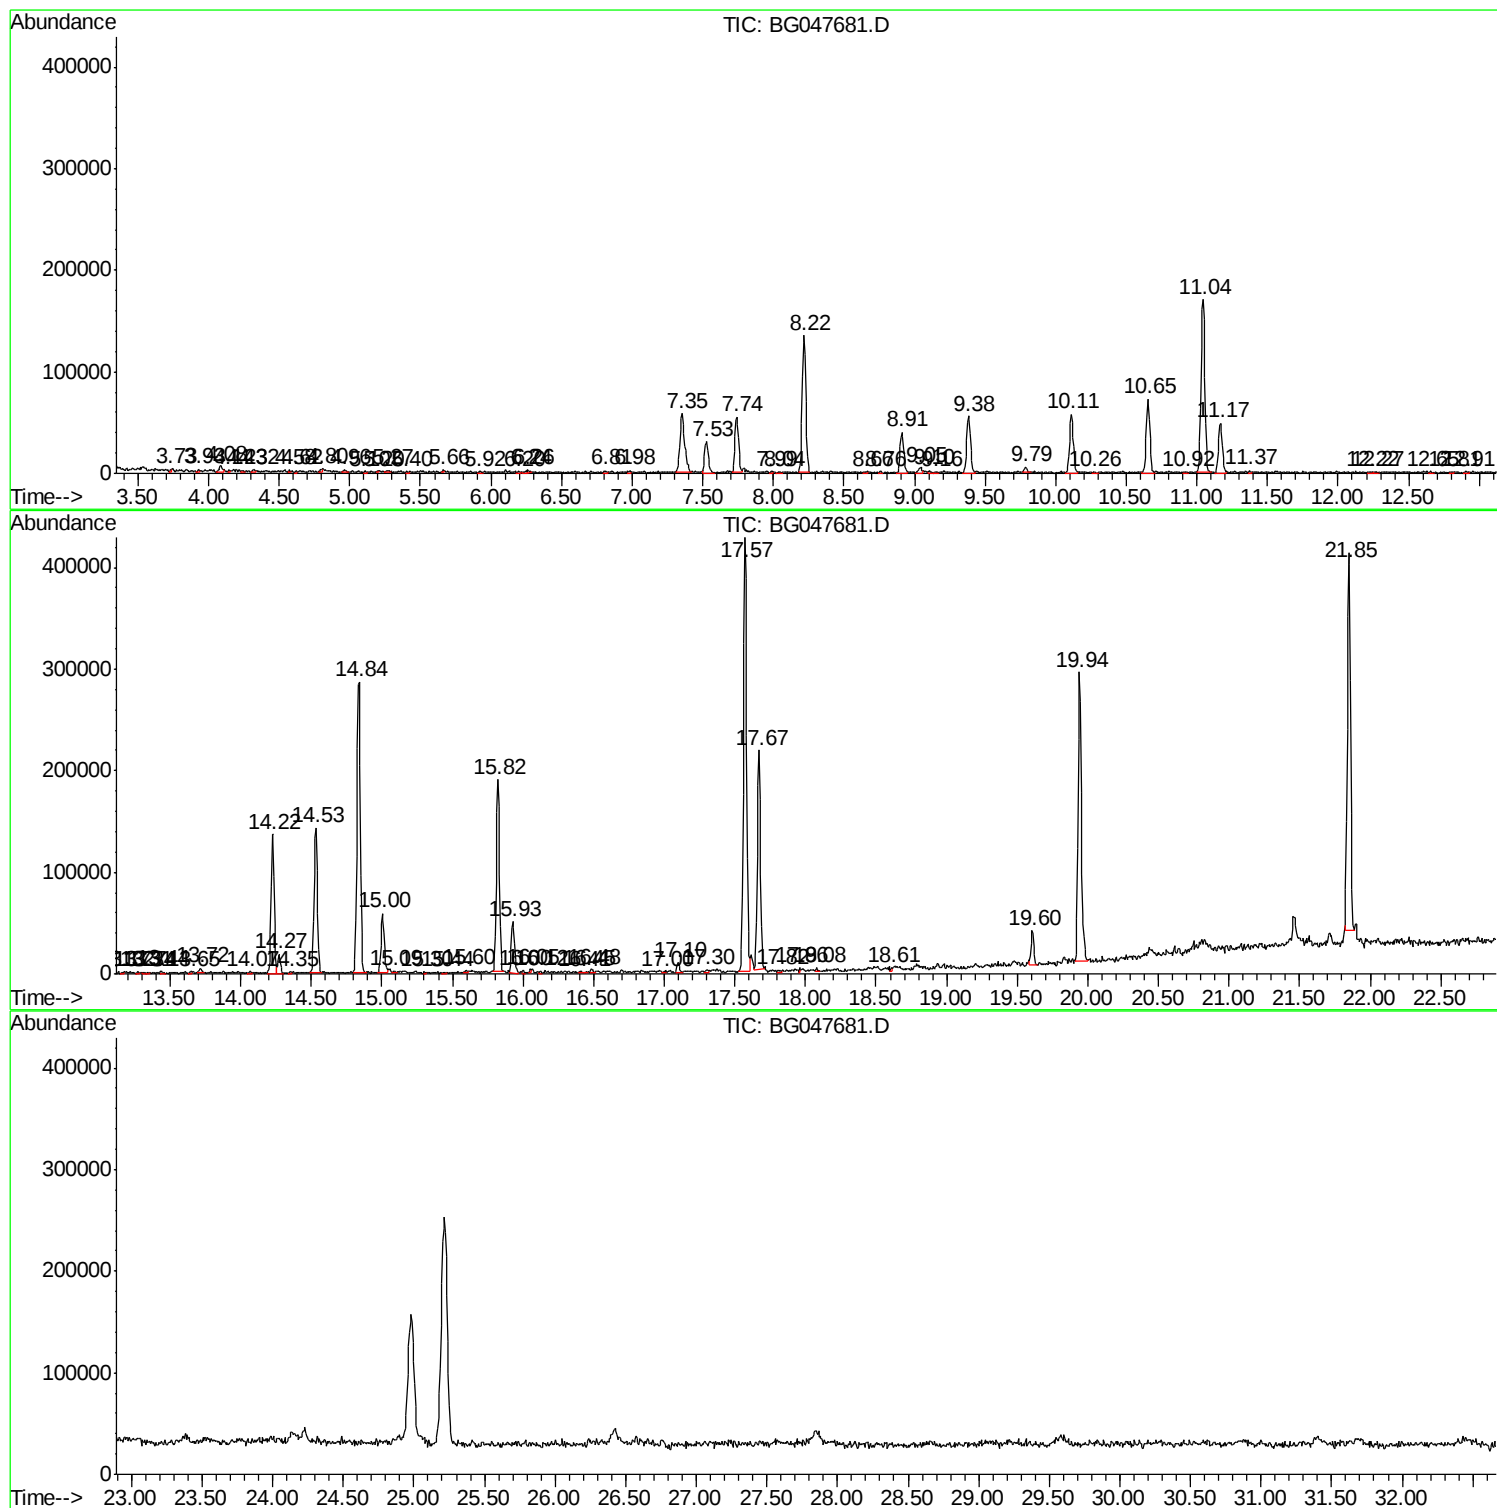

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120820\
Data File : BG047681.D
Acq On : 9 Dec 2020 19:59
Operator : CG/JU
Sample : L4941-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AW6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120820\
Data File : BG047681.D
Acq On : 9 Dec 2020 19:59
Operator : CG/JU
Sample : L4941-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AW6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc