

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047687.D
 Acq On : 10 Dec 2020 00:43
 Operator : CG/JU
 Sample : L4941-19
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.719	64	65	68	rVB	2517	1974	0.28%	0.064%
2	3.831	81	84	86	rBV2	2158	2377	0.34%	0.077%
3	4.882	260	263	266	rVB	1743	2442	0.35%	0.079%
4	4.965	275	277	280	rVB	1960	1750	0.25%	0.057%
5	6.187	483	485	489	rBV	1221	1717	0.25%	0.055%
6	6.281	498	501	504	rBV	1940	2052	0.29%	0.066%
7	6.616	557	558	563	rVB	1532	1725	0.25%	0.056%
8	6.892	601	605	606	rBV	1494	1833	0.26%	0.059%
9	7.356	678	684	691	rBV5	12143	24326	3.48%	0.786%
10	7.526	706	713	717	rBV2	9333	16192	2.32%	0.523%
11	7.656	731	735	737	rBV2	2061	2185	0.31%	0.071%
12	7.738	743	749	757	rBV4	13252	25472	3.64%	0.823%
13	8.085	804	808	813	rVB4	2163	3613	0.52%	0.117%
14	8.214	824	830	839	rVB	138349	230481	32.97%	7.450%
15	8.907	943	948	955	rBV4	15249	27597	3.95%	0.892%
16	9.383	1022	1029	1034	rBV4	14140	24856	3.56%	0.803%
17	9.506	1049	1050	1055	rBV4	1788	1952	0.28%	0.063%
18	10.106	1146	1152	1158	rBV4	11942	23146	3.31%	0.748%
19	10.646	1240	1244	1250	rBV4	19408	33958	4.86%	1.098%
20	10.817	1269	1273	1277	rBV4	1537	2336	0.33%	0.076%
21	11.040	1304	1311	1321	rBV	165172	305496	43.71%	9.875%
22	11.163	1326	1332	1342	rVB2	15066	28633	4.10%	0.926%
23	11.645	1411	1414	1417	rBV2	1160	1698	0.24%	0.055%
24	12.180	1501	1505	1506	rBV2	1782	2306	0.33%	0.075%
25	13.537	1734	1736	1741	rBV2	1251	1723	0.25%	0.056%
26	13.713	1762	1766	1768	rBV2	1581	2160	0.31%	0.070%
27	14.007	1813	1816	1819	rBV2	1824	2229	0.32%	0.072%
28	14.130	1835	1837	1841	rVB2	1952	1964	0.28%	0.063%
29	14.224	1848	1853	1858	rBV3	36058	55580	7.95%	1.797%
30	14.277	1858	1862	1866	rVB3	8354	12553	1.80%	0.406%
31	14.530	1900	1905	1912	rVB	36311	58514	8.37%	1.891%
32	14.835	1949	1957	1965	rBV2	300914	477101	68.26%	15.422%
33	14.924	1970	1972	1974	rBV	2309	1906	0.27%	0.062%
34	15.012	1983	1987	1992	rVB4	5498	9166	1.31%	0.296%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047687.D
 Acq On : 10 Dec 2020 00:43
 Operator : CG/JU
 Sample : L4941-19
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

35	15.447	2057	2061	2064	rVB4	1605	2143	0.31%	0.069%
36	15.676	2094	2100	2105	rVB4	1515	3252	0.47%	0.105%
37	15.752	2110	2113	2118	rBV4	879	2026	0.29%	0.065%
38	15.823	2119	2125	2132	rVB2	49132	78840	11.28%	2.548%
39	15.934	2141	2144	2148	rBV	3716	4746	0.68%	0.153%
40	16.475	2234	2236	2239	rBV	2150	2265	0.32%	0.073%
41	16.780	2286	2288	2292	rVB	2098	2175	0.31%	0.070%
42	17.350	2383	2385	2387	rBV	1658	1906	0.27%	0.062%
43	17.450	2400	2402	2404	rBV	2044	2150	0.31%	0.069%
44	17.526	2411	2415	2416	rBV	1569	1690	0.24%	0.055%
45	17.573	2417	2423	2434	rVV	439585	669333	95.76%	21.635%
46	17.667	2434	2439	2446	rVV	59958	91940	13.15%	2.972%
47	17.861	2469	2472	2475	rBV	1982	2318	0.33%	0.075%
48	17.967	2488	2490	2491	rBV	2148	1834	0.26%	0.059%
49	18.467	2573	2575	2576	rBV	3064	2110	0.30%	0.068%
50	18.502	2579	2581	2585	rBV	2360	2912	0.42%	0.094%
51	18.572	2590	2593	2595	rBV	4055	3236	0.46%	0.105%
52	19.677	2779	2781	2782	rBV2	4928	3439	0.49%	0.111%
53	19.941	2821	2826	2830	rBV	85855	123448	17.66%	3.990%
54	21.851	3144	3151	3157	rBV	415360	698962	100.00%	22.593%


Sum of corrected areas: 3093738

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
Data File : BG047687.D
Acq On : 10 Dec 2020 00:43
Operator : CG/JU
Sample : L4941-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B52

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

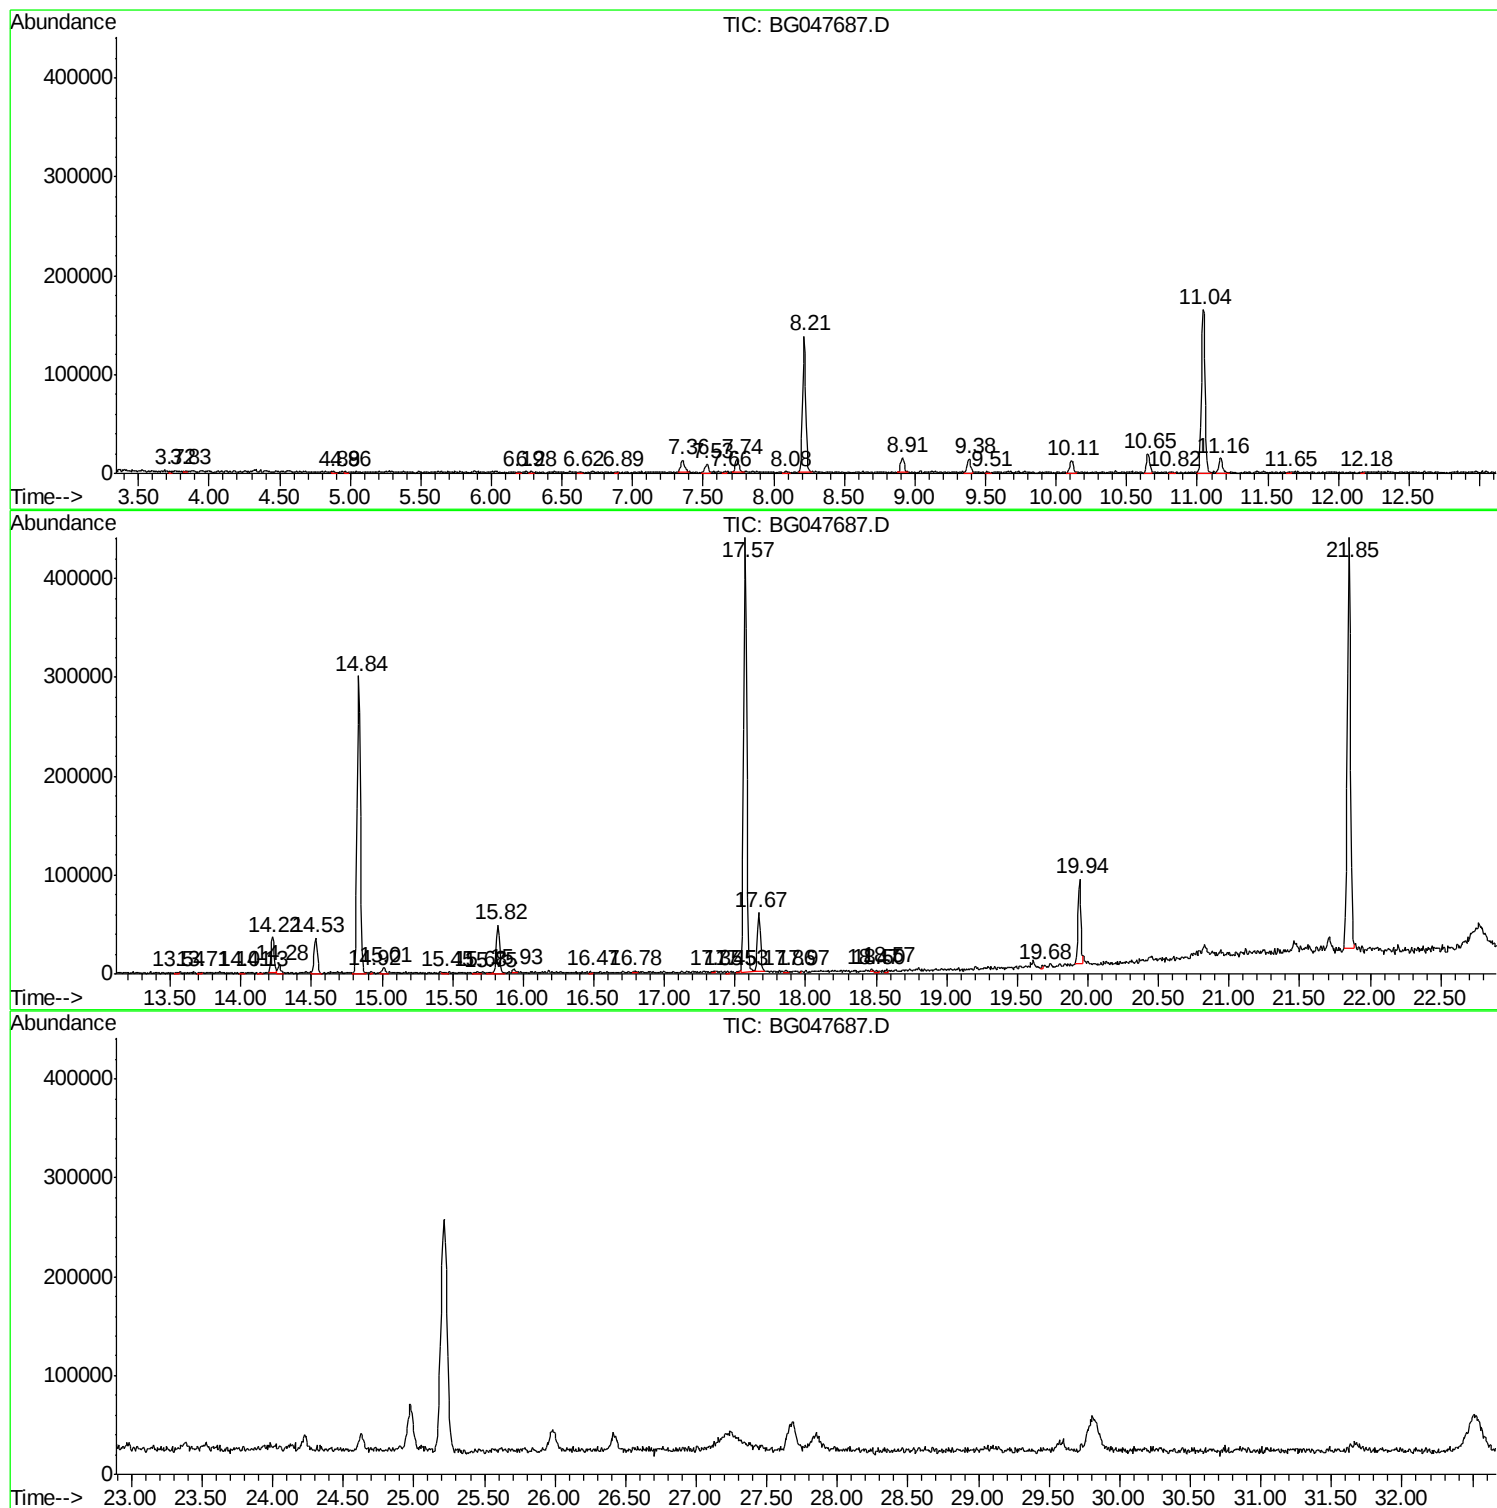

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120820\
Data File : BG047687.D
Acq On : 10 Dec 2020 00:43
Operator : CG/JU
Sample : L4941-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B52

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120820\
Data File : BG047687.D
Acq On : 10 Dec 2020 00:43
Operator : CG/JU
Sample : L4941-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B52

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc