

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047690.D
 Acq On : 10 Dec 2020 2:45
 Operator : CG/JU
 Sample : L4941-11
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	10	11	14	rBV2	3981	3325	0.53%	0.068%
2	4.139	134	136	139	rBV3	2281	1675	0.27%	0.035%
3	4.474	190	193	196	rVB2	2485	2544	0.41%	0.052%
4	4.968	275	277	280	rVB	1970	1765	0.28%	0.036%
5	5.214	317	319	324	rVB	1925	2260	0.36%	0.047%
6	6.190	481	485	488	rBV	2043	2355	0.38%	0.049%
7	6.813	589	591	596	rBV	1509	2484	0.40%	0.051%
8	6.848	596	597	601	rVB	1962	2109	0.34%	0.043%
9	7.059	628	633	636	rVB	1532	2223	0.36%	0.046%
10	7.130	642	645	648	rBV	1708	2245	0.36%	0.046%
11	7.206	656	658	662	rBV	1203	1632	0.26%	0.034%
12	7.353	677	683	696	rVB5	50182	104276	16.77%	2.148%
13	7.529	706	713	721	rVB	28867	53074	8.53%	1.093%
14	7.741	743	749	755	rVB2	48395	84525	13.59%	1.741%
15	8.217	823	830	837	rVB	109455	196392	31.58%	4.046%
16	8.775	921	925	927	rVB	1662	1782	0.29%	0.037%
17	8.910	942	948	954	rBV2	46678	79706	12.82%	1.642%
18	9.039	966	970	976	rVB3	6284	11291	1.82%	0.233%
19	9.380	1022	1028	1036	rVB	49286	90248	14.51%	1.859%
20	9.791	1092	1098	1101	rBV	3171	4687	0.75%	0.097%
21	10.109	1146	1152	1159	rBV3	51746	87795	14.12%	1.809%
22	10.291	1180	1183	1186	rBV3	1677	2180	0.35%	0.045%
23	10.350	1190	1193	1196	rBV3	1440	1661	0.27%	0.034%
24	10.655	1237	1245	1251	rBV2	67479	124456	20.01%	2.564%
25	10.843	1275	1277	1282	rVB2	1466	1748	0.28%	0.036%
26	11.043	1302	1311	1318	rBV	148620	270465	43.49%	5.572%
27	11.166	1326	1332	1342	rVB3	51353	96828	15.57%	1.995%
28	11.601	1404	1406	1412	rVB	1986	2945	0.47%	0.061%
29	11.672	1414	1418	1419	rBV	2674	2234	0.36%	0.046%
30	11.895	1453	1456	1460	rBV	1166	1669	0.27%	0.034%
31	12.471	1549	1554	1555	rBV	1324	1874	0.30%	0.039%
32	12.653	1581	1585	1588	rBV	1198	1718	0.28%	0.035%
33	13.117	1660	1664	1666	rBV	1661	2117	0.34%	0.044%
34	13.875	1789	1793	1797	rBV	1335	2160	0.35%	0.044%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
 Data File : BG047690.D
 Acq On : 10 Dec 2020 2:45
 Operator : CG/JU
 Sample : L4941-11
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

35	14.227	1847	1853	1857	rBV	137754	194739	31.32%	4.012%
36	14.274	1857	1861	1865	rVB	23652	34238	5.51%	0.705%
37	14.380	1877	1879	1881	rBV	2192	1970	0.32%	0.041%
38	14.445	1888	1890	1893	rVB	1939	1680	0.27%	0.035%
39	14.527	1898	1904	1912	rVV	137708	217645	35.00%	4.484%
40	14.674	1926	1929	1931	rVB	1978	2081	0.33%	0.043%
41	14.833	1950	1956	1963	rVB	263661	425165	68.37%	8.759%
42	15.003	1980	1985	1995	rBV2	62603	107436	17.28%	2.213%
43	15.285	2030	2033	2035	rBV2	1810	1636	0.26%	0.034%
44	15.655	2093	2096	2097	rBV	2154	1861	0.30%	0.038%
45	15.714	2104	2106	2110	rVB	2521	2343	0.38%	0.048%
46	15.820	2117	2124	2133	rBV	194449	289091	46.49%	5.956%
47	15.925	2138	2142	2149	rVV2	56173	88913	14.30%	1.832%
48	15.990	2151	2153	2157	rVB2	2320	2704	0.43%	0.056%
49	16.061	2163	2165	2170	rBV	2511	2928	0.47%	0.060%
50	16.155	2178	2181	2182	rBV	1864	1824	0.29%	0.038%
51	16.290	2202	2204	2207	rVB	2060	1827	0.29%	0.038%
52	16.789	2287	2289	2294	rVB3	2701	2323	0.37%	0.048%
53	16.889	2303	2306	2308	rBV	2135	2420	0.39%	0.050%
54	17.153	2350	2351	2353	rBV	2690	1724	0.28%	0.036%
55	17.300	2374	2376	2380	rVB	2722	3133	0.50%	0.065%
56	17.571	2415	2422	2428	rBV	388502	621862	100.00%	12.811%
57	17.670	2433	2439	2446	rVB2	223134	342055	55.00%	7.047%
58	17.964	2487	2489	2492	rBV	3191	2943	0.47%	0.061%
59	18.440	2565	2570	2573	rBV4	4986	8373	1.35%	0.172%
60	19.604	2765	2768	2774	rVB	54933	73720	11.85%	1.519%
61	19.938	2819	2825	2835	rBV2	326908	549919	88.43%	11.329%
62	21.848	3145	3150	3156	rVB2	372741	617040	99.22%	12.712%


Sum of corrected areas: 4854041

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120820\
Data File : BG047690.D
Acq On : 10 Dec 2020 2:45
Operator : CG/JU
Sample : L4941-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

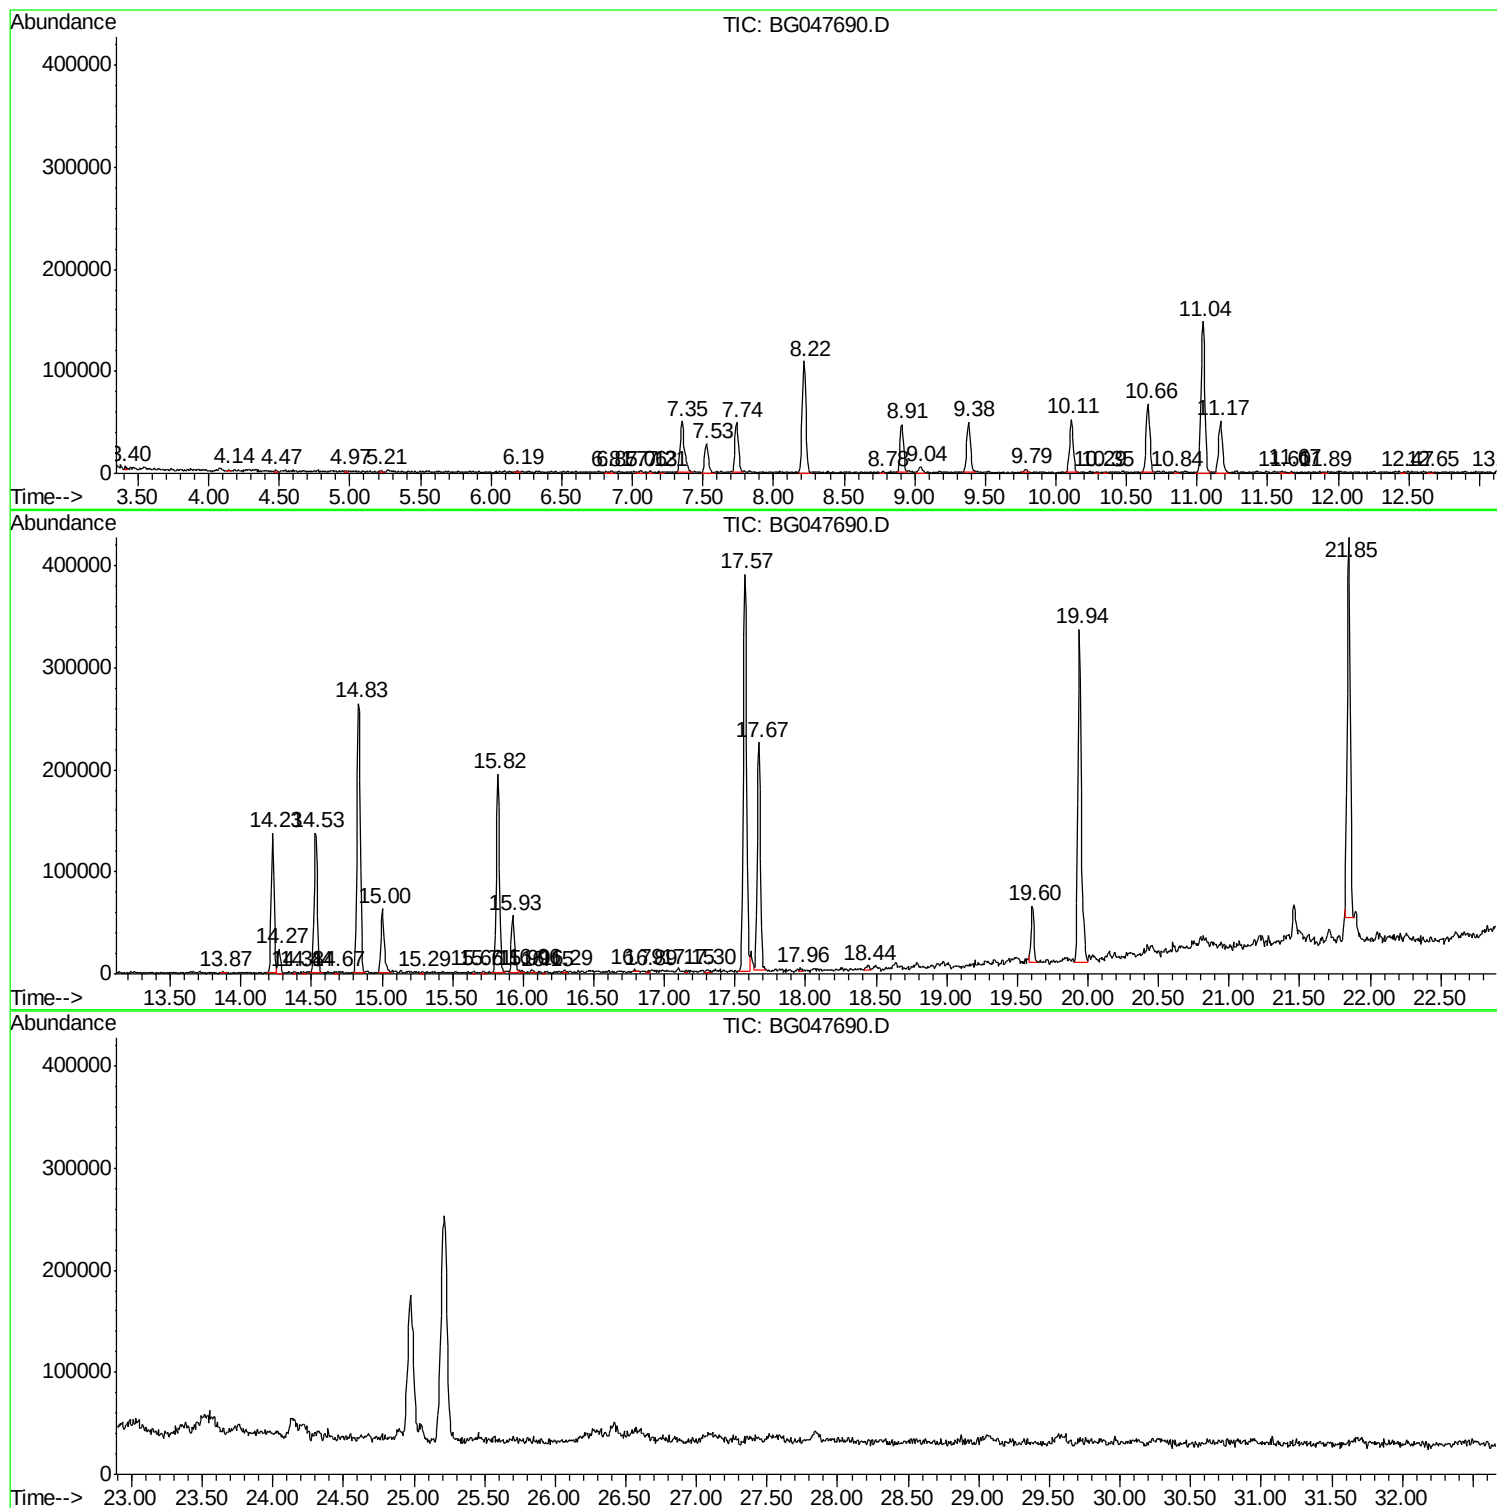

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120820\
Data File : BG047690.D
Acq On : 10 Dec 2020 2:45
Operator : CG/JU
Sample : L4941-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120820\
Data File : BG047690.D
Acq On : 10 Dec 2020 2:45
Operator : CG/JU
Sample : L4941-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc