


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120822\
Data File : BG055925.D
Acq On : 8 Dec 2022 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 09 07:57:14 2022

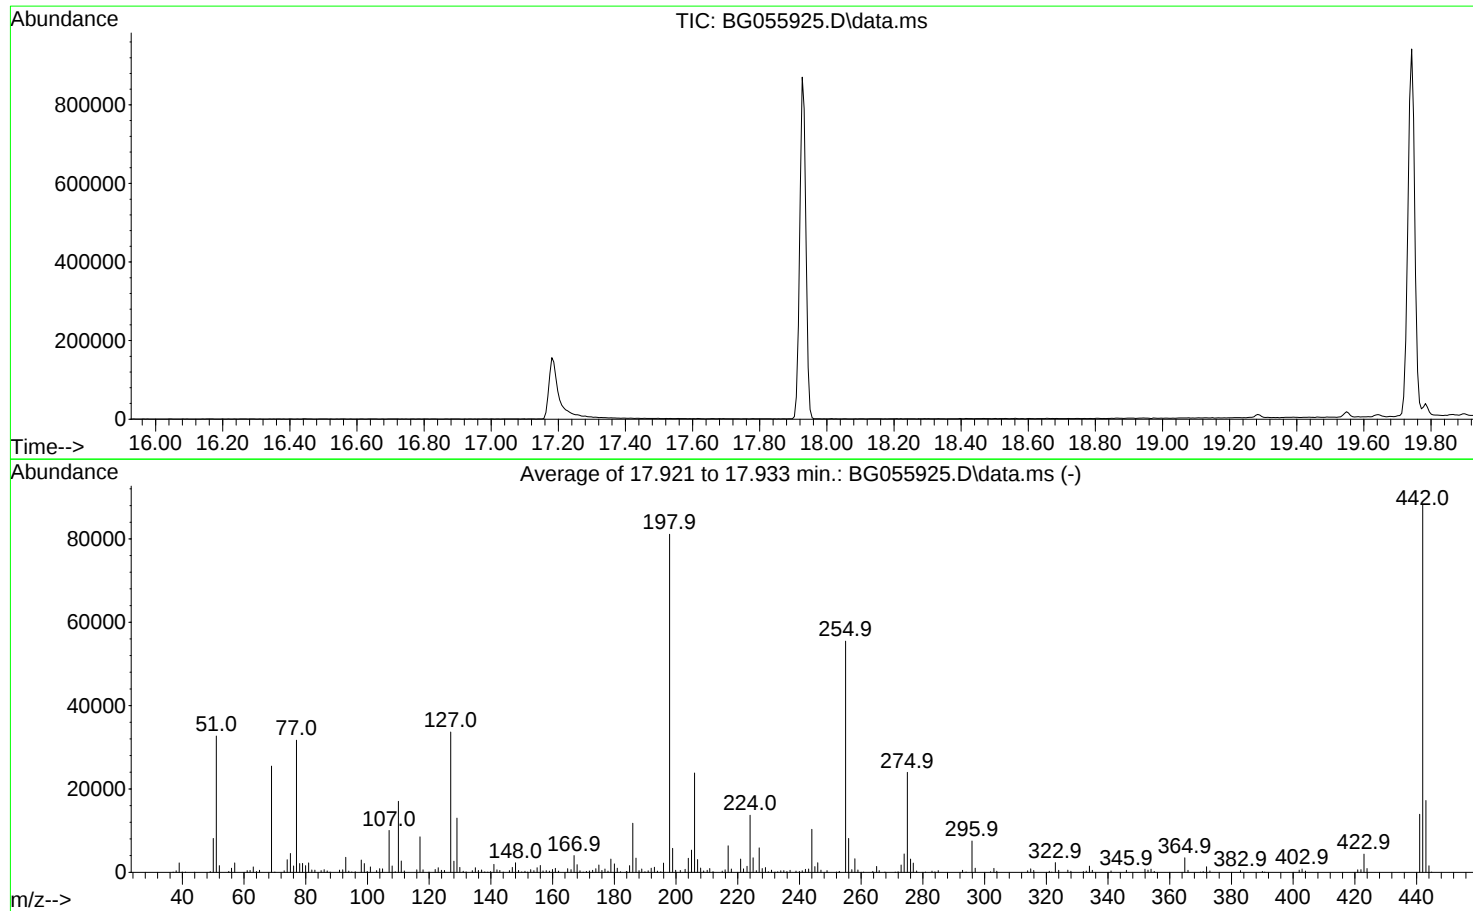




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	32707	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.4	25477	PASS
70	69	0.00	2	0.2	53	PASS
127	198	10	80	41.5	33659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81123	PASS
199	198	5	9	7.1	5729	PASS
275	198	10	60	29.6	23992	PASS
365	198	1	100	4.3	3467	PASS
441	198	0.01	100	17.2	13938	PASS
442	442	50	100	100.0	88272	PASS
443	442	15	24	19.5	17218	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120822\
 Data File : BG055925.D
 Acq On : 8 Dec 2022 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Dec 09 09:04:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 09 07:57:14 2022
 Response via : Initial Calibration

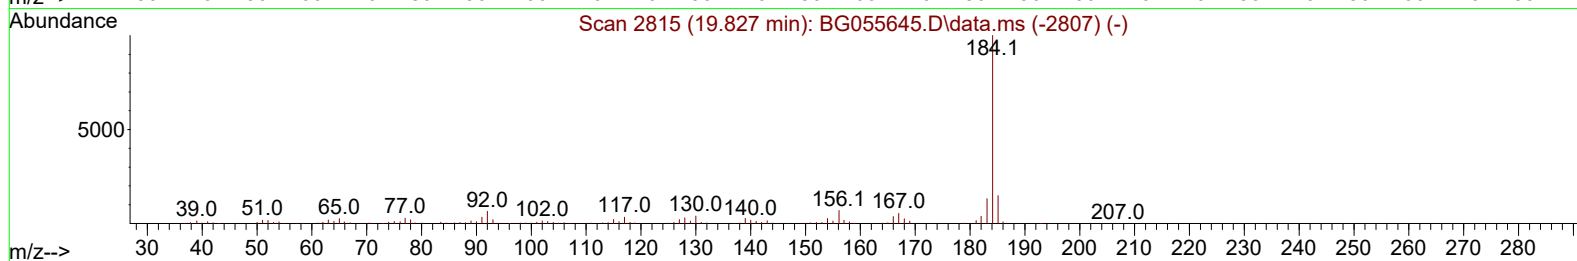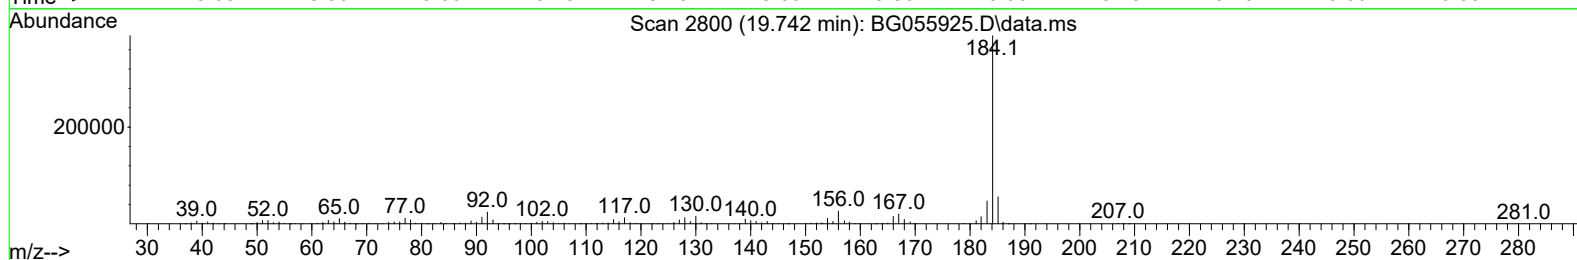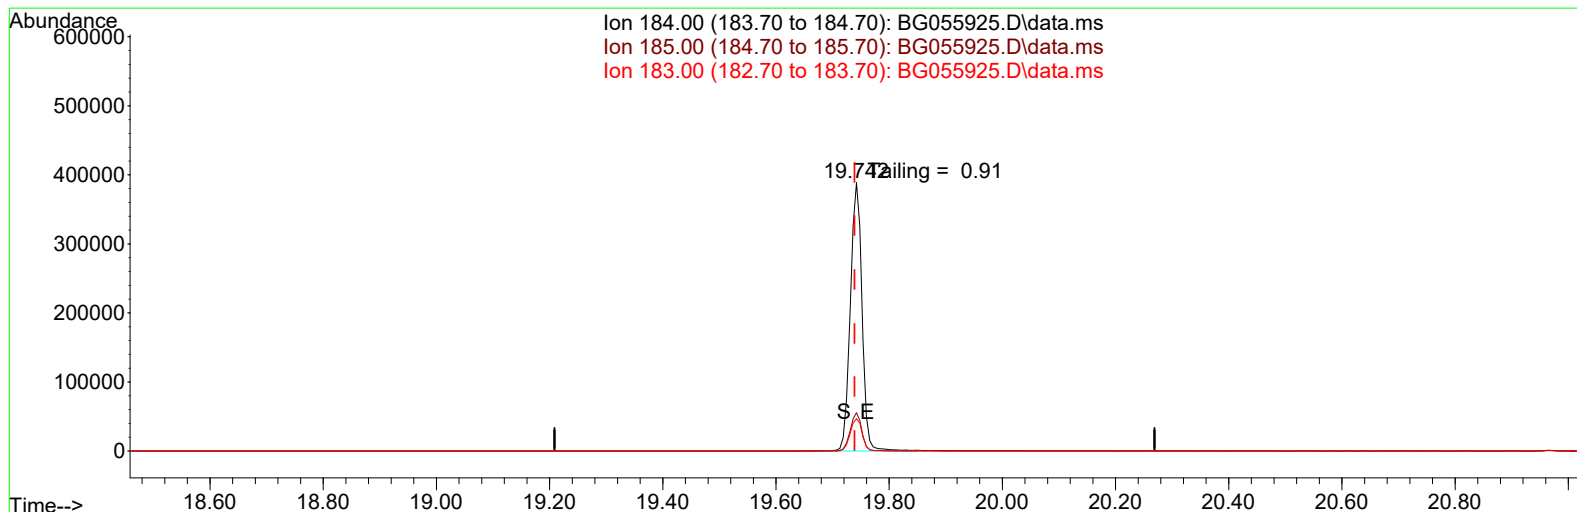

TIC: BG055925.D\data.ms

(77) Benzidine

19.742min (+ 0.004) 447302.51 ng




response 558798

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.29
183.00	13.20	12.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120822\
Data File : BG055925.D
Acq On : 8 Dec 2022 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 09 09:04:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 07:57:14 2022
Response via : Initial Calibration

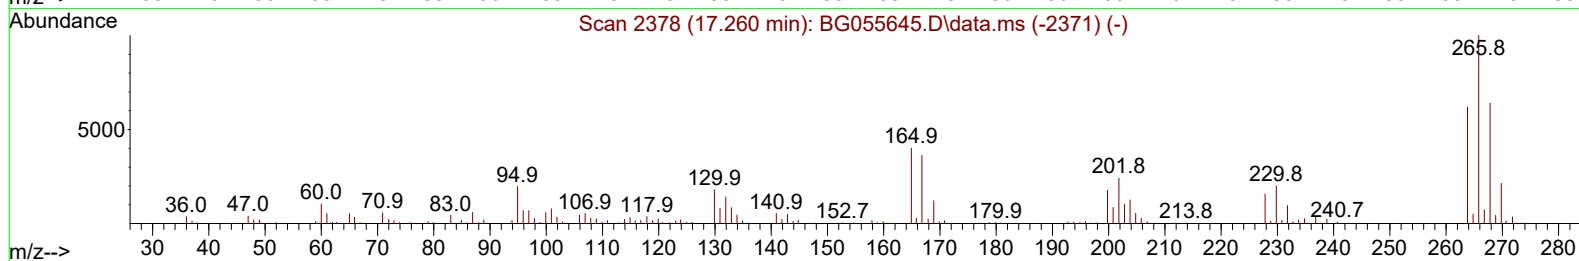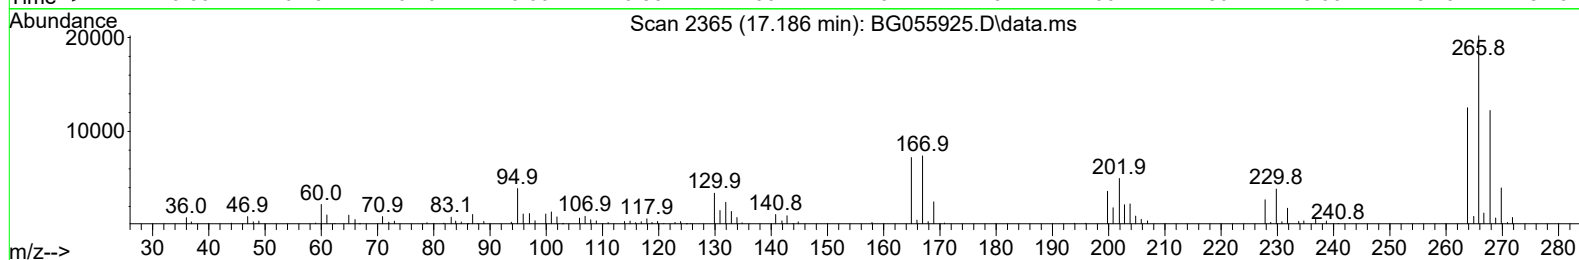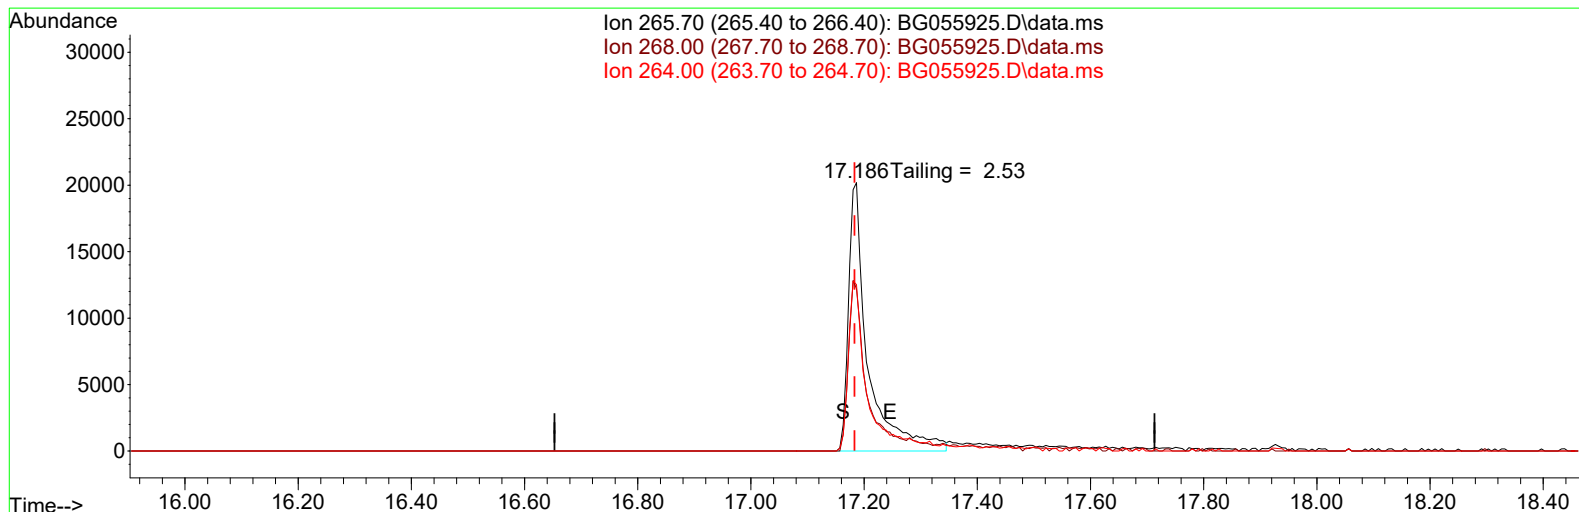

TIC: BG055925.D\data.ms

(70) Pentachlorophenol (C)

17.186min (+ 0.004) 12910.35 ng

response 46796

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	60.51
264.00	61.90	62.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/8/2022	BNA_G	<u>BG055925.D</u>
Compound Name	Response	Retention Time
DDT	251470	20.964
DDD	6157	20.571
DDE	597	20.024
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6754	258224	2.62

Instrument :
BNA_G
ClientSampleId :
DFTPP