


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120919\
 Data File : BG043787.D
 Acq On : 9 Dec 2019 12:13
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 09 18:16:57 2019

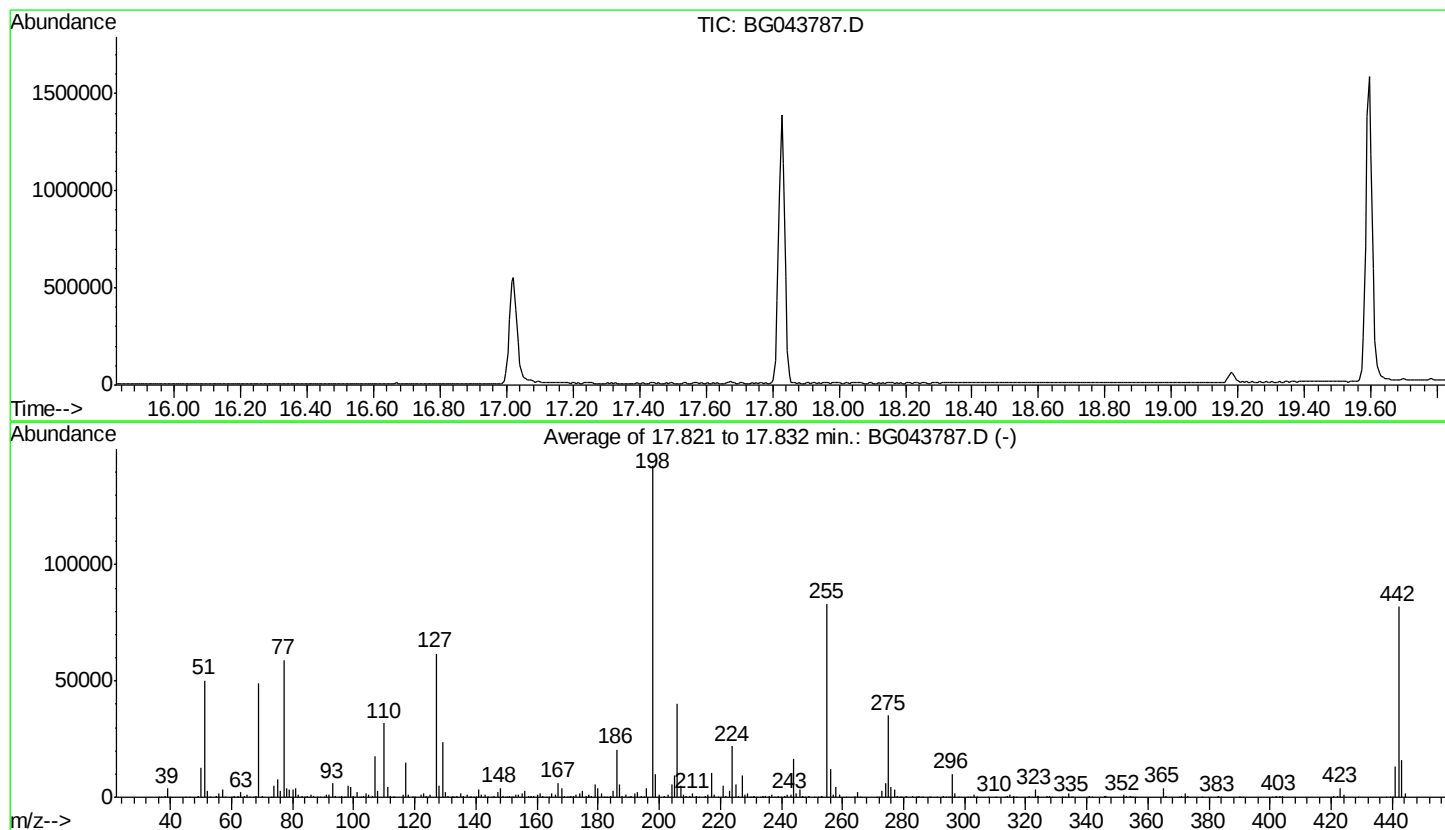

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	50245	PASS
68	69	0.00	2	0.7	347	PASS
69	198	0.00	100	34.4	49077	PASS
70	69	0.00	2	0.6	312	PASS
127	198	10	80	43.4	61890	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	142693	PASS
199	198	5	9	7.1	10087	PASS
275	198	10	60	24.7	35224	PASS
365	198	1	100	2.9	4143	PASS
441	198	0.01	100	9.3	13268	PASS
442	198	50	100	57.5	82068	PASS
443	442	15	24	19.3	15821	PASS