

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051446.D
 Acq On : 10 Dec 2021 00:52
 Operator : CG/JU
 Sample : M4938-07 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EX8E3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
 Supervised By :Yogesh Patel 12/15/2021

Quant Time: Dec 10 04:15:59 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 03:21:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.181	152	24753	20.000	ng/ul	0.00
20) Naphthalene-d8	11.013	136	109118	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.815	164	75198	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.570	188	167779	20.000	ng/ul	0.00
79) Chrysene-d12	21.871	240	153718	20.000	ng/ul	0.00
88) Perylene-d12	25.267	264	141911	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.534	96	1857	2.464	ng/uL	0.00
4) Pyridine-d5	3.986	84	12629	5.835	ng/ul	0.02
7) Phenol-d5	7.377	99	19105	7.582	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.500	67	50577	31.298	ng/ul	0.00
11) 2-Chlorophenol-d4	7.723	132	45060	25.134	ng/ul	0.00
15) 4-Methylphenol-d8	8.916	113	34128	17.240	ng/ul	0.00
21) Nitrobenzene-d5	9.368	128	31019	32.770	ng/ul	0.00
24) 2-Nitrophenol-d4	10.097	143	33336	31.123	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.655	165	52063	29.878	ng/ul	0.00
31) 4-Chloroaniline-d4	11.166	131	65611	25.743	ng/ul	0.00
46) Dimethylphthalate-d6	14.216	166	205435	35.306	ng/ul	0.00
49) Acenaphthylene-d8	14.515	160	252347	34.242	ng/ul	0.00
54) 4-Nitrophenol-d4	15.156	143	4857m	5.544	ng/ul	0.09
60) Fluorene-d10	15.808	176	182272	35.189	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.955	200	30532	30.624	ng/ul	0.00
73) Anthracene-d10	17.670	188	311990	39.742	ng/ul	0.00
81) Pyrene-d10	19.950	212	365797	39.591	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.032	264	309954	42.346	ng/ul	0.00
Target Compounds						
8) Phenol	7.400	94	2653	1.029	ng/ul	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051446.D
Acq On : 10 Dec 2021 00:52
Operator : CG/JU
Sample : M4938-07 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
EX8E3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
Supervised By :Yogesh Patel 12/15/2021


Quant Time: Dec 10 04:15:59 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 09 03:21:41 2021
Response via : Initial Calibration

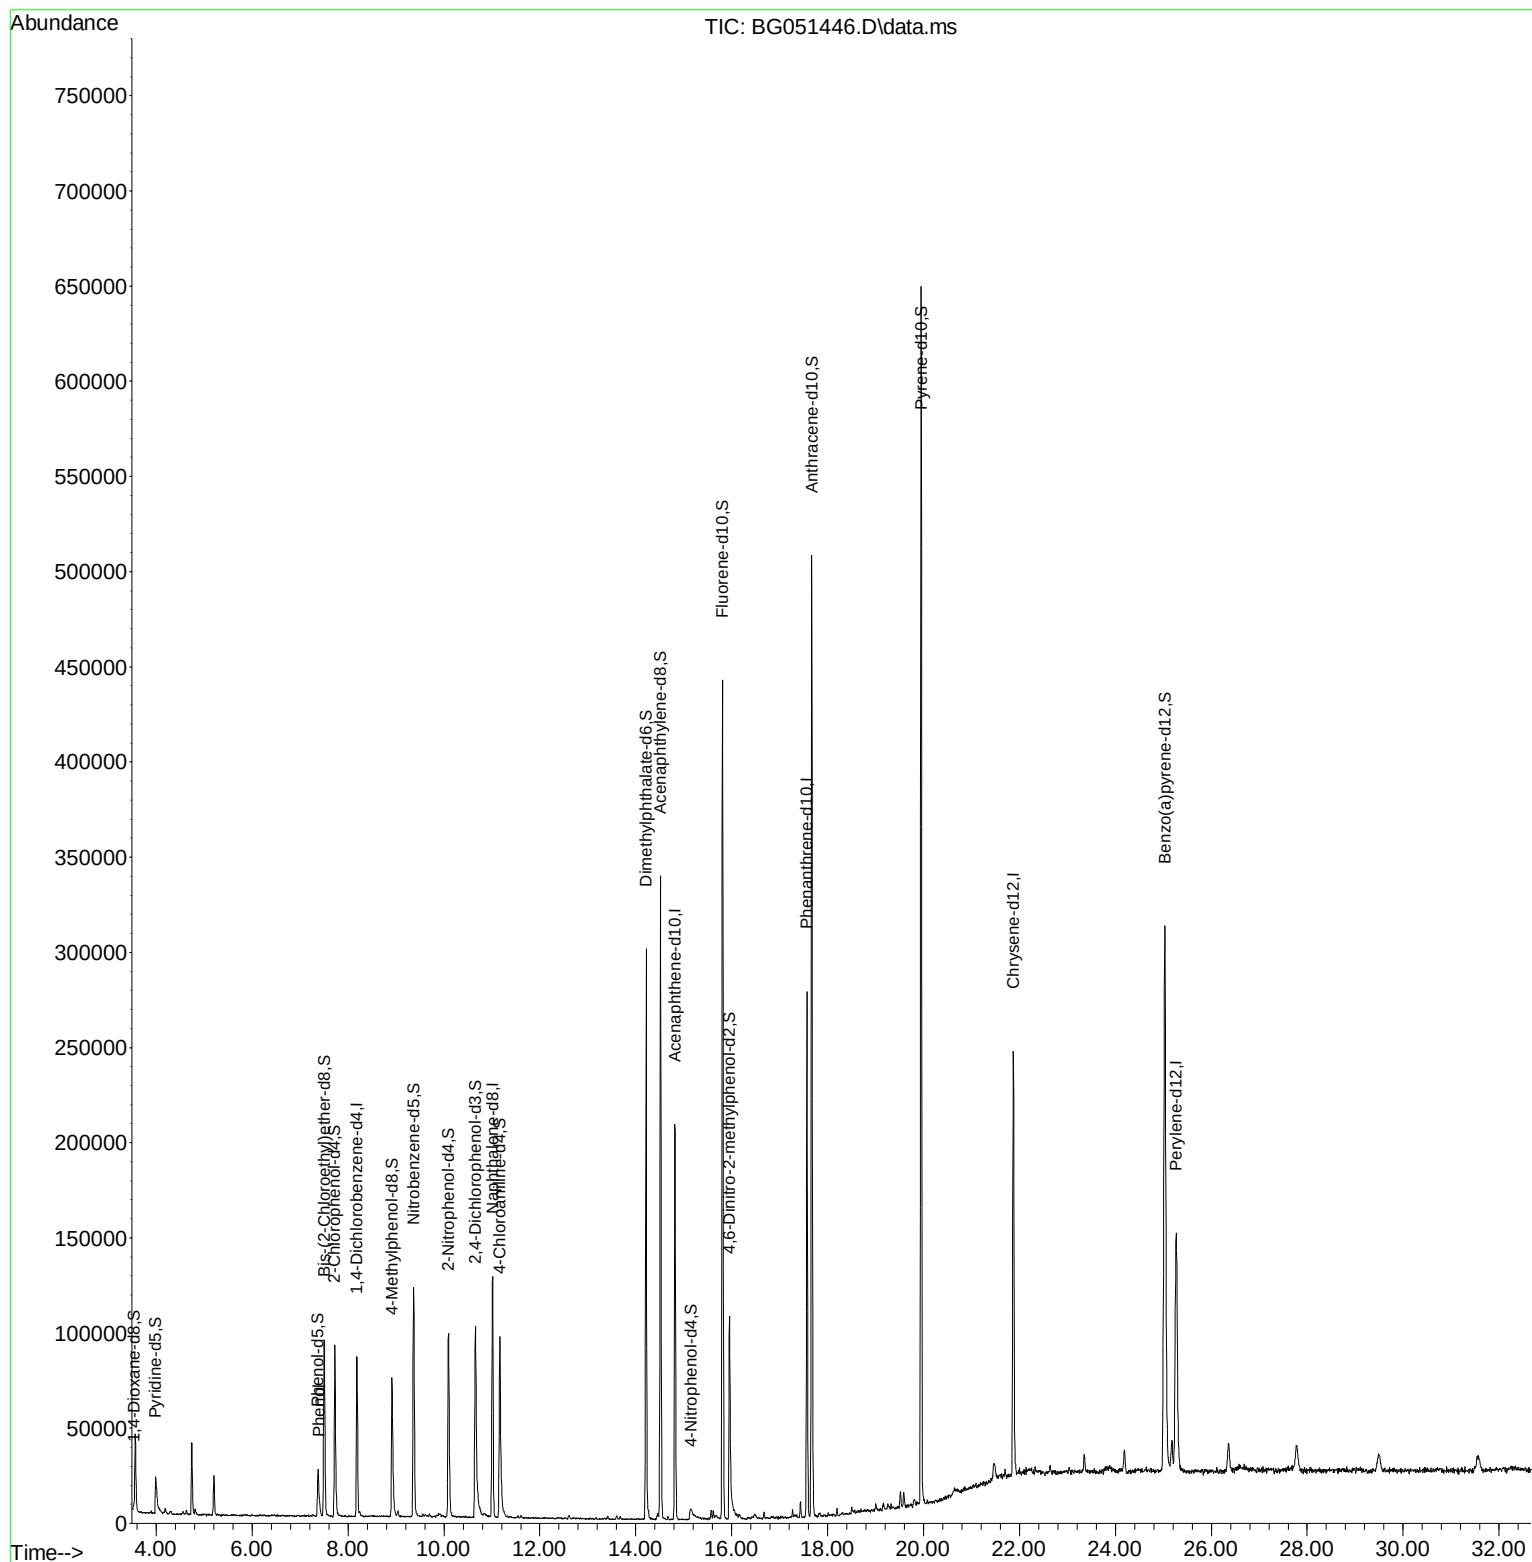

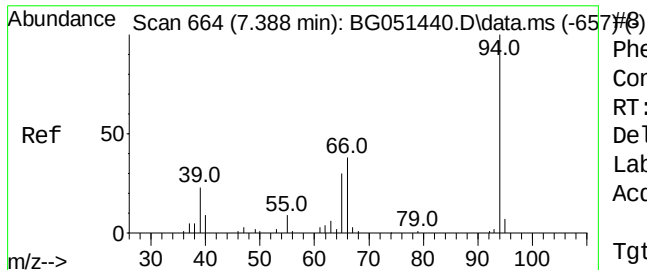

Phenol
 Concen: 1.029 ng/ul
 RT: 7.400 min Scan# 666
 Delta R.T. 0.016 min
 Lab File: BG051446.D
 Acq: 10 Dec 2021 00:52

Instrument :
 BNA_G
 ClientSampleId :
 EX8E3

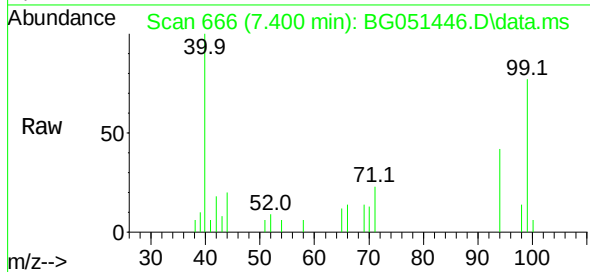

Tgt Ion: 94 Resp: 265

Ion	Ratio	Lower	Upper
94	100		
65	28.7	25.1	37.7
66	32.9	31.6	47.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/10/2021
 Supervised By :Yogesh Patel 12/15/2021

